

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
 Data File : PD062276.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 20:49
 Operator : AR\AJ
 Sample : M2106-12
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-25-9.5-10.0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 22:10:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.980	11463326	144.2E6	13.691	16.599
28)	SA Decachlor...	8.257	9.041	18850994	136.1E6	15.321	14.414
Target Compounds							
12)	B 4,4'-DDE	5.655	6.316	1166922	14912972	1.038	1.294



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
Data File : PD062276.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 20:49
Operator : AR\AJ
Sample : M2106-12
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SB-25-9.5-10.0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 22:10:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

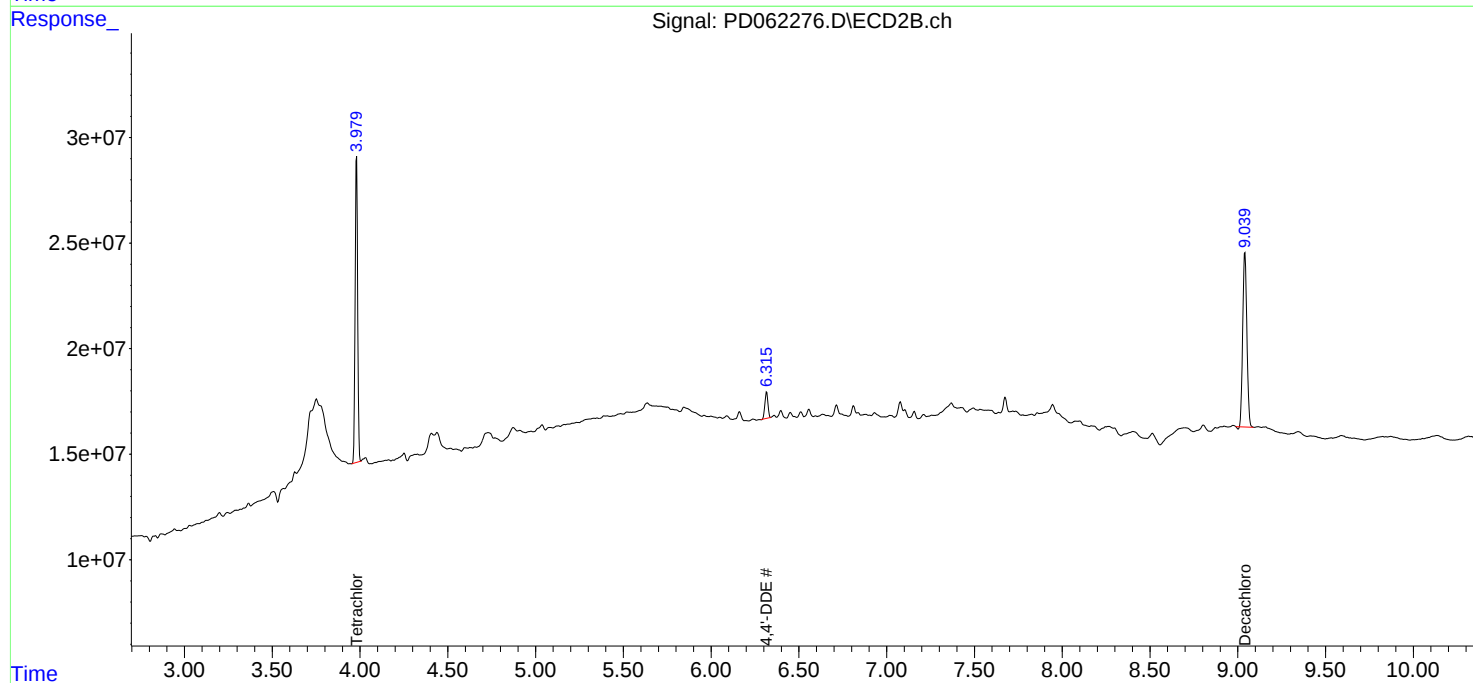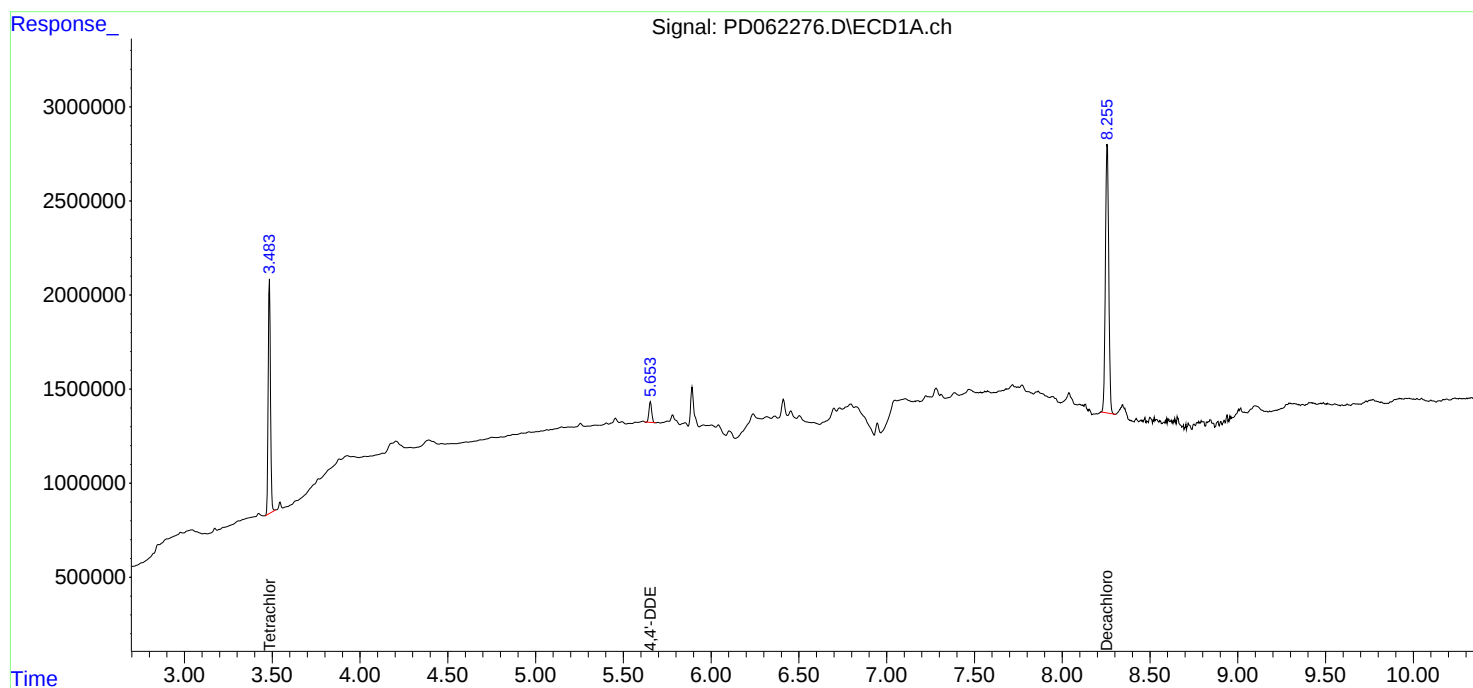


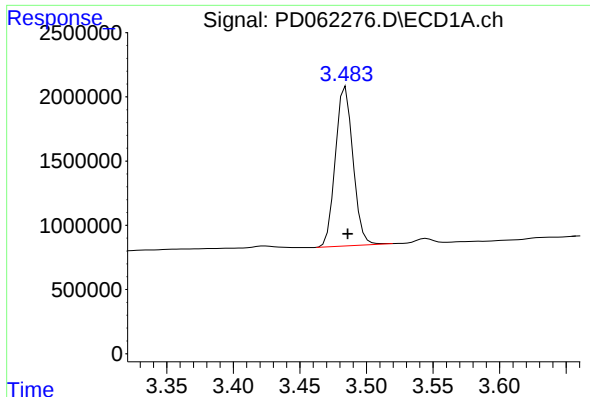

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 11463326
Conc: 13.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-25-9.5-10.0

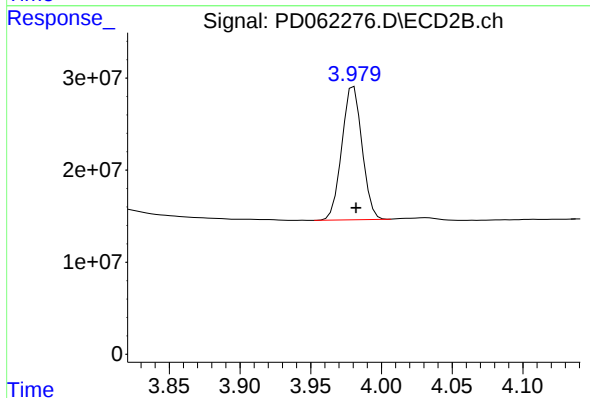


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 144223752
Conc: 16.60 ng/ml

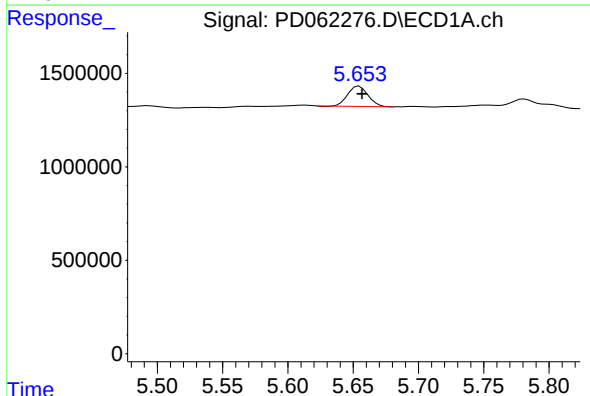


#12 4,4'-DDE

R.T.: 5.655 min
Delta R.T.: -0.002 min
Response: 1166922
Conc: 1.04 ng/ml

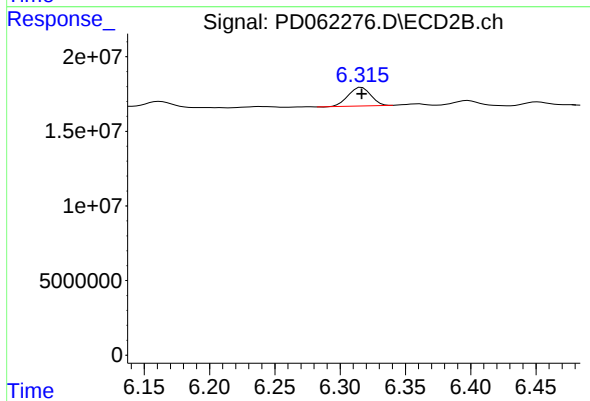

#12 4,4'-DDE


R.T.: 6.316 min
Delta R.T.: 0.000 min
Response: 14912972
Conc: 1.29 ng/ml

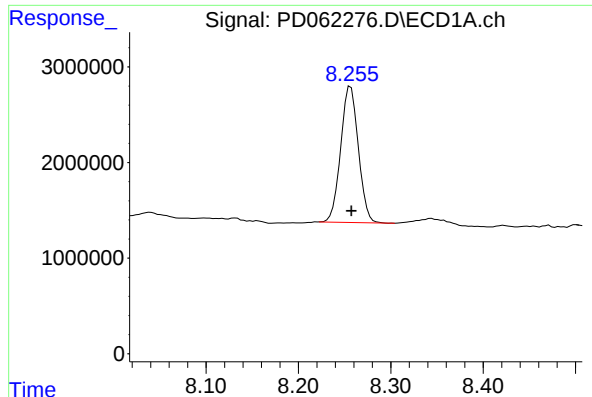

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 18850994
Conc: 15.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-25-9.5-10.0

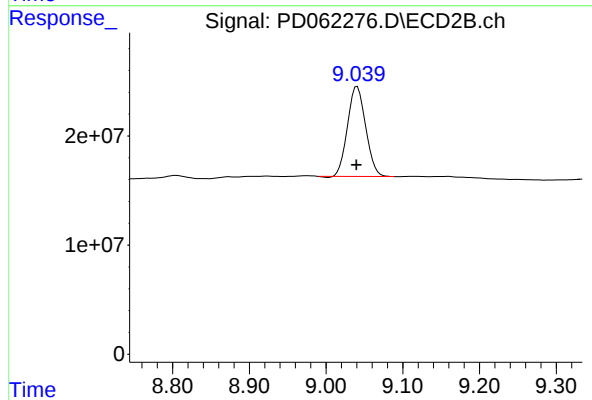

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 136073176
Conc: 14.41 ng/ml