

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
 Data File : PD062277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 21:03
 Operator : AR\AJ
 Sample : M2106-13
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-26-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:50:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 22:10:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.980	11008157	138.9E6	13.147	15.985
28)	SA Decachlor...	8.256	9.040	17960863	131.5E6	14.597	13.928
Target Compounds							
11)	B alpha-Chl...	5.490	6.162	477812	15311709	0.411m	1.343 #
12)	B 4,4'-DDE	5.654	6.316	7296447	84247160	6.493	7.311
17)	MA 4,4'-DDT	6.412	7.105	4945820	38148373	5.491	3.994 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
Data File : PD062277.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 21:03
Operator : AR\AJ
Sample : M2106-13
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SB-26-0-2.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:50:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 22:10:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

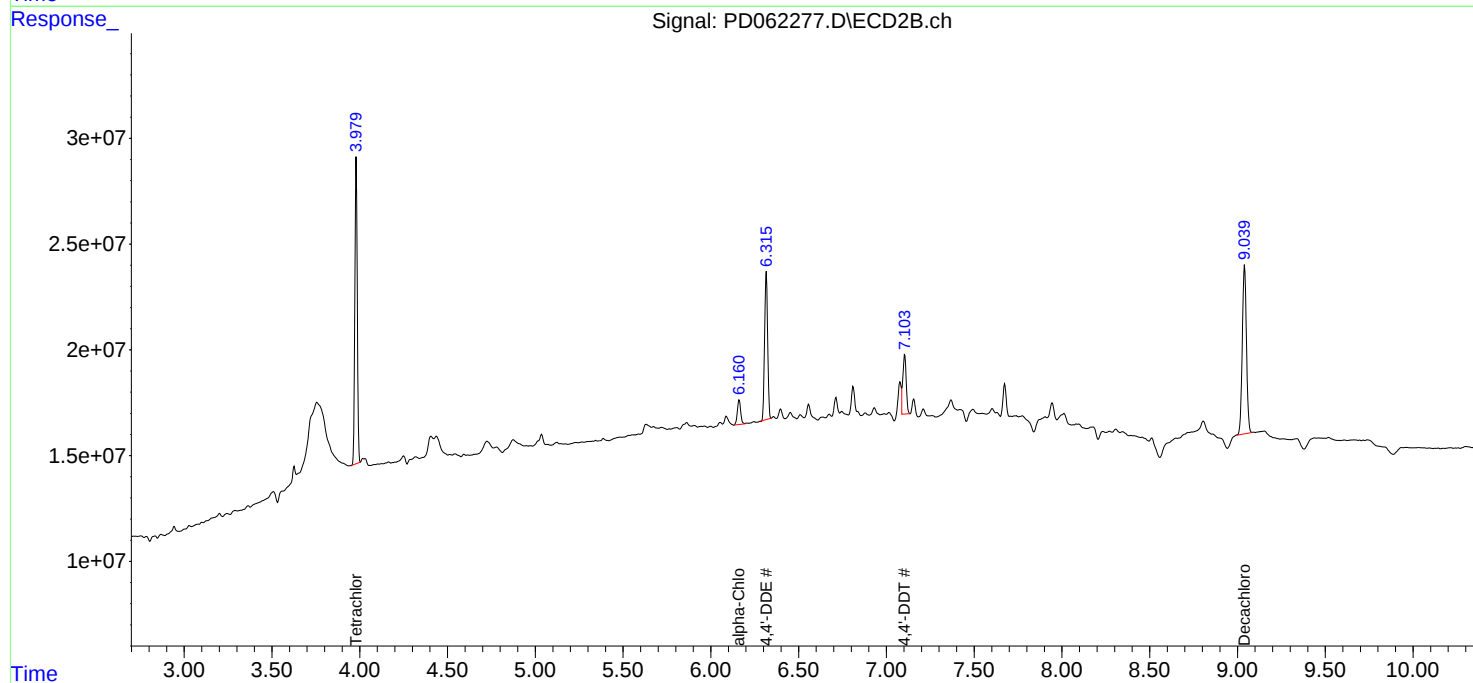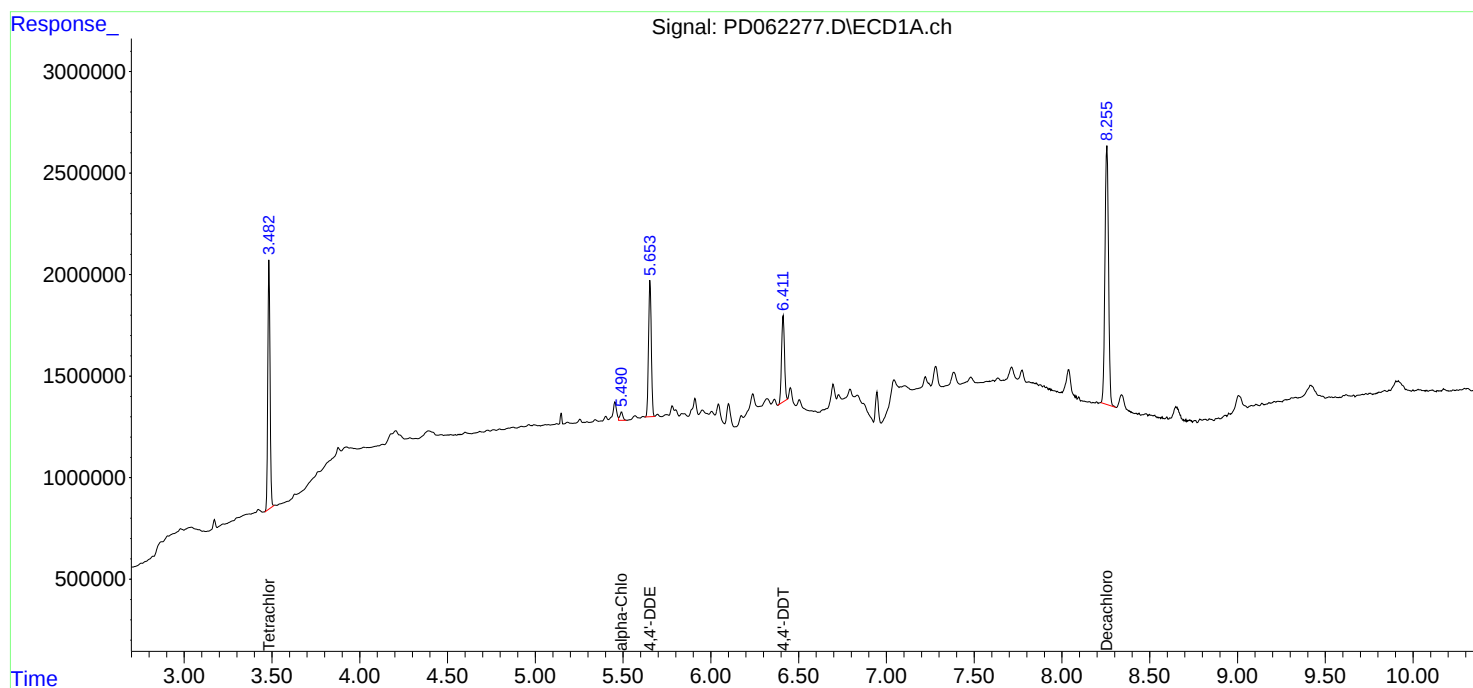

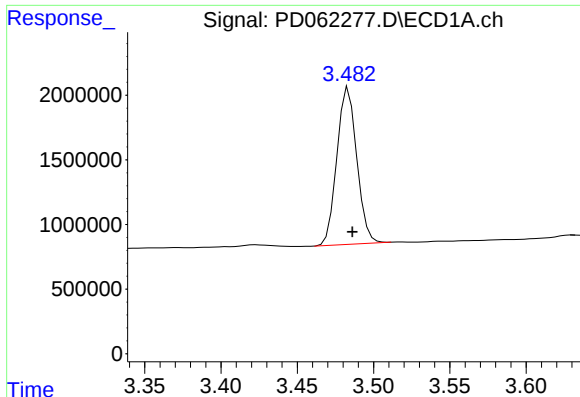


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 11008157
Conc: 13.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-26-0-2.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:50:14 PM

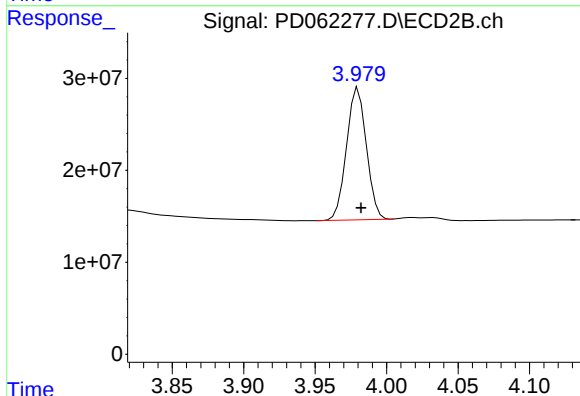


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 138894817
Conc: 15.99 ng/ml

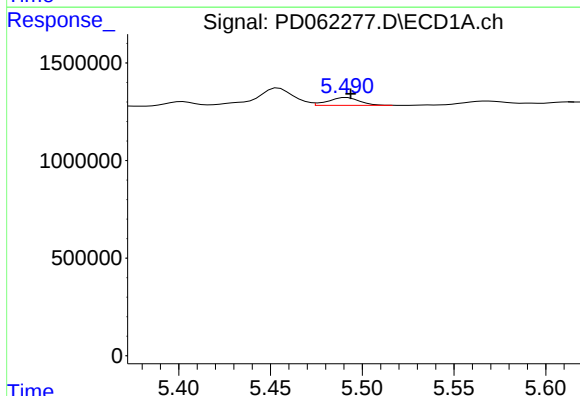


#11 alpha-Chlordane

R.T.: 5.490 min
Delta R.T.: -0.003 min
Response: 477812
Conc: 0.41 ng/ml m

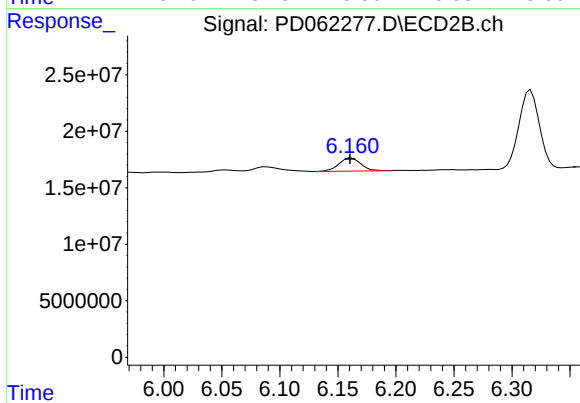

#11 alpha-Chlordane

R.T.: 6.162 min
Delta R.T.: 0.001 min
Response: 15311709
Conc: 1.34 ng/ml

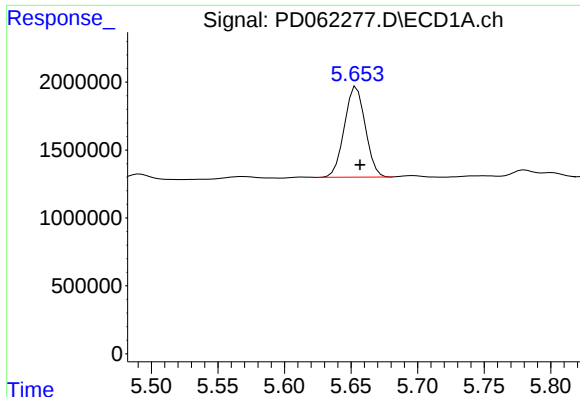


#12 4,4'-DDE

R.T.: 5.654 min
Delta R.T.: -0.003 min
Response: 7296447
Conc: 6.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-26-0-2.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:50:14 PM

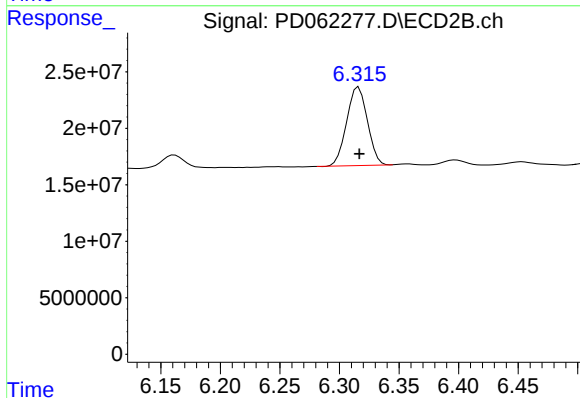


#12 4,4'-DDE

R.T.: 6.316 min
Delta R.T.: 0.000 min
Response: 84247160
Conc: 7.31 ng/ml

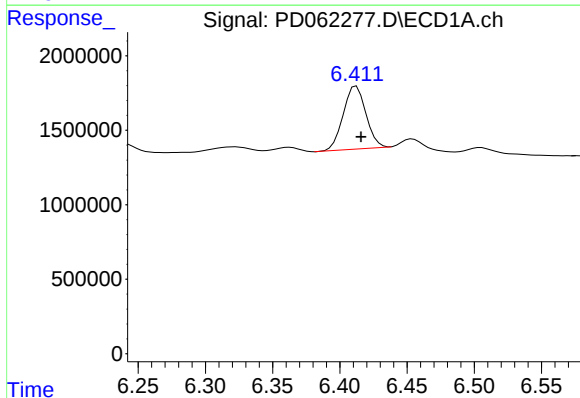


#17 4,4'-DDT

R.T.: 6.412 min
Delta R.T.: -0.003 min
Response: 4945820
Conc: 5.49 ng/ml

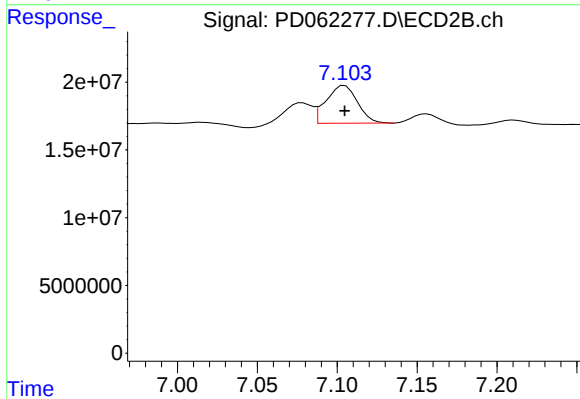

#17 4,4'-DDT

R.T.: 7.105 min
Delta R.T.: 0.000 min
Response: 38148373
Conc: 3.99 ng/ml

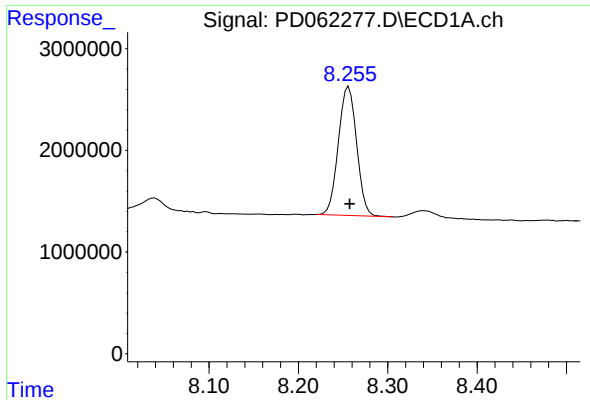


#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.001 min
Response: 17960863
Conc: 14.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-26-0-2.0

Manual Integrations
APPROVED

Ankita
4/23/2021 4:50:14 PM

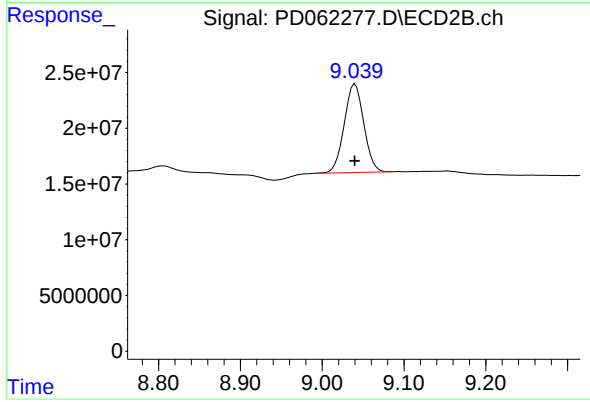

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 131484021
Conc: 13.93 ng/ml