

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042224\
 Data File : PD082550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2024 12:06
 Operator : AR\AJ
 Sample : P2037-24RX
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1CX9

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/23/2024
 Supervised By :Ankita Jodhani 04/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 21:26:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 02:08:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.562	2.773	16570353	31183230	10.927m	9.045m
2) SA Decachlor...	9.120	7.907	18545776	31108988	9.484m	9.560
Target Compounds						
5) MB Aldrin	5.285	4.236	3926881	9376503	1.688m	2.039m
9) A Endosulfan I	6.109	5.095	9592522	12658475	4.439	3.296 #
12) B 4,4'-DDE	6.255	5.229	7988202	5398361	3.881m	1.393m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042224\
Data File : PD082550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2024 12:06
Operator : AR\AJ
Sample : P2037-24RX
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 21:26:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 02:08:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

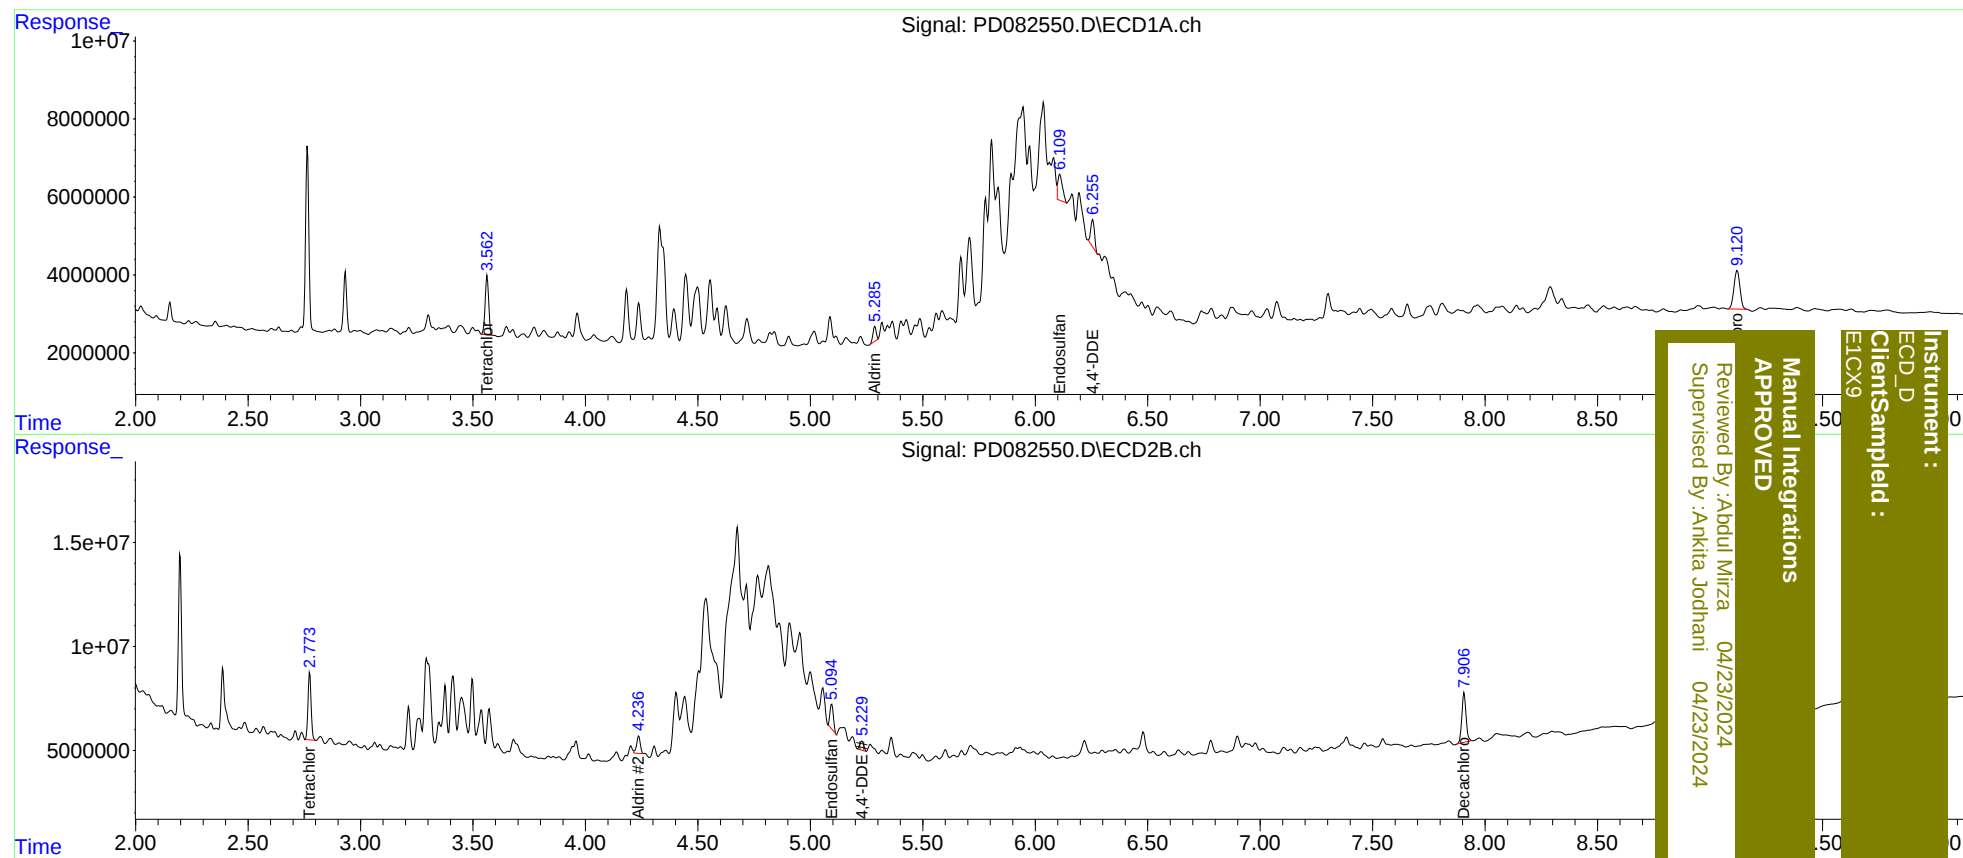

Instrument :
ECD_D
ClientSampled :
E1CX9

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/23/2024
Supervised By :Ankita Jodhani 04/23/2024