

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042319\
 Data File : PD053036.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2019 11:34
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 03:56:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042319CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 24 03:53:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds


2) A	alpha-BHC	0.000	4.458f	0 11233815	N.D.	0.295
6) B	beta-BHC	0.000	4.931f	0 12101160	N.D.	0.786

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042319\
Data File : PD053036.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2019 11:34
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 03:56:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042319CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 24 03:53:52 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

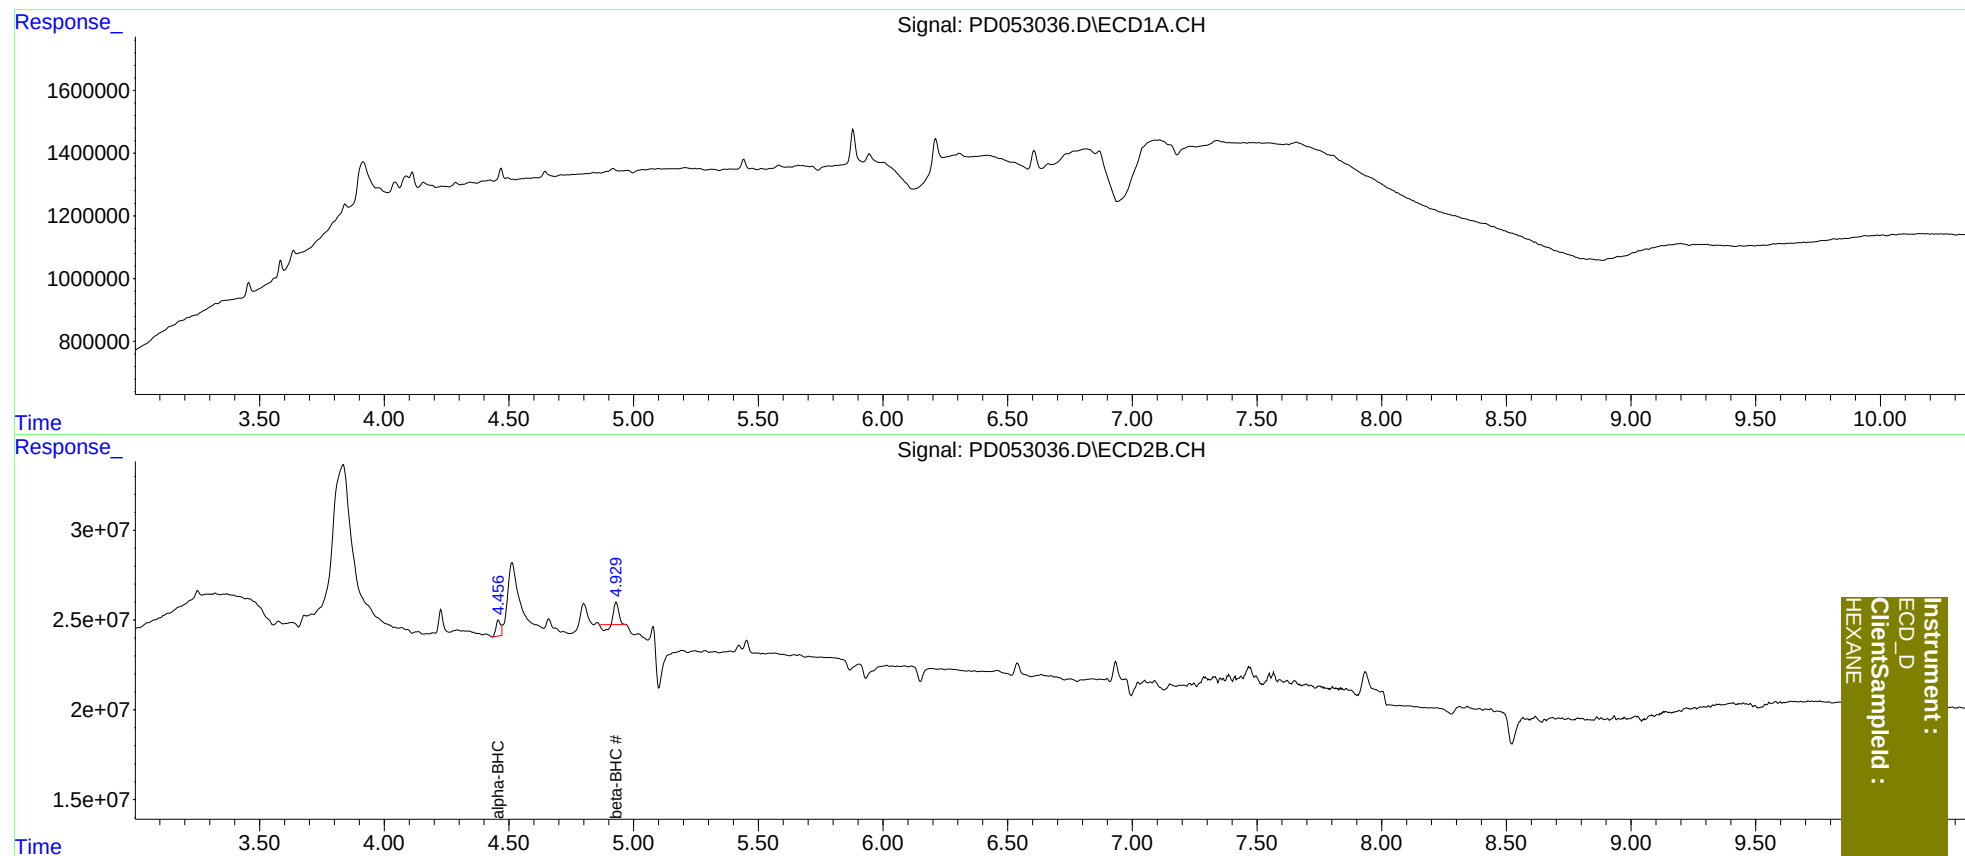


Instrument :
ECD_D
ClientSampleId :
HEXANE

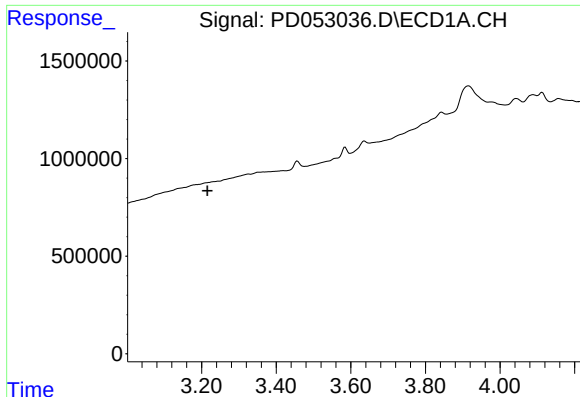

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.216 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

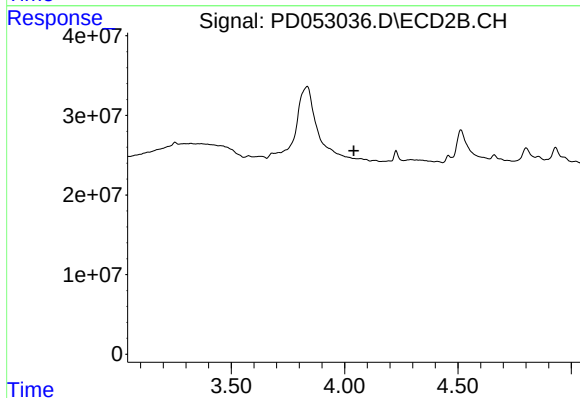


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.040 min
Response: 0
Conc: N.D.

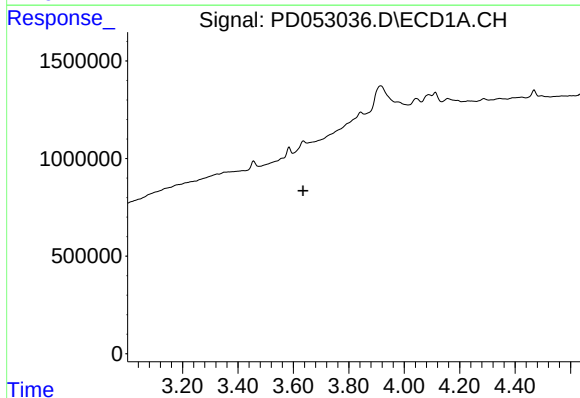


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.635 min
Response: 0
Conc: N.D.

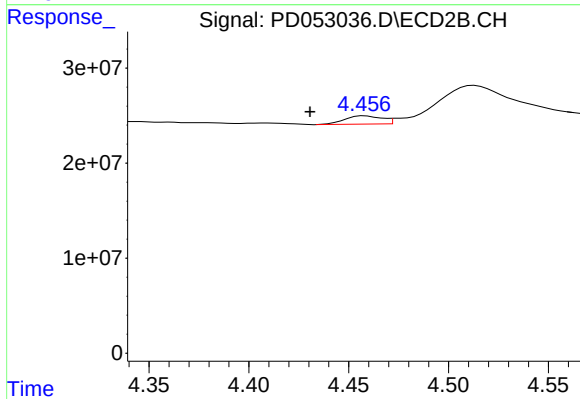

#2 alpha-BHC


R.T.: 4.458 min
Delta R.T.: 0.027 min
Response: 11233815
Conc: 0.29 ng/ml

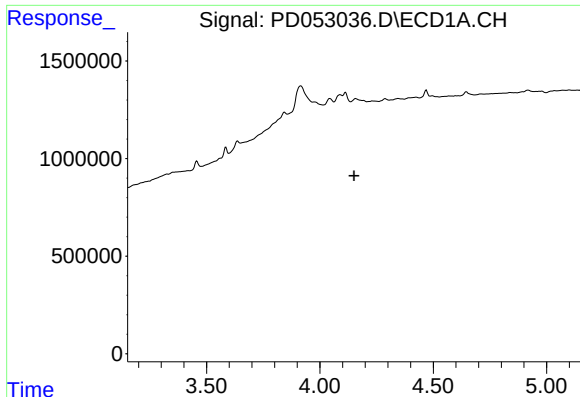

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

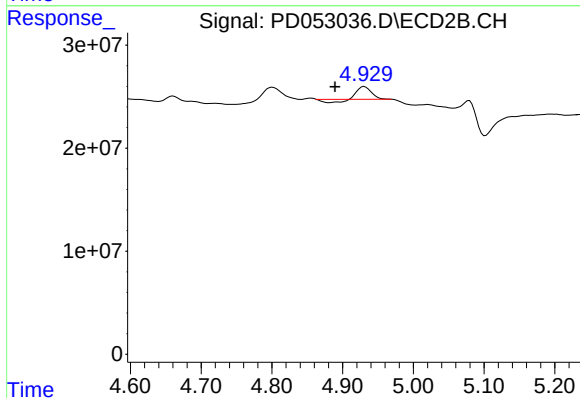


#6 beta-BHC

R.T.: 4.931 min
Delta R.T.: 0.041 min
Response: 12101160
Conc: 0.79 ng/ml

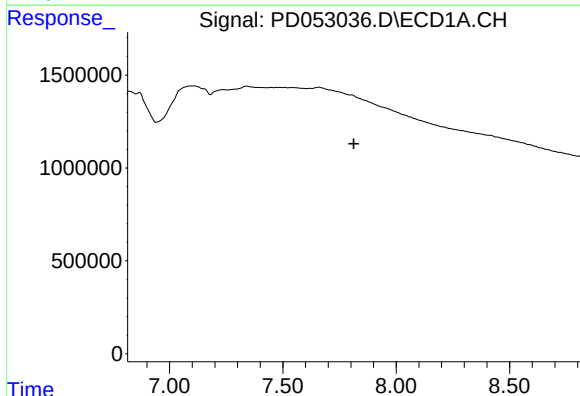

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.813 min
Response: 0
Conc: N.D.

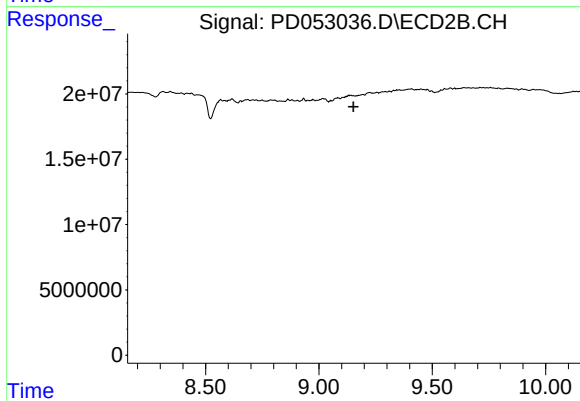

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.153 min
Response: 0
Conc: N.D.