

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042321\
 Data File : PD062294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2021 16:50
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 23:25:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
3) MA	gamma-BHC...	0.000	4.654	0	671994	N.D. 0.043 #
5) MB	Aldrin	0.000	5.472	0	220761	N.D. 0.015 #
8) B	Heptachlo...	0.000	5.860	0	28617715	N.D. 2.083 #
9) A	Endosulfan I	0.000	6.202	0	2429374	N.D. 0.185 #
11) B	alpha-Chl...	0.000	6.139f	0	14151431	N.D. 1.031 #
15) B	Endosulfa...	0.000	6.899	0	8364348	N.D. 0.727 #
20) A	Methoxychlor	0.000	7.572	0	3049385	N.D. 0.624 #
24)	Chlordane-2	0.000	5.472f	0	220761	N.D. 0.464 #
26)	Chlordane-4	0.000	6.139f	0	14151431	N.D. 6.215 #
27)	Chlordane-5	0.000	6.968	0	4740103	N.D. 11.521 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042321\
Data File : PD062294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2021 16:50
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 23:25:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

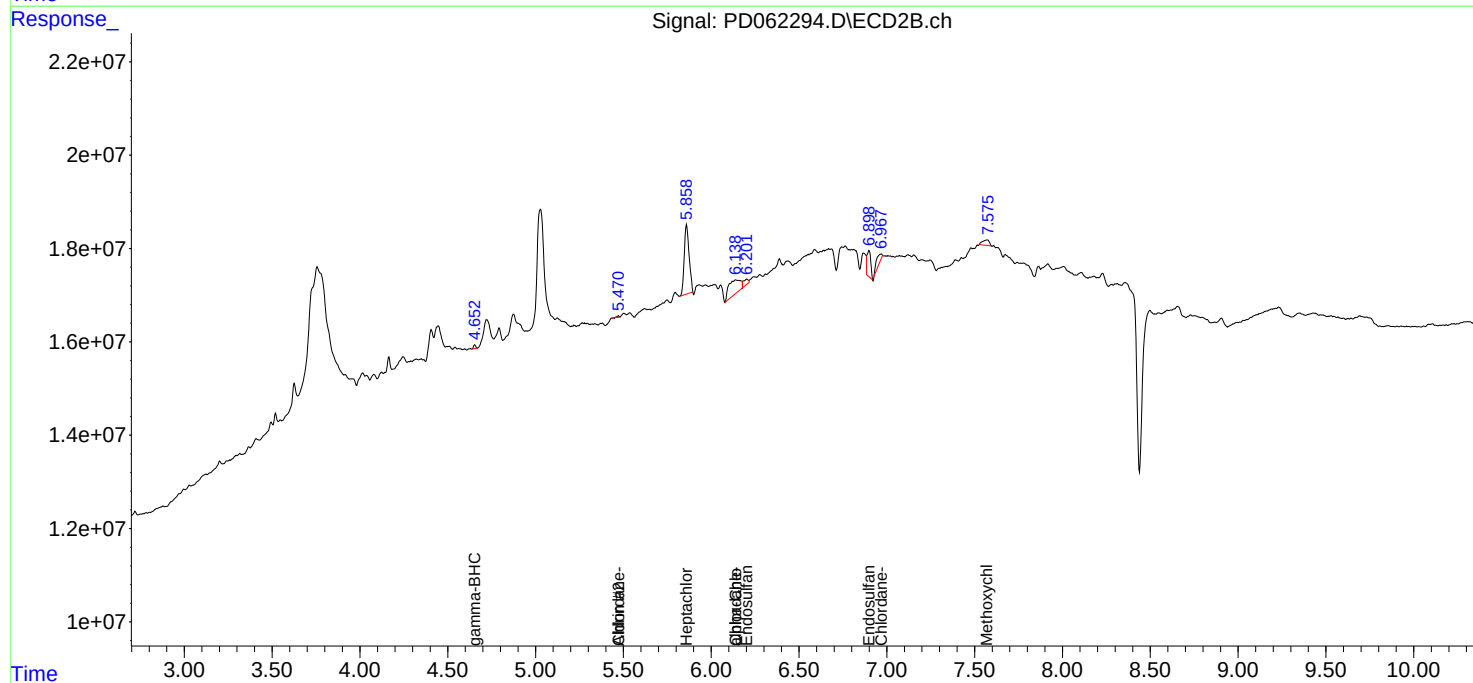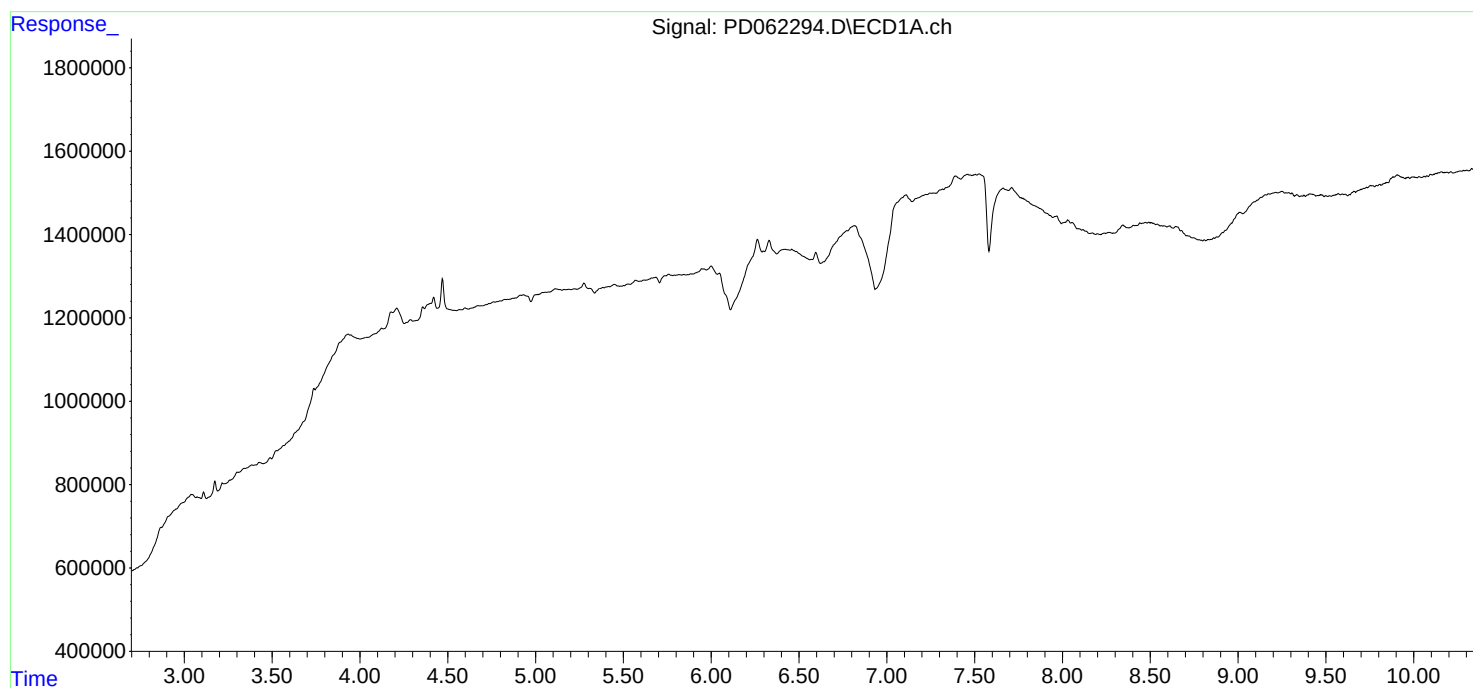


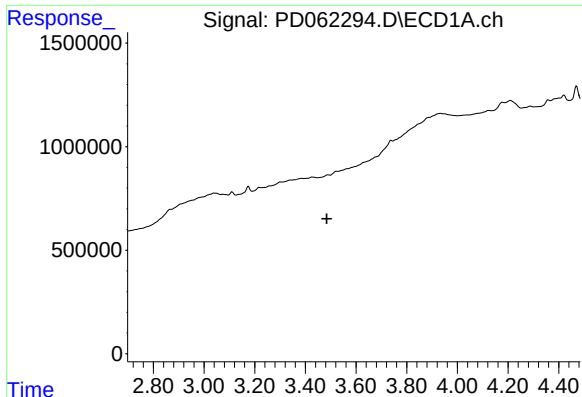

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.485 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

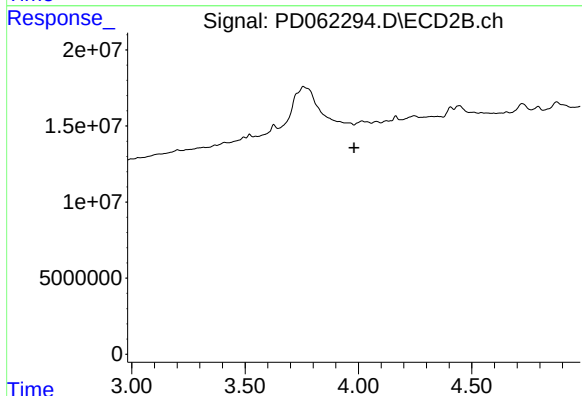


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.981 min
Response: 0
Conc: N.D.

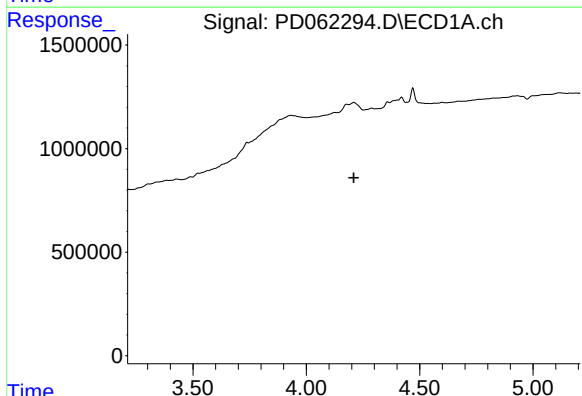


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.209 min
Response: 0
Conc: N.D.

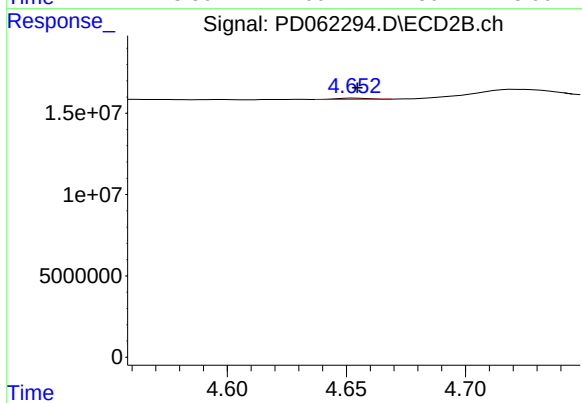

#3 gamma-BHC (Lindane)


R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 671994
Conc: 0.04 ng/ml

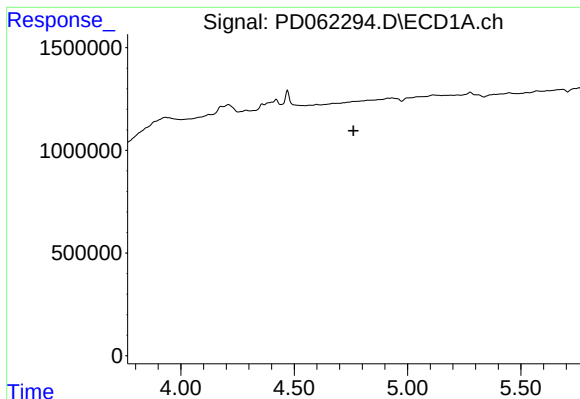

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.762 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

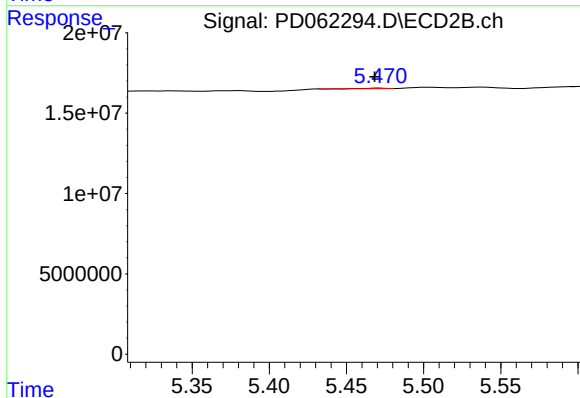


#5 Aldrin

R.T.: 5.472 min
Delta R.T.: 0.003 min
Response: 220761
Conc: 0.01 ng/ml

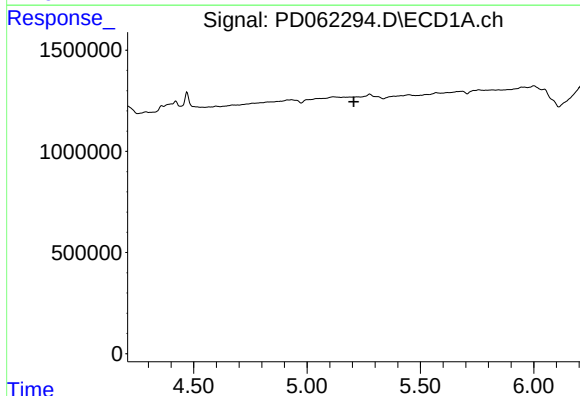


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.206 min
Response: 0
Conc: N.D.

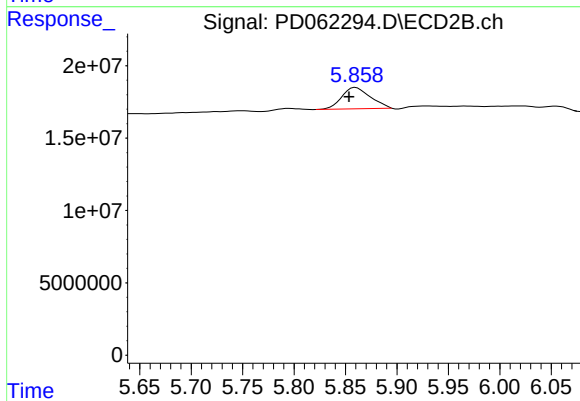

#8 Heptachlor epoxide


R.T.: 5.860 min
Delta R.T.: 0.006 min
Response: 28617715
Conc: 2.08 ng/ml

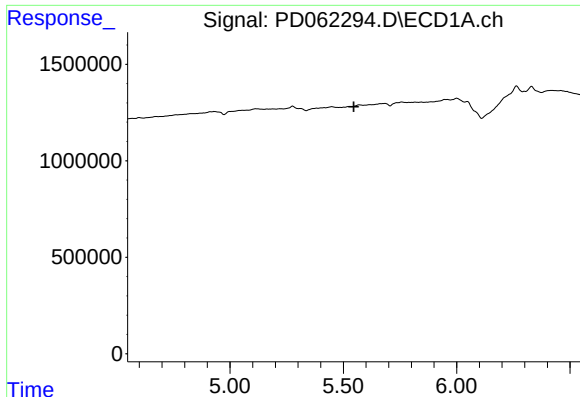

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.547 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

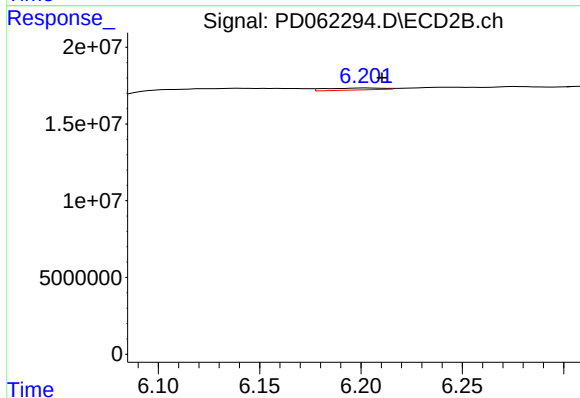


#9 Endosulfan I

R.T.: 6.202 min
Delta R.T.: -0.008 min
Response: 2429374
Conc: 0.19 ng/ml

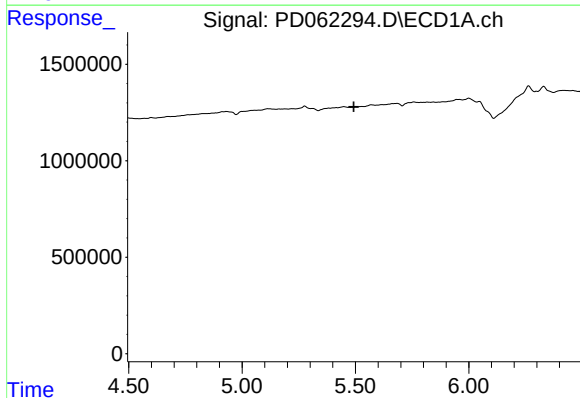


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.492 min
Response: 0
Conc: N.D.

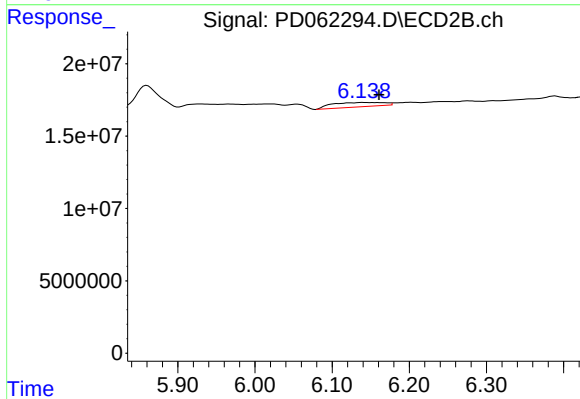

#11 alpha-Chlordane


R.T.: 6.139 min
Delta R.T.: -0.022 min
Response: 14151431
Conc: 1.03 ng/ml

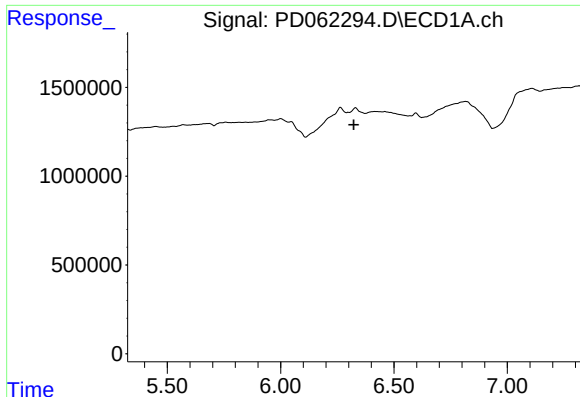

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

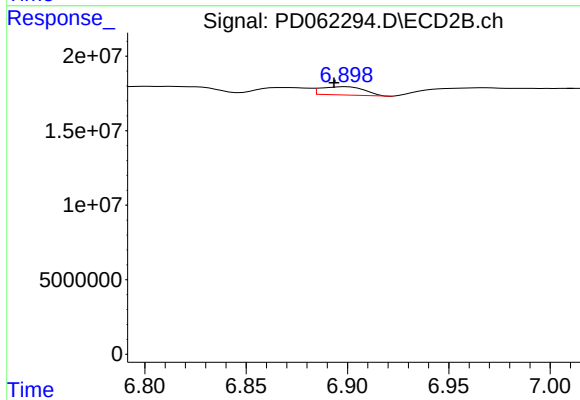


#15 Endosulfan II

R.T.: 6.899 min
Delta R.T.: 0.006 min
Response: 8364348
Conc: 0.73 ng/ml

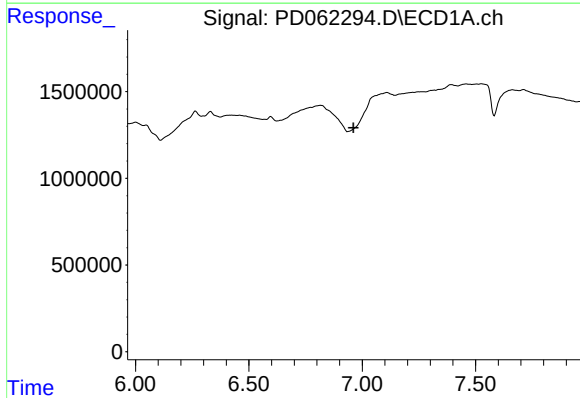


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.962 min
Response: 0
Conc: N.D.

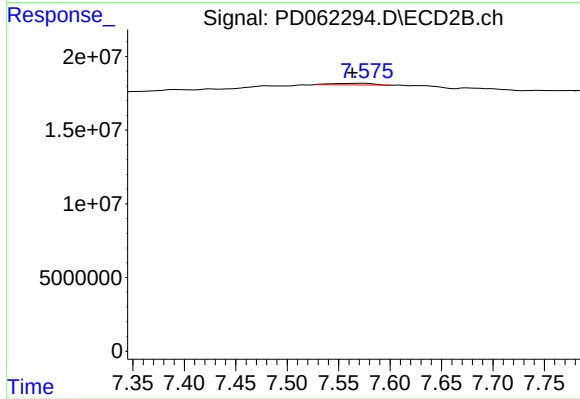

#20 Methoxychlor


R.T.: 7.572 min
Delta R.T.: 0.009 min
Response: 3049385
Conc: 0.62 ng/ml

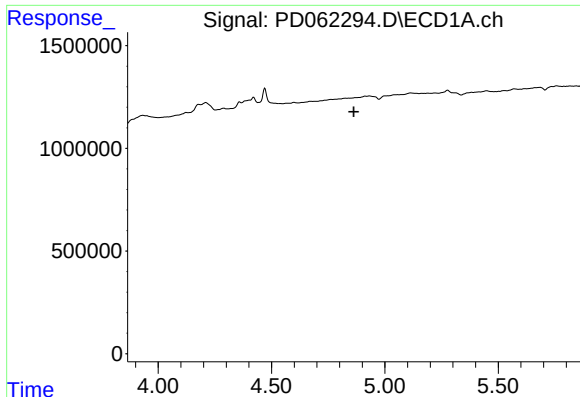

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.862 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

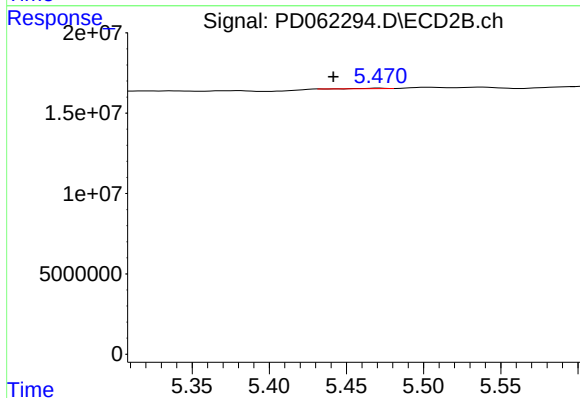


#24 Chlordane-2

R.T.: 5.472 min
Delta R.T.: 0.030 min
Response: 220761
Conc: 0.46 ng/ml

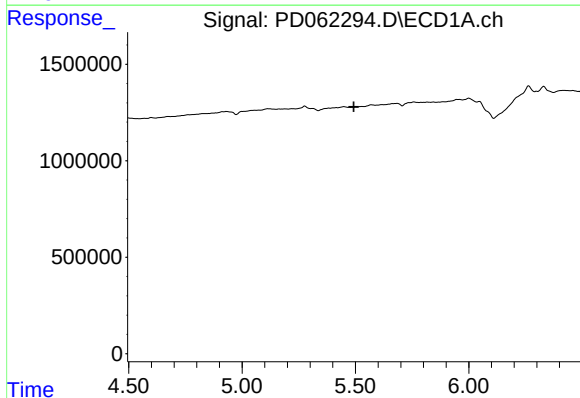


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.493 min
Response: 0
Conc: N.D.

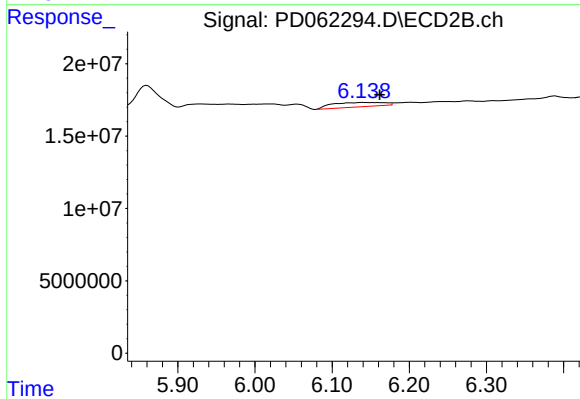

#26 Chlordane-4


R.T.: 6.139 min
Delta R.T.: -0.022 min
Response: 14151431
Conc: 6.21 ng/ml

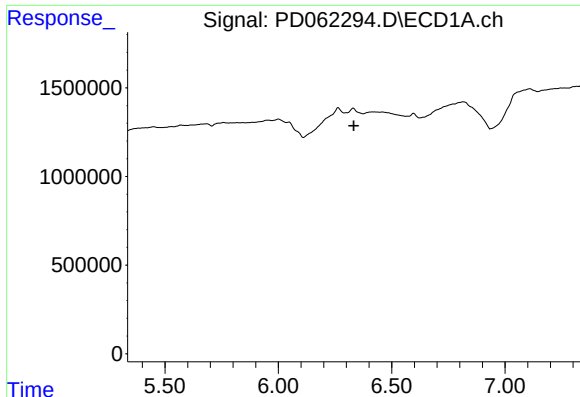

#27 Chlor dane-5


R.T.: 0.000 min
Exp R.T. : 6.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

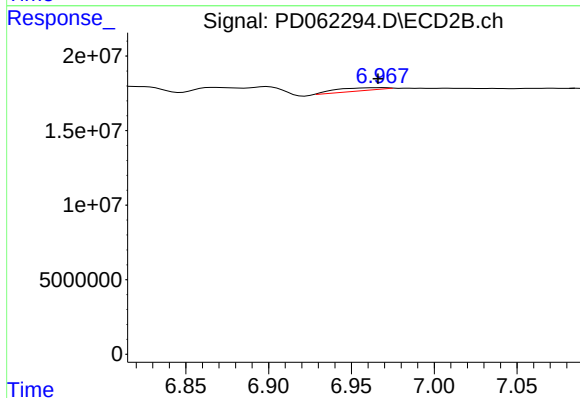


#27 Chlor dane-5

R.T.: 6.968 min
Delta R.T.: 0.002 min
Response: 4740103
Conc: 11.52 ng/ml

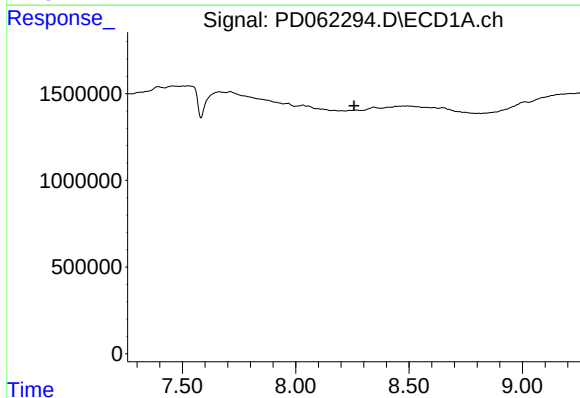

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.258 min
Response: 0
Conc: N.D.

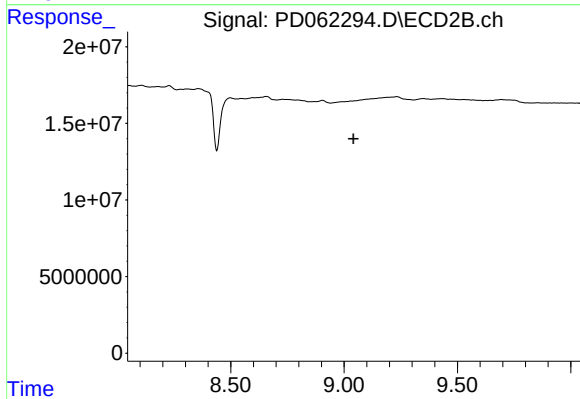

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.042 min
Response: 0
Conc: N.D.