

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042321\
 Data File : PD062303.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2021 18:56
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 23:13:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:13:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	47611613	528.2E6	50.000	50.000
28)	SA Decachlor...	8.257	9.042	57877129	421.4E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.360	4.974	17351462	246.9E6	500.000	500.000
24)	Chlordane-2	4.862	5.442	20889495	238.0E6	500.000	500.000
25)	Chlordane-3	5.434	6.087	62352584	982.3E6	500.000	500.000
26)	Chlordane-4	5.493	6.162	52394360	1138.5E6	500.000	500.000
27)	Chlordane-5	6.333	6.966	22659217	205.7E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042321\
Data File : PD062303.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2021 18:56
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 23:13:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:13:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

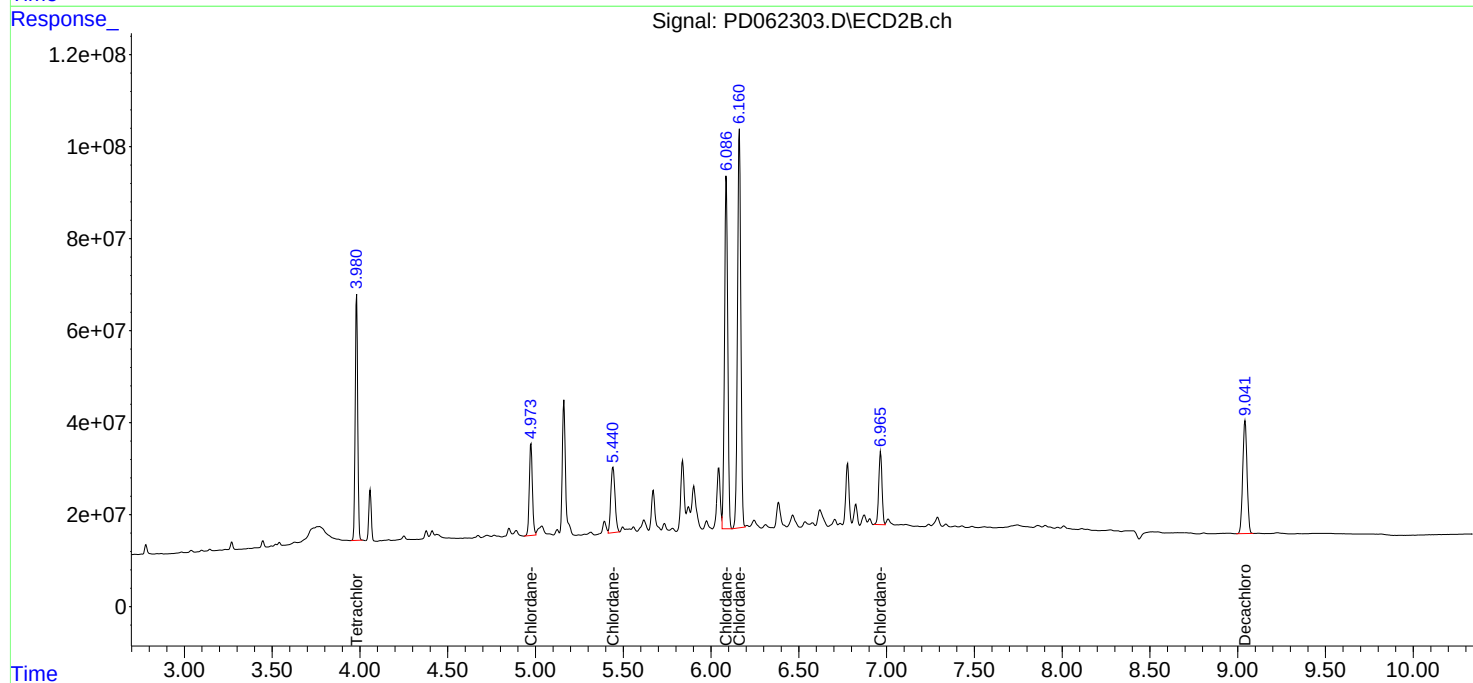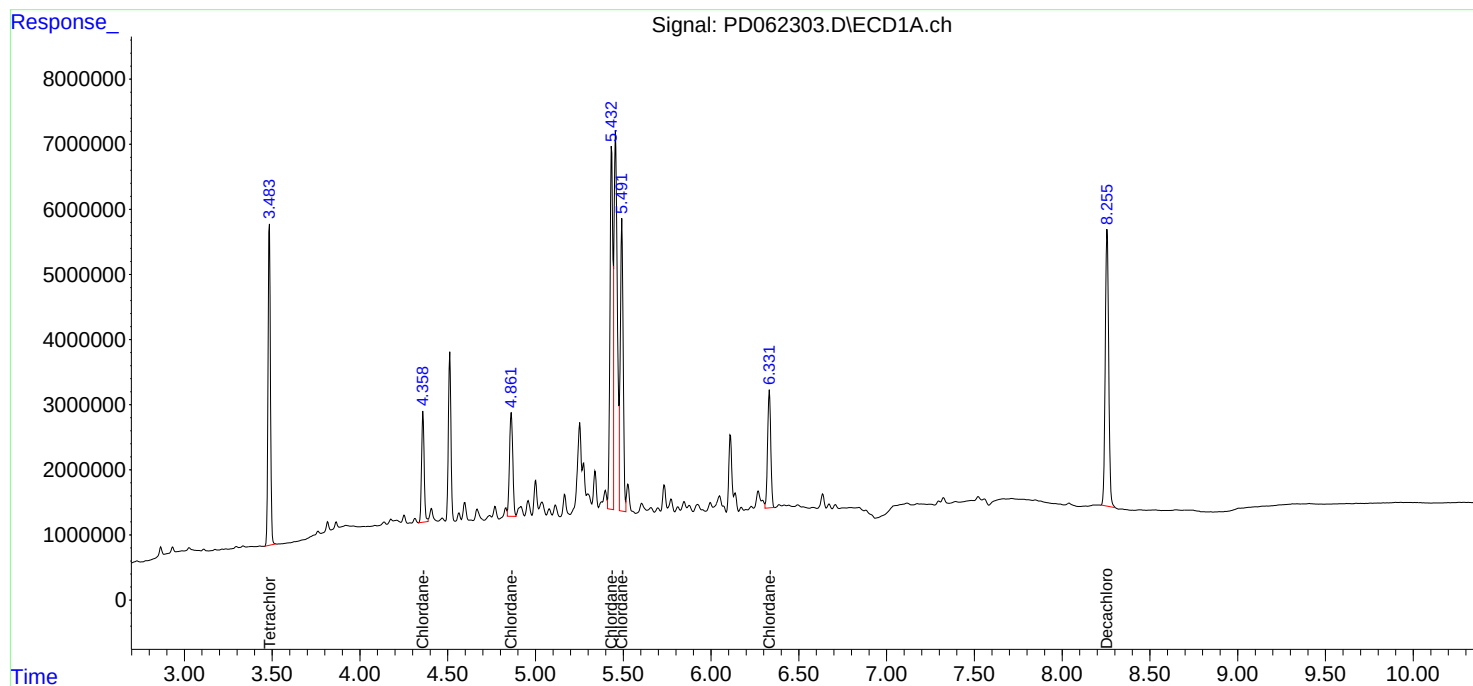


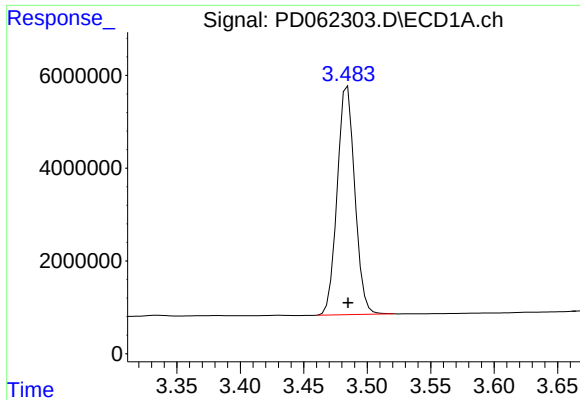

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 47611613
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

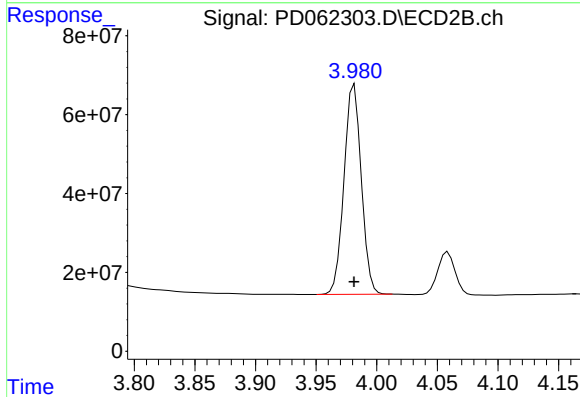


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 528178310
Conc: 50.00 ng/ml

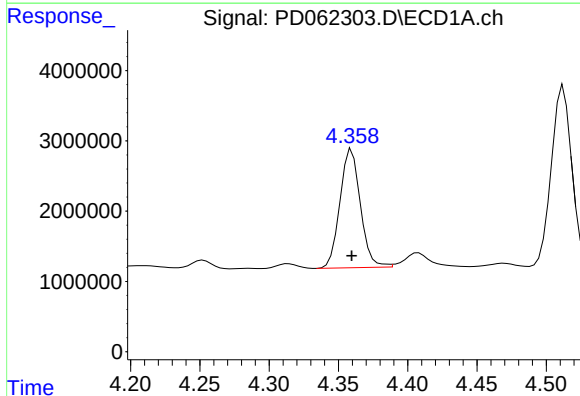


#23 Chlordane-1

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 17351462
Conc: 500.00 ng/ml

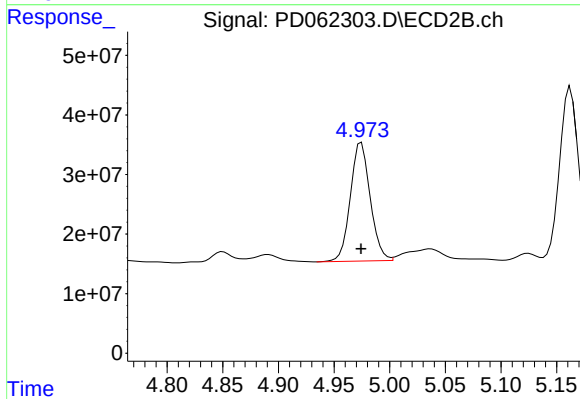

#23 Chlordane-1


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 246851260
Conc: 500.00 ng/ml

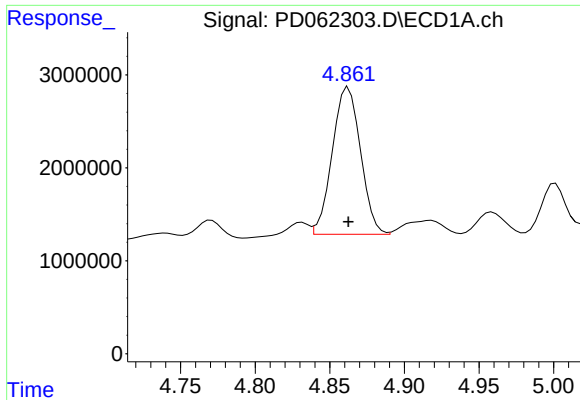

#24 Chlordane-2


R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 20889495
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

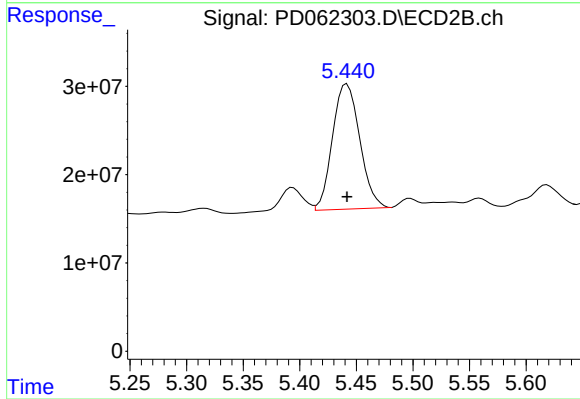


#24 Chlordane-2

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 238012910
Conc: 500.00 ng/ml

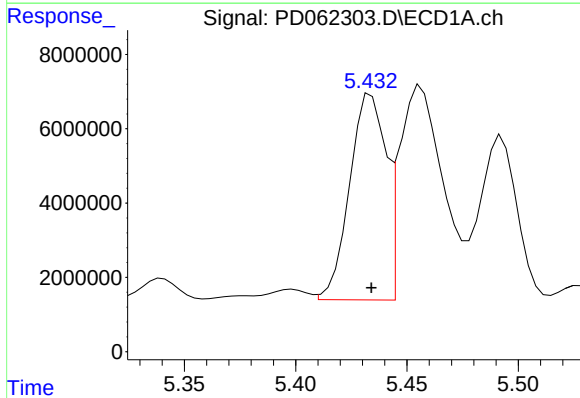


#25 Chlordane-3

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 62352584
Conc: 500.00 ng/ml

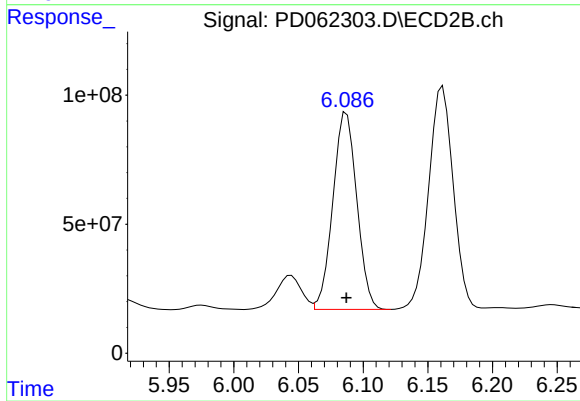

#25 Chlordane-3


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 982330589
Conc: 500.00 ng/ml

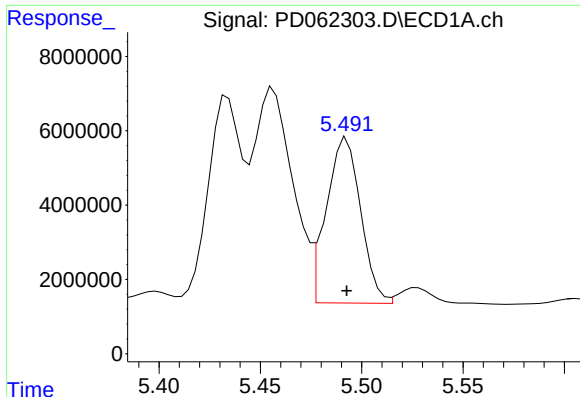

#26 Chlordane-4


R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 52394360
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

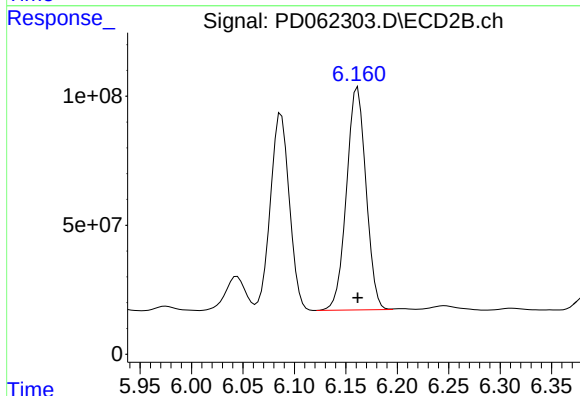


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 1138508665
Conc: 500.00 ng/ml

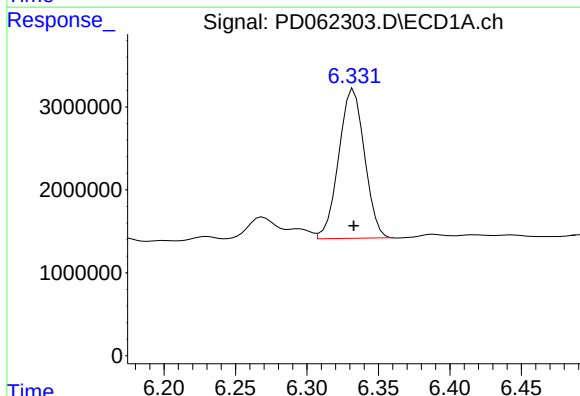


#27 Chlordane-5

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 22659217
Conc: 500.00 ng/ml

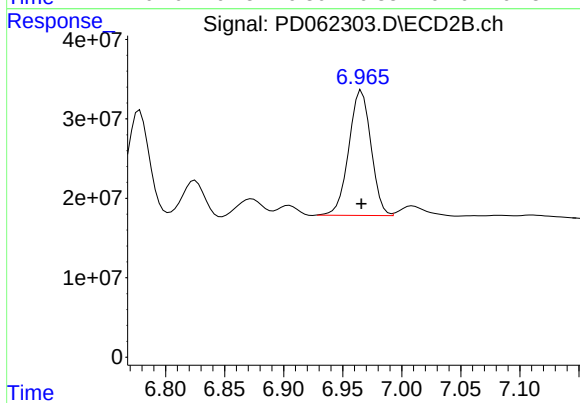

#27 Chlordane-5


R.T.: 6.966 min
Delta R.T.: 0.000 min
Response: 205718709
Conc: 500.00 ng/ml

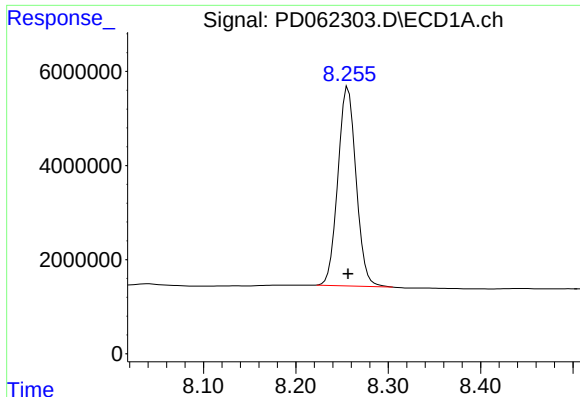

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 57877129
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

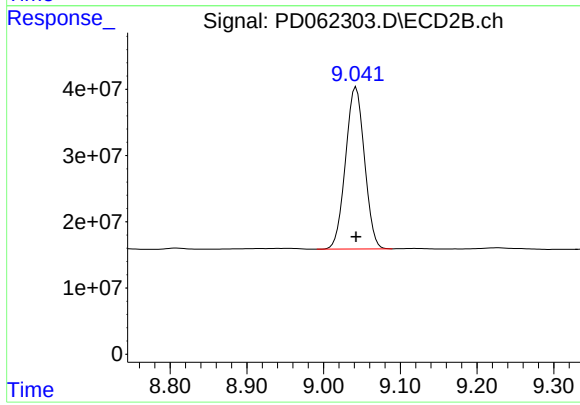

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 421421919
Conc: 50.00 ng/ml