

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042321\
 Data File : PD062320.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2021 22:53
 Operator : AR\AJ
 Sample : M2106-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-26-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/26/2021 4:22:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 23:30:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	10270869	134.6E6	12.610	12.782
28)	SA Decachlor...	8.257	9.042	16362105	120.3E6	13.489	14.182
Target Compounds							
12)	B 4,4'-DDE	5.654	6.317	6816964	82684139	5.616m	5.856
17)	MA 4,4'-DDT	6.414	7.106	4802191	49799865	4.703	4.994

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042321\
Data File : PD062320.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2021 22:53
Operator : AR\AJ
Sample : M2106-13
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SB-26-0-2.0


Manual Integrations
APPROVED

Ankita
4/26/2021 4:22:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 23:30:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

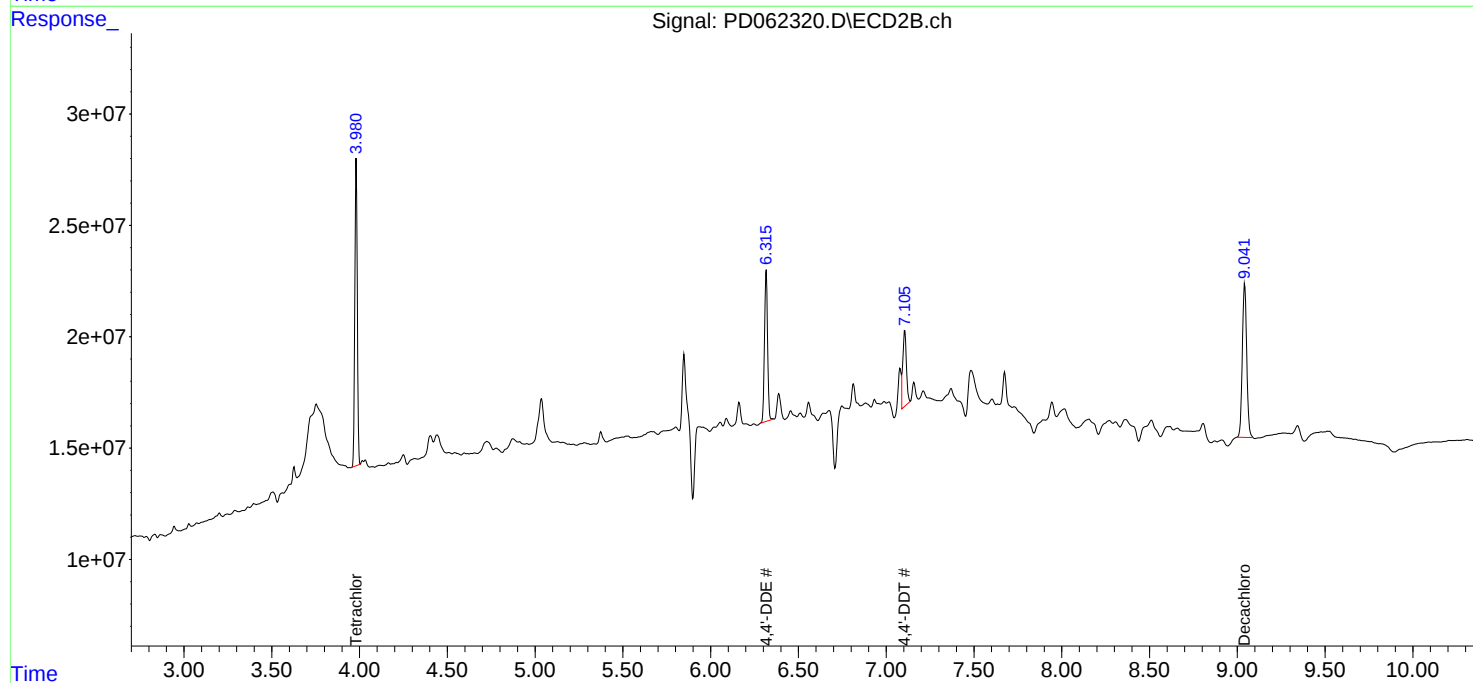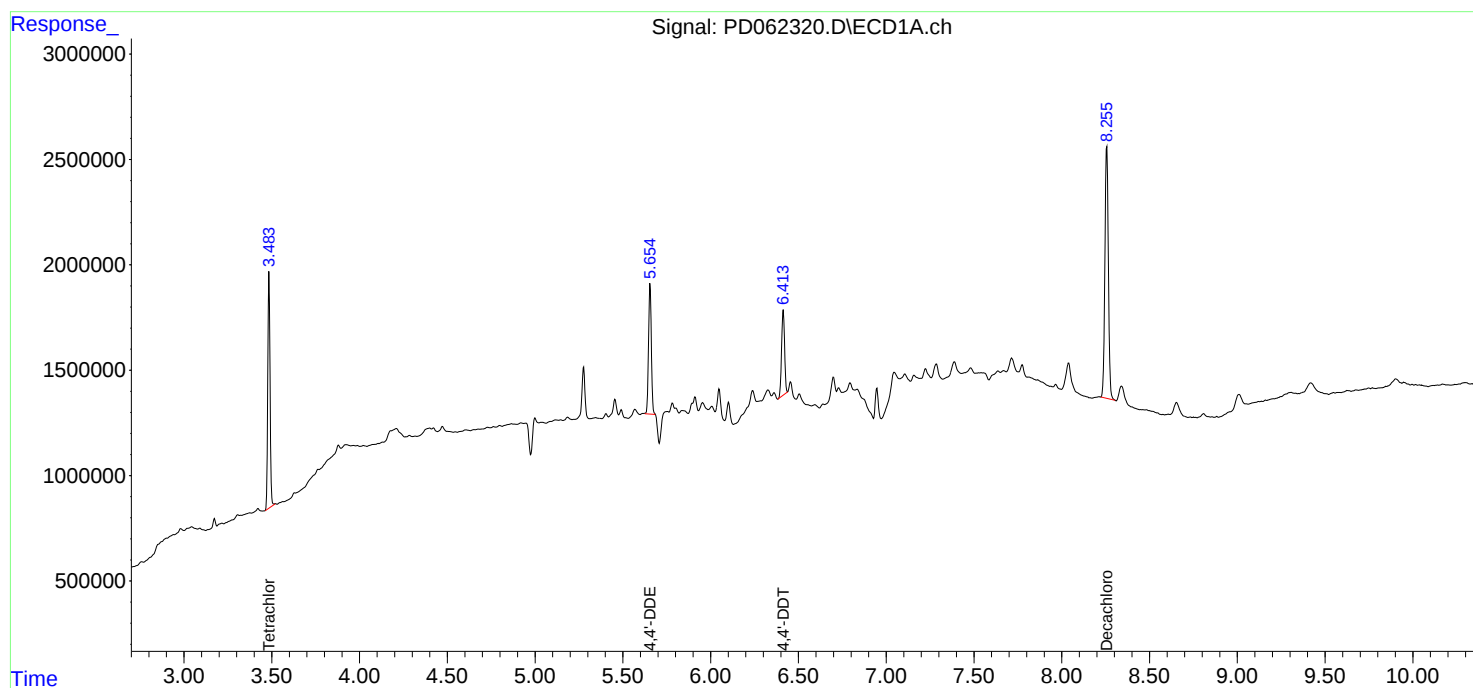

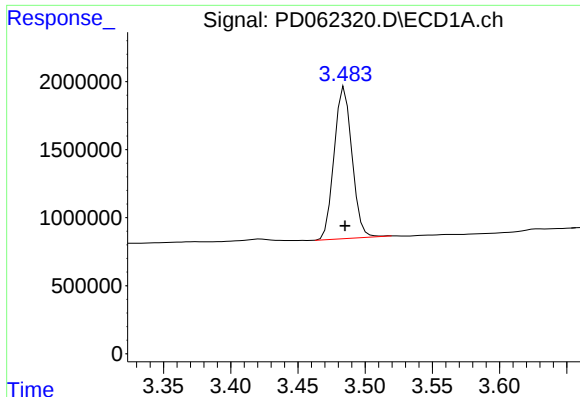


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 10270869
Conc: 12.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-26-0-2.0


Manual Integrations
APPROVED

Ankita
4/26/2021 4:22:59 PM

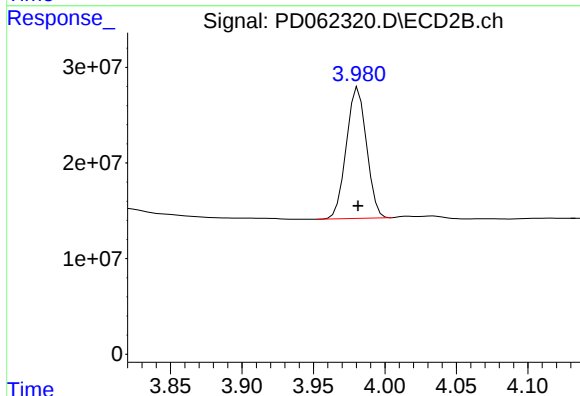


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 134612325
Conc: 12.78 ng/ml

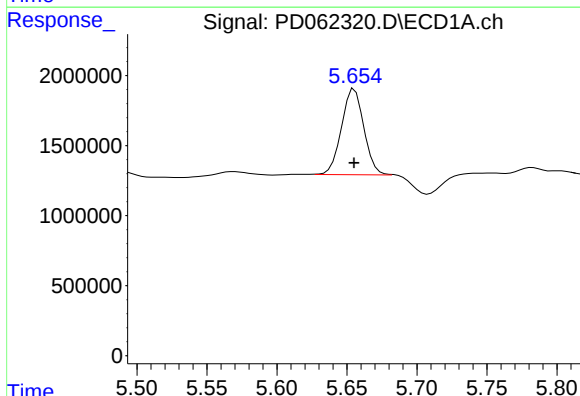


#12 4,4'-DDE

R.T.: 5.654 min
Delta R.T.: -0.001 min
Response: 6816964
Conc: 5.62 ng/ml m

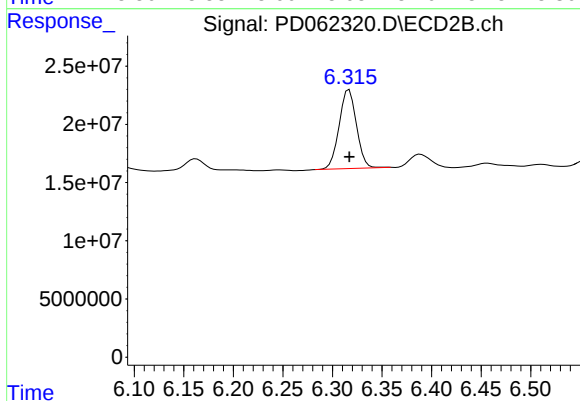

#12 4,4'-DDE

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 82684139
Conc: 5.86 ng/ml

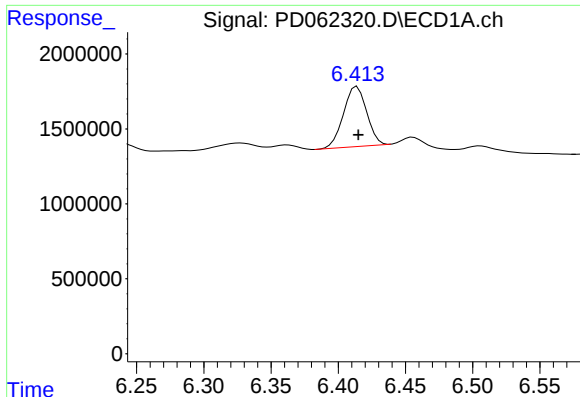


#17 4,4'-DDT

R.T.: 6.414 min
Delta R.T.: -0.001 min
Response: 4802191
Conc: 4.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-26-0-2.0


Manual Integrations
APPROVED

Ankita
4/26/2021 4:22:59 PM

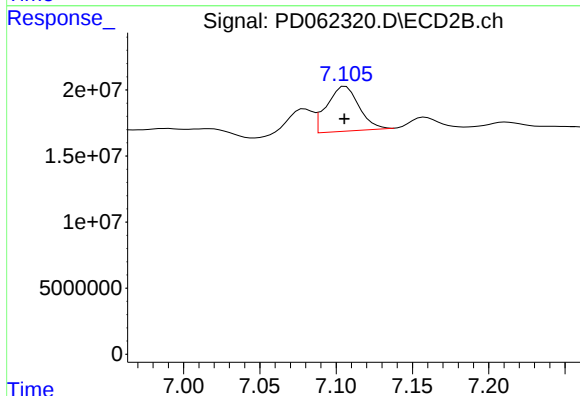


#17 4,4'-DDT

R.T.: 7.106 min
Delta R.T.: 0.000 min
Response: 49799865
Conc: 4.99 ng/ml

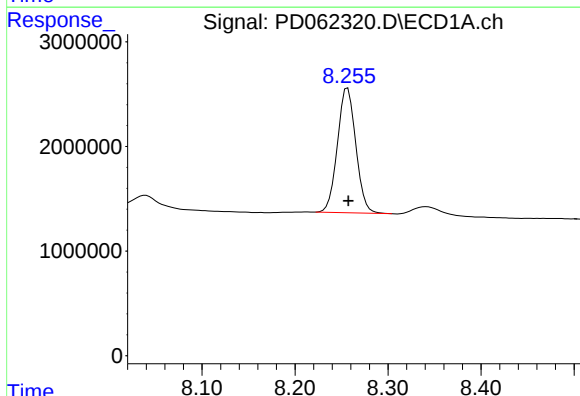

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 16362105
Conc: 13.49 ng/ml

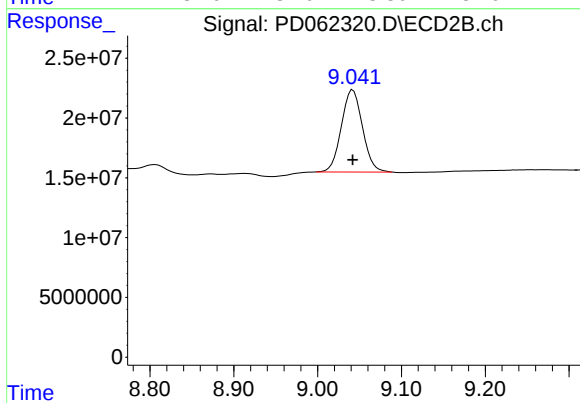

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 120334801
Conc: 14.18 ng/ml