

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042324\
 Data File : PD082564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2024 14:43
 Operator : AR\AJ
 Sample : P2037-23
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1CX8

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/26/2024
 Supervised By :Ankita Jodhani 04/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 04:52:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 02:08:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.569	2.776	18814552	35090574	12.407m	10.178m
2) SA Decachlor...	9.127	7.909	20178102	37933274	10.318m	11.658m
Target Compounds						
5) MB Aldrin	5.293	4.237	8578252	17326102	3.687m	3.769m
9) A Endosulfan I	6.113	5.096	10223467	25808193	4.731m	6.720m#
12) B 4,4'-DDE	6.261	5.230	18332994	10477142	8.907m	2.704m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042324\
Data File : PD082564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2024 14:43
Operator : AR\AJ
Sample : P2037-23
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 04:52:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 02:08:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

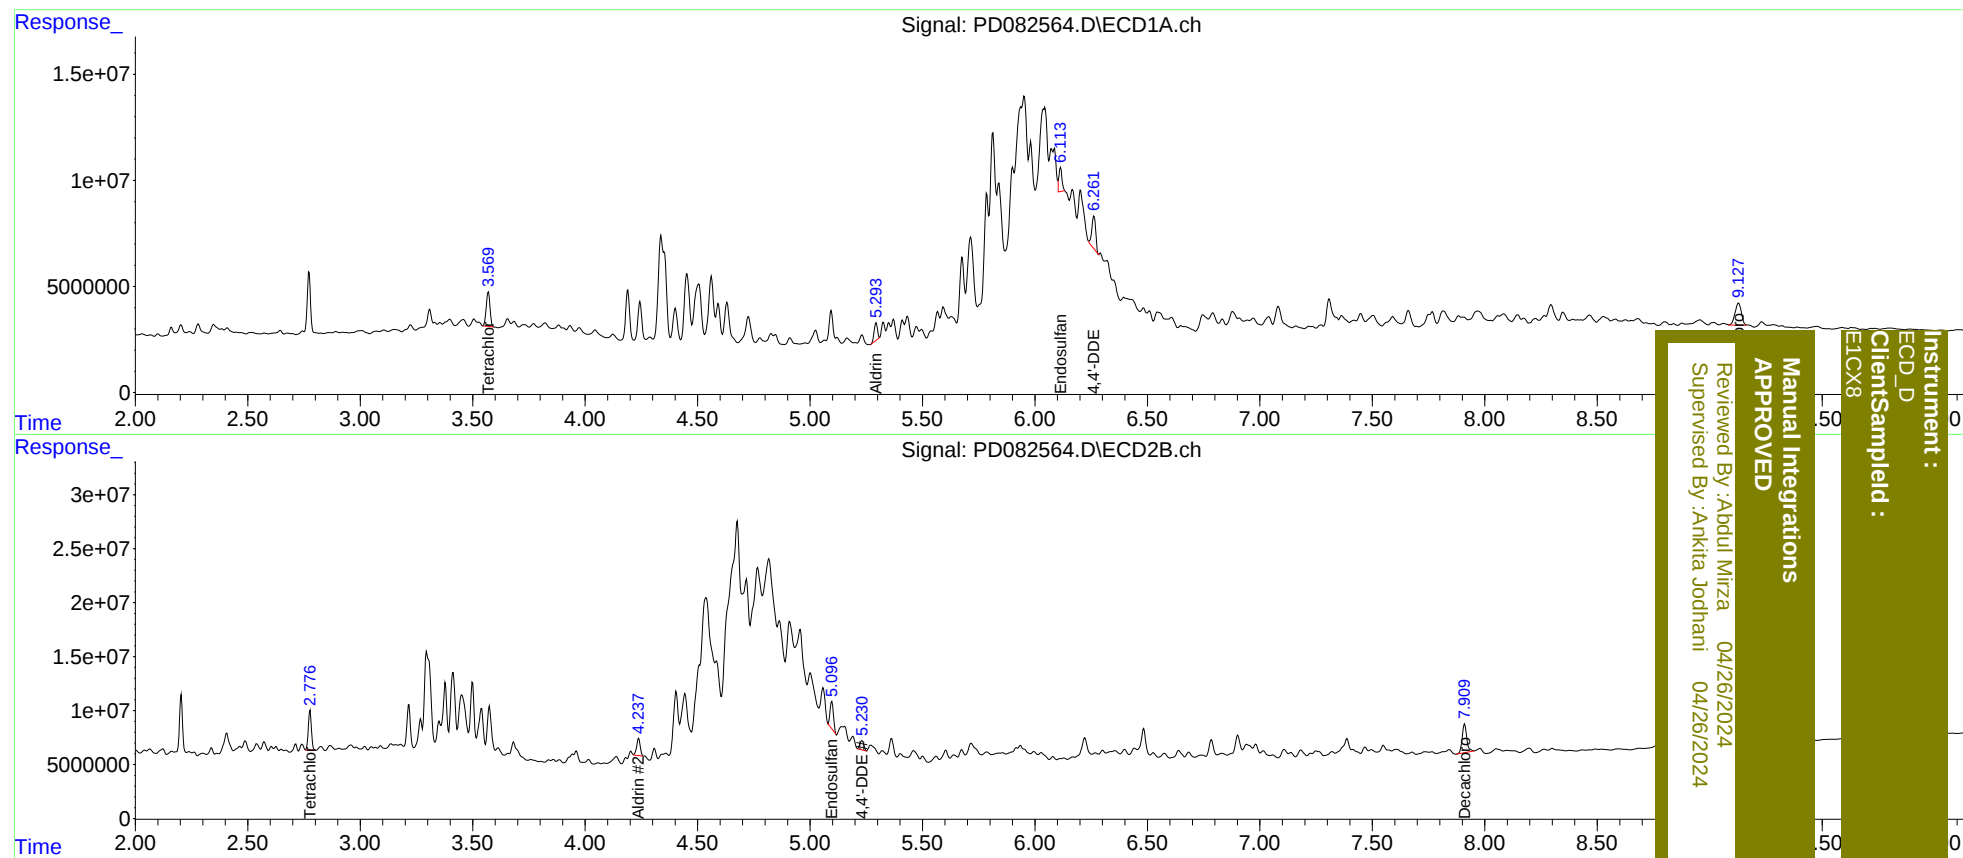

Instrument :
ECD_D
ClientSampled :
E1CX8

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 04/26/2024
Supervised By: Ankita Jodhani 04/26/2024