

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042419\
 Data File : PD053059.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Apr 2019 8:38
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:44:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042319CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 24 03:53:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	0.000	4.928f	0 29764054	N.D.	1.933
8) B	Heptachlo...	0.000	5.923	0 71849795	N.D.	2.338
14) MA	Endrin	0.000	6.760	0 65159315	N.D.	2.706
20) A	Methoxychlor	0.000	7.586f	0 2102194	N.D.	0.208


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042419\
Data File : PD053059.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Apr 2019 8:38
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:44:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042319CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 24 03:53:52 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

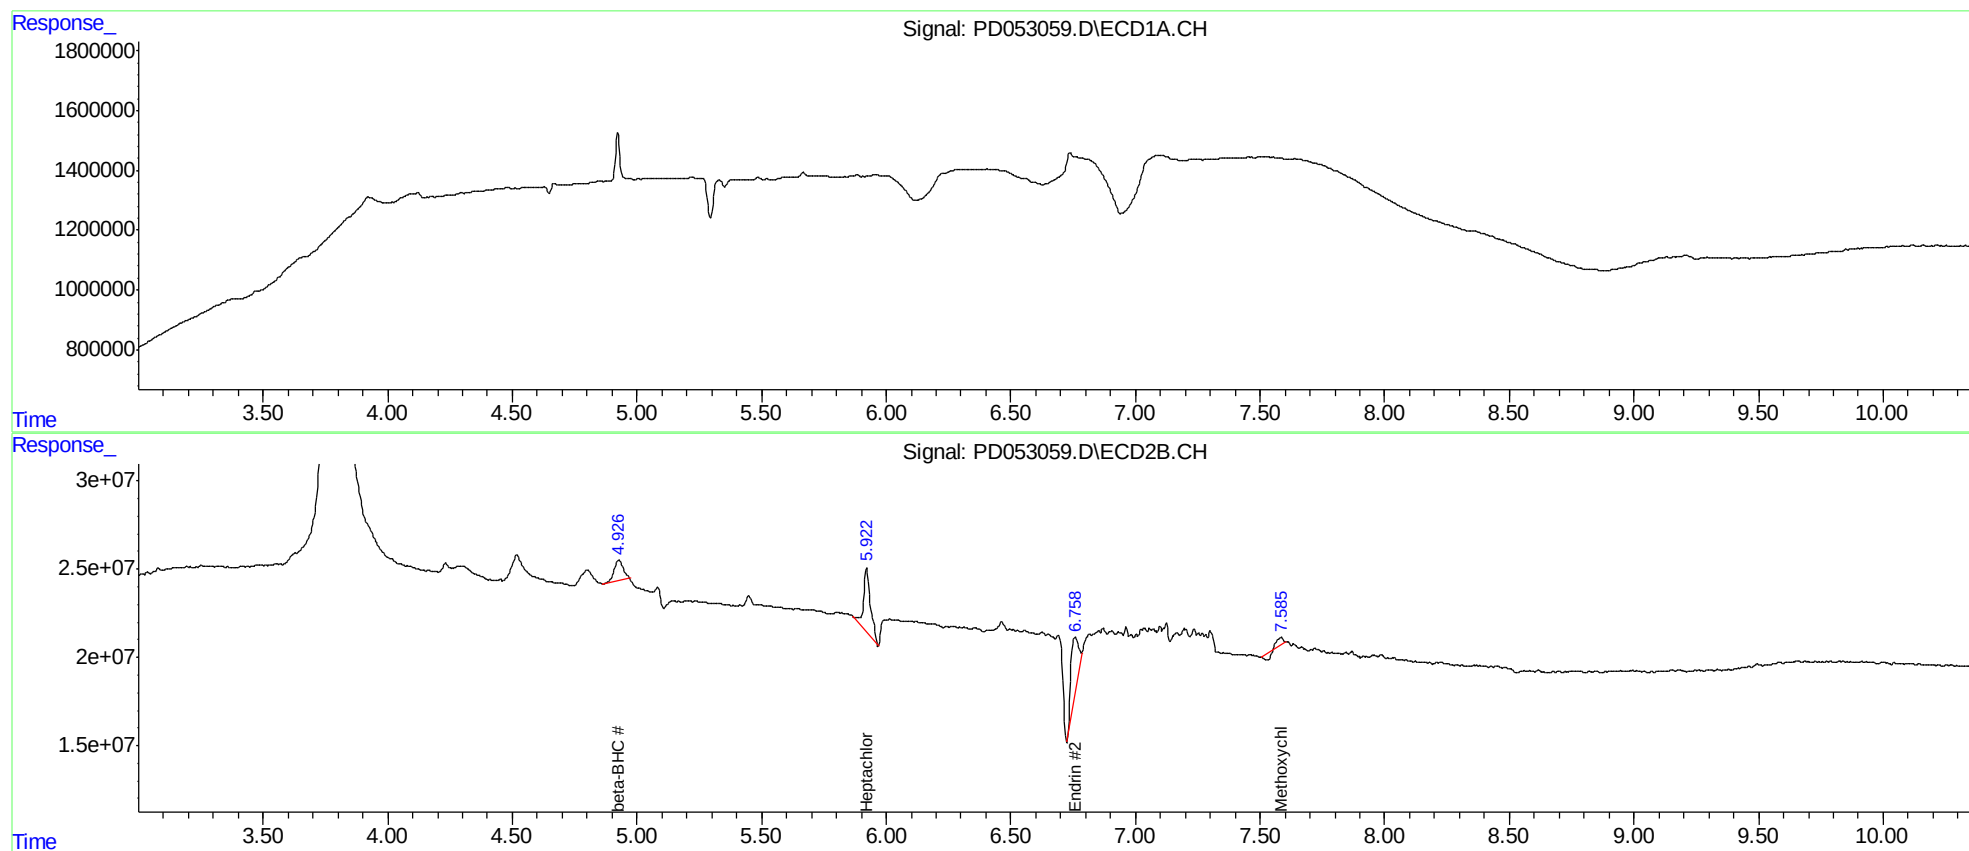


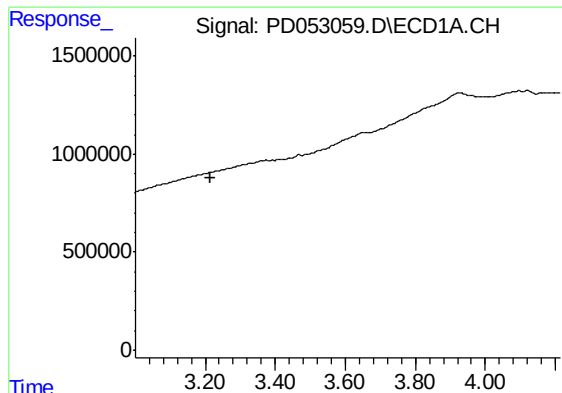

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.216 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

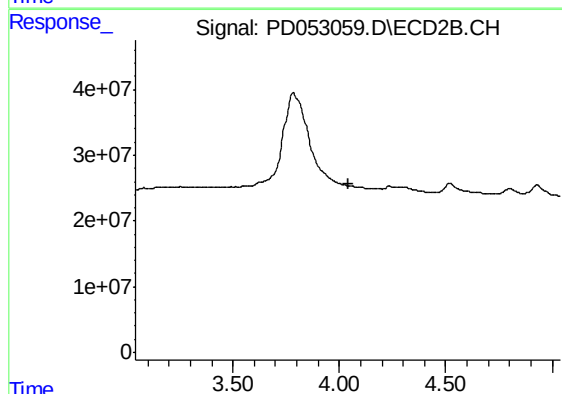


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.040 min
Response: 0
Conc: N.D.

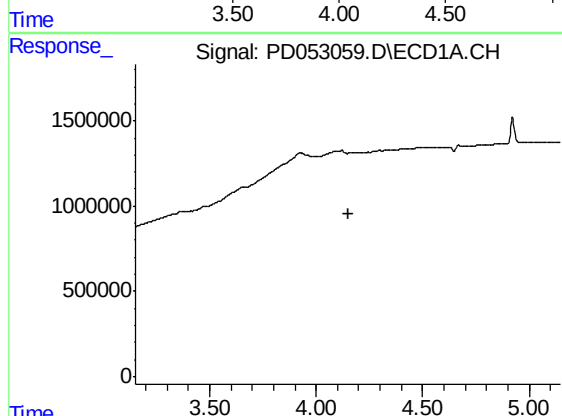


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.151 min
Response: 0
Conc: N.D.

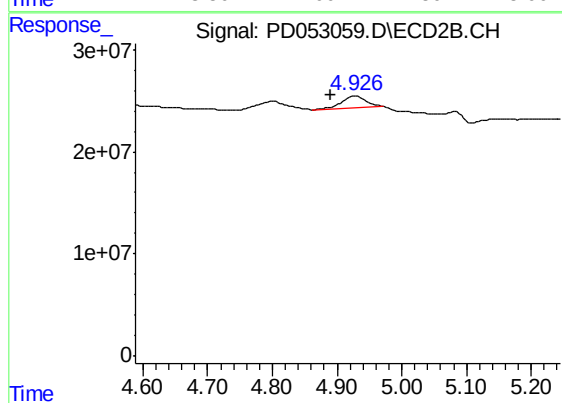

#6 beta-BHC


R.T.: 4.928 min
Delta R.T.: 0.038 min
Response: 29764054
Conc: 1.93 ng/ml

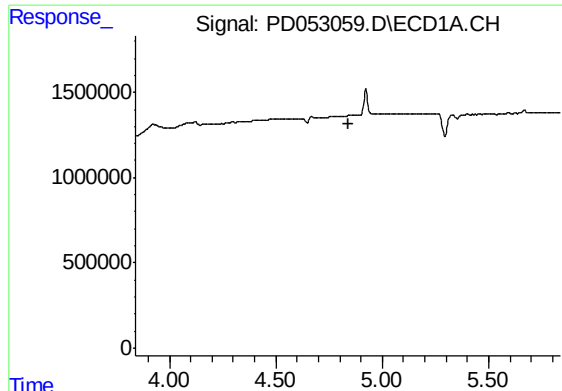

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.840 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

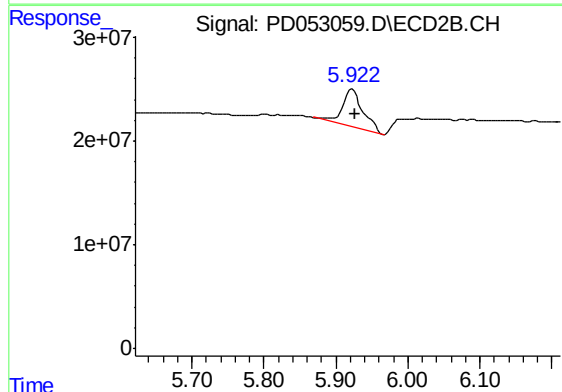


#8 Heptachlor epoxide

R.T.: 5.923 min
Delta R.T.: -0.003 min
Response: 71849795
Conc: 2.34 ng/ml

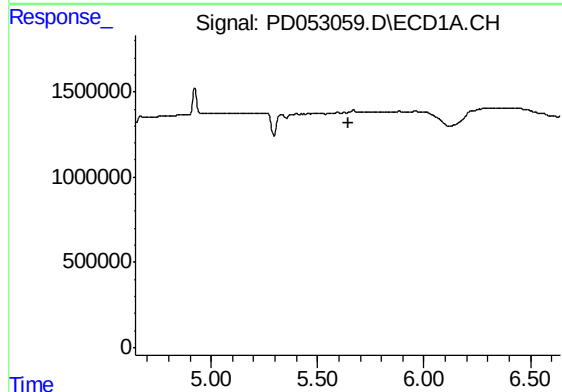


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.643 min
Response: 0
Conc: N.D.

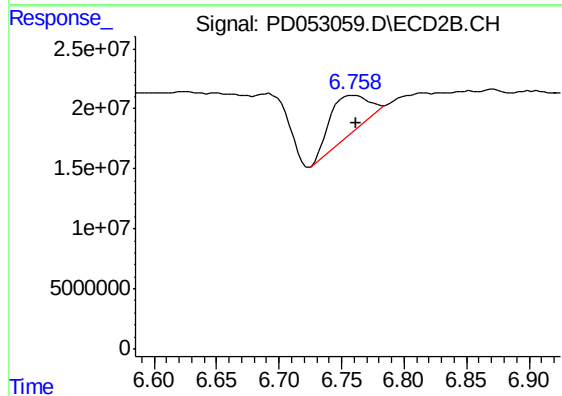

#14 Endrin


R.T.: 6.760 min
Delta R.T.: -0.002 min
Response: 65159315
Conc: 2.71 ng/ml

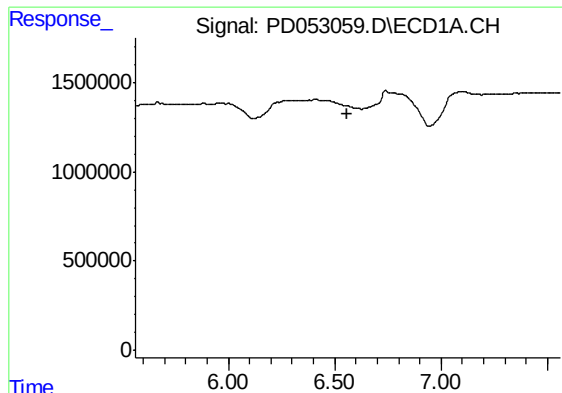

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.561 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

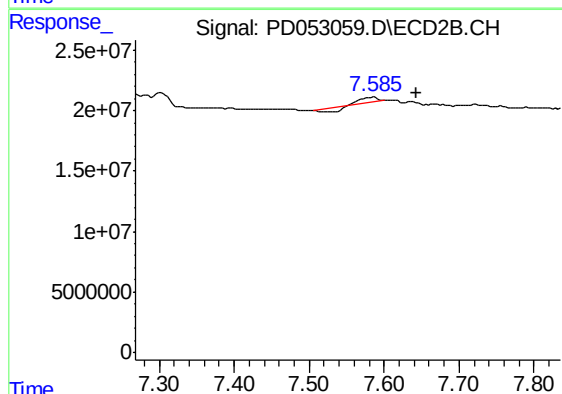


#20 Methoxychlor

R.T.: 7.586 min
Delta R.T.: -0.057 min
Response: 2102194
Conc: 0.21 ng/ml

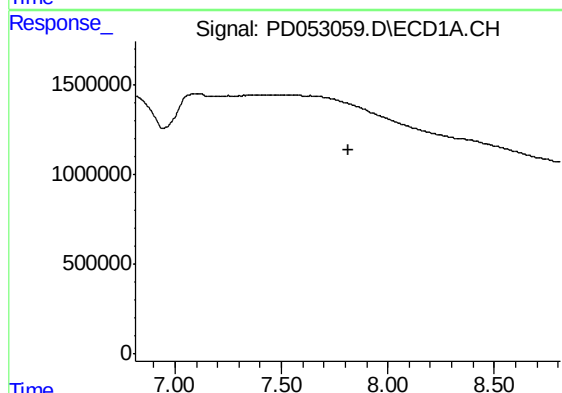

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.813 min
Response: 0
Conc: N.D.

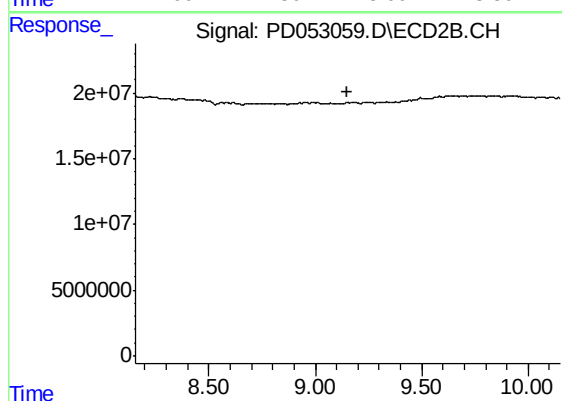

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.153 min
Response: 0
Conc: N.D.