

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
 Data File : PD062331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2021 08:42
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 06:47:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds



Target Compounds						
5) MB	Aldrin	0.000	5.477	0	1884071	0.125 #
8) B	Heptachlo...	0.000	5.849	0	16999162	1.237 #
9) A	Endosulfan I	0.000	6.203	0	331774	0.025 #
10) B	gamma-Chl...	0.000	6.102	0	1313814	0.093 #
15) B	Endosulfa...	0.000	6.894	0	1522428	0.132 #
17) MA	4,4'-DDT	0.000	7.090f	0	11669279	1.170 #
19) B	Endosulfa...	0.000	7.259f	0	837828	0.077 #
21) B	Endrin ke...	0.000	7.720	0	7177295	0.715 #
22)	Mirex	0.000	8.175	0	1159195	0.185 #
23)	Chlordane-1	0.000	4.949f	0	935464	1.895 #
25)	Chlordane-3	0.000	6.102	0	1313814	0.669 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
Data File : PD062331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2021 08:42
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 06:47:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

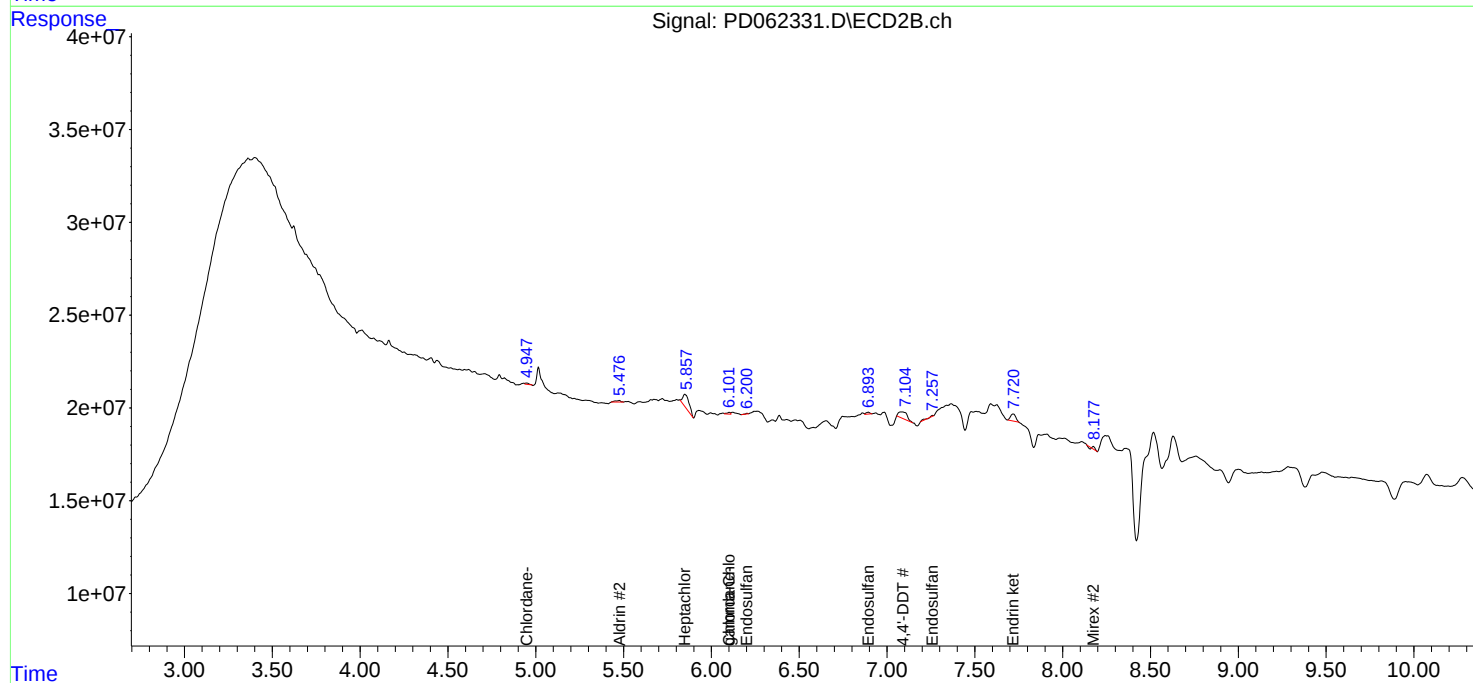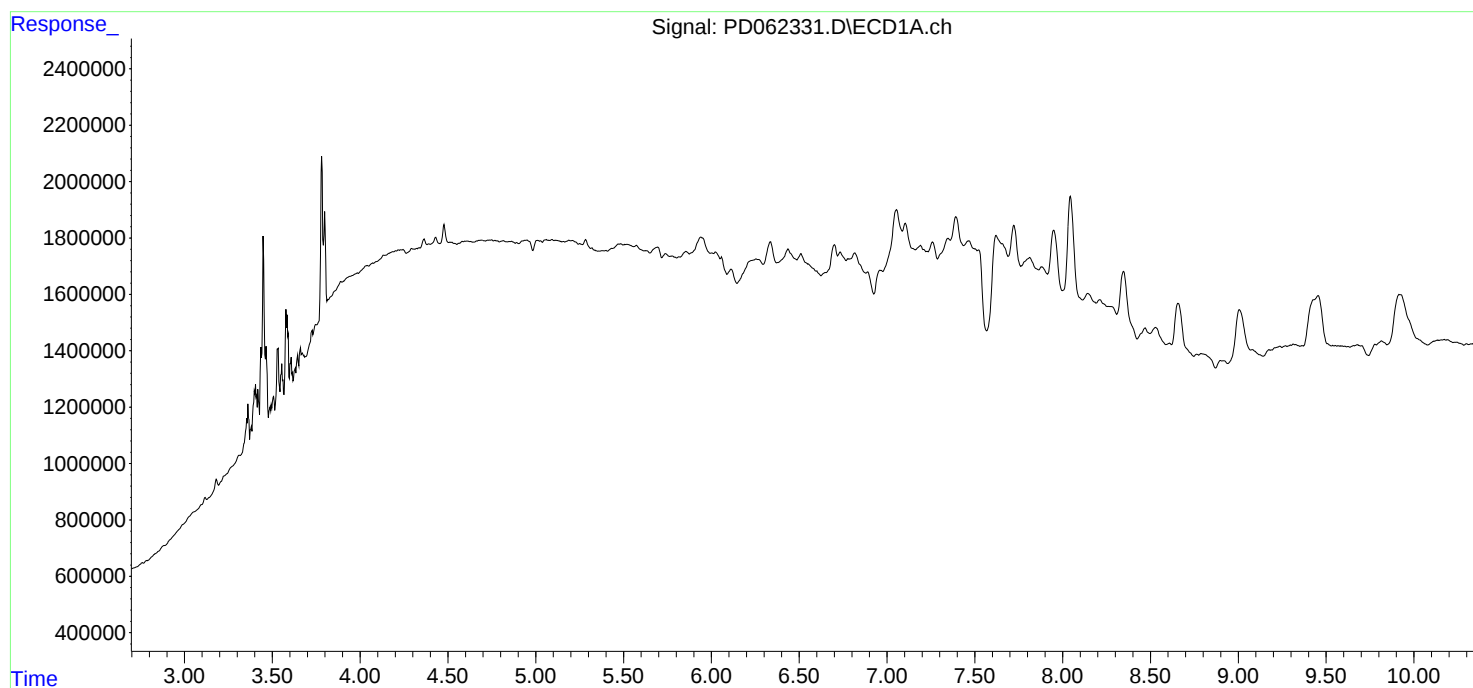

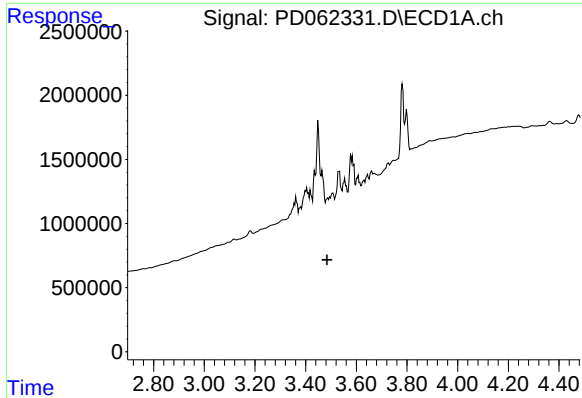


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.485 min
Response: 0
Conc: N.D.

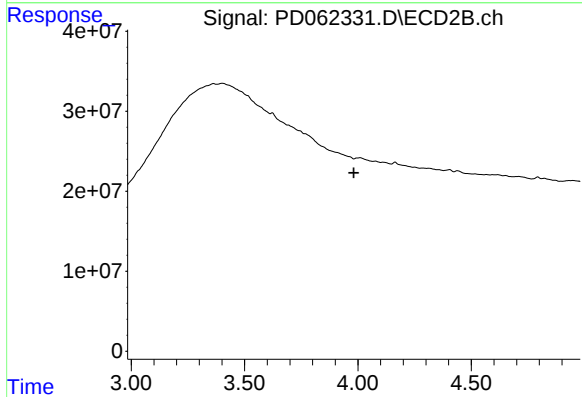


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.981 min
Response: 0
Conc: N.D.

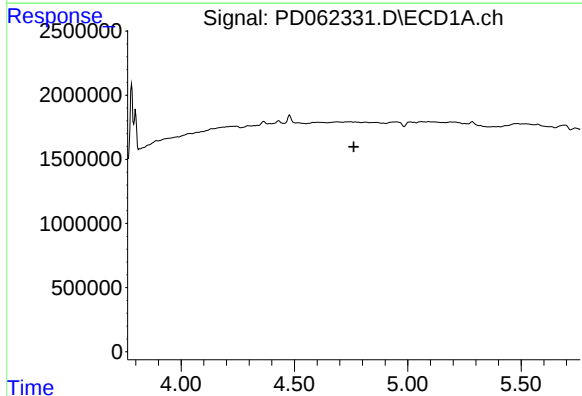


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.762 min
Response: 0
Conc: N.D.

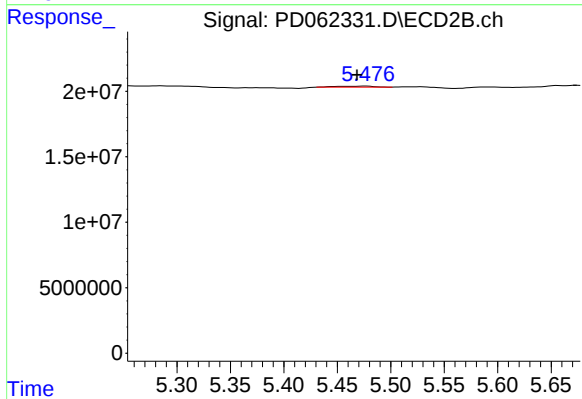


#5 Aldrin

R.T.: 5.477 min
Delta R.T.: 0.009 min
Response: 1884071
Conc: 0.13 ng/ml

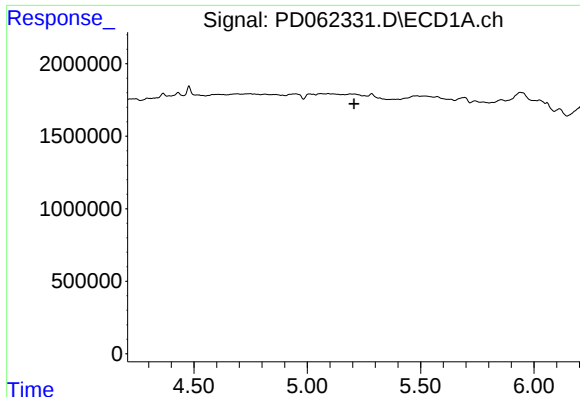


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.206 min
Response: 0
Conc: N.D.

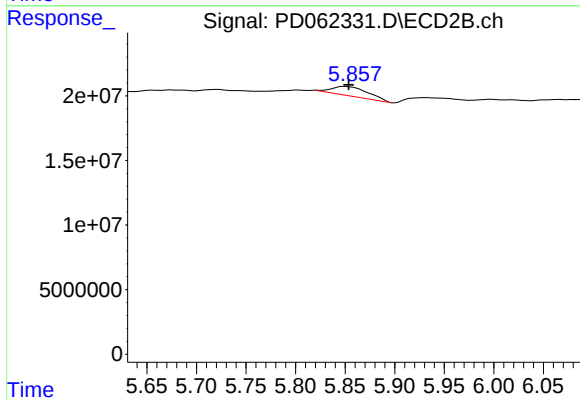


#8 Heptachlor epoxide

R.T.: 5.849 min
Delta R.T.: -0.005 min
Response: 16999162
Conc: 1.24 ng/ml

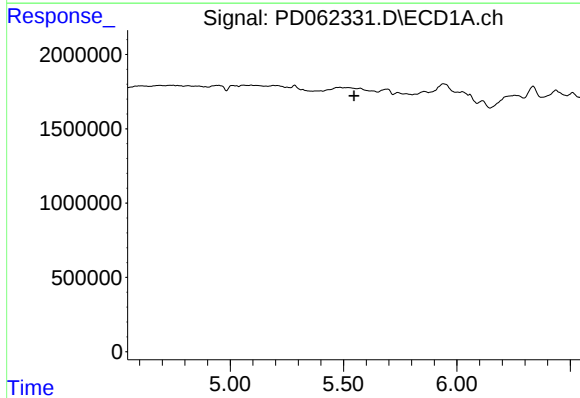


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.547 min
Response: 0
Conc: N.D.

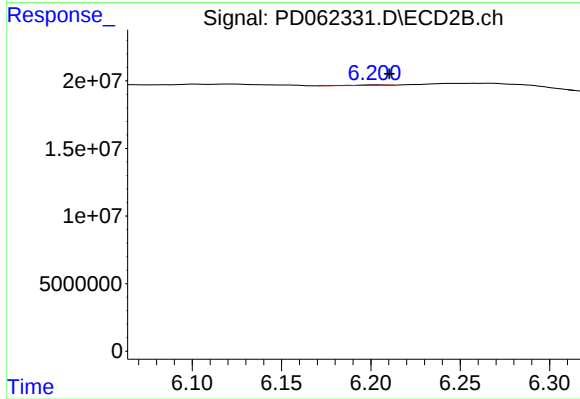


#9 Endosulfan I

R.T.: 6.203 min
Delta R.T.: -0.007 min
Response: 331774
Conc: 0.03 ng/ml

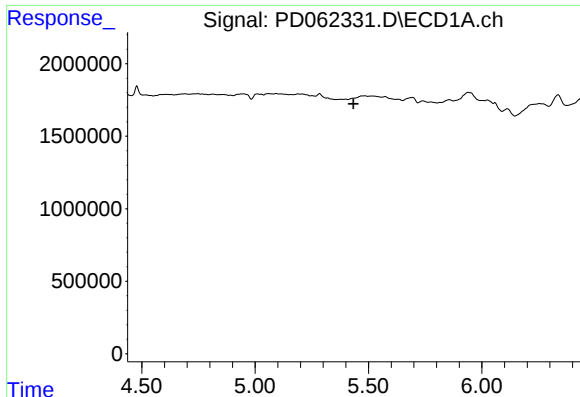


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.434 min
Response: 0
Conc: N.D.

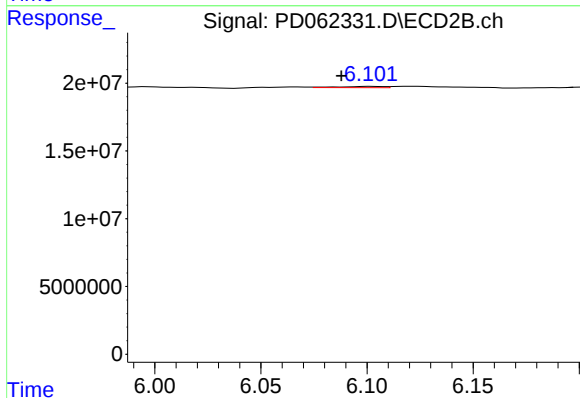


#10 gamma-Chlordane

R.T.: 6.102 min
Delta R.T.: 0.014 min
Response: 1313814
Conc: 0.09 ng/ml

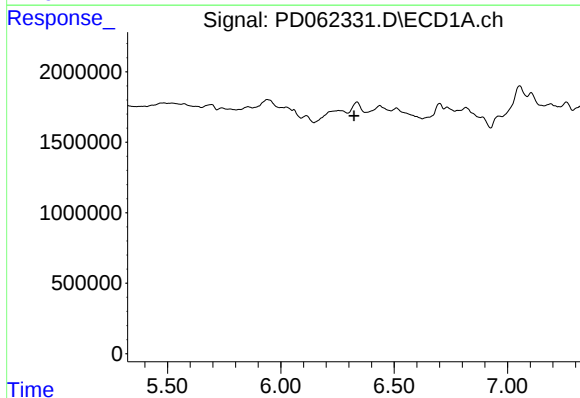


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.323 min
Response: 0
Conc: N.D.

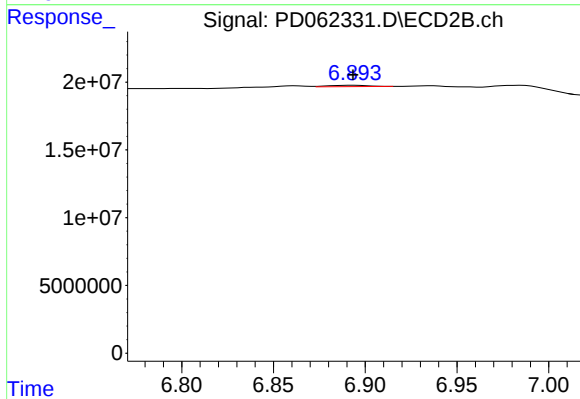


#15 Endosulfan II

R.T.: 6.894 min
Delta R.T.: 0.000 min
Response: 1522428
Conc: 0.13 ng/ml

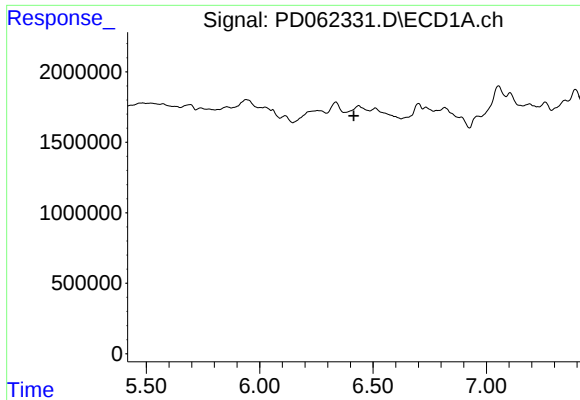


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.415 min
Response: 0
Conc: N.D.

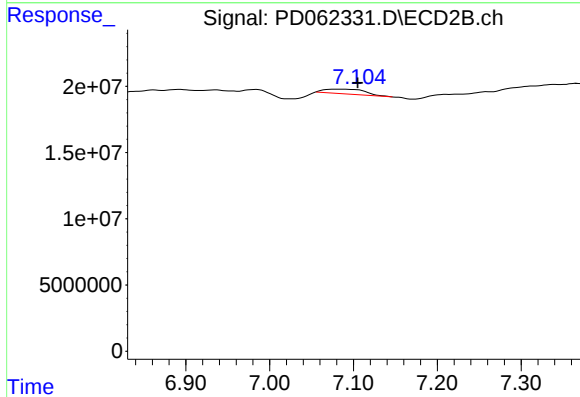


#17 4,4'-DDT

R.T.: 7.090 min
Delta R.T.: -0.016 min
Response: 11669279
Conc: 1.17 ng/ml

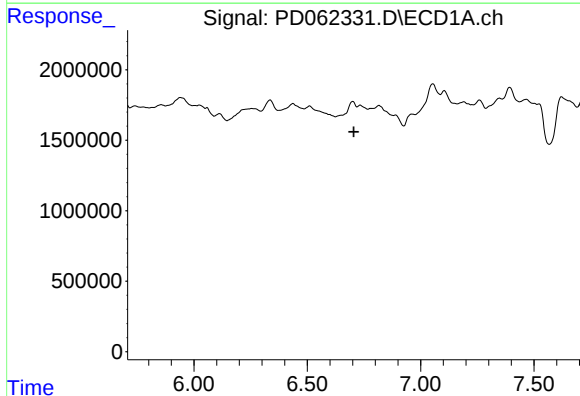


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.705 min
Response: 0
Conc: N.D.

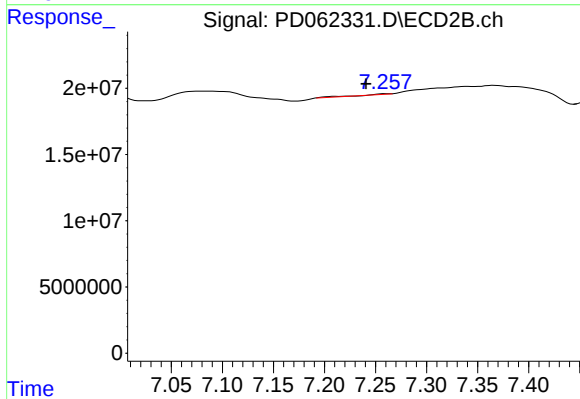


#19 Endosulfan Sulfate

R.T.: 7.259 min
Delta R.T.: 0.019 min
Response: 837828
Conc: 0.08 ng/ml

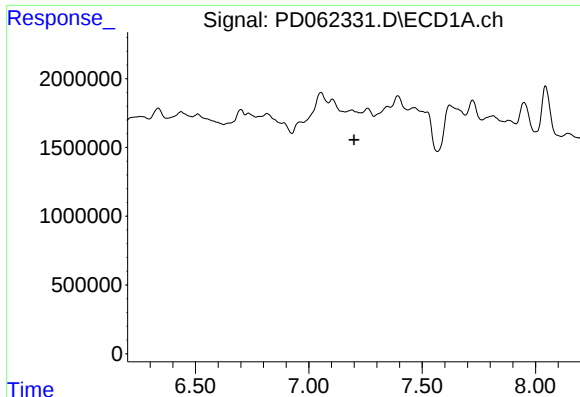


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

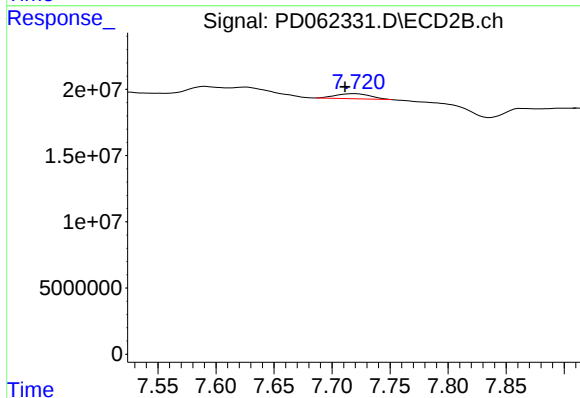


#21 Endrin ketone

R.T.: 7.720 min
Delta R.T.: 0.008 min
Response: 7177295
Conc: 0.72 ng/ml

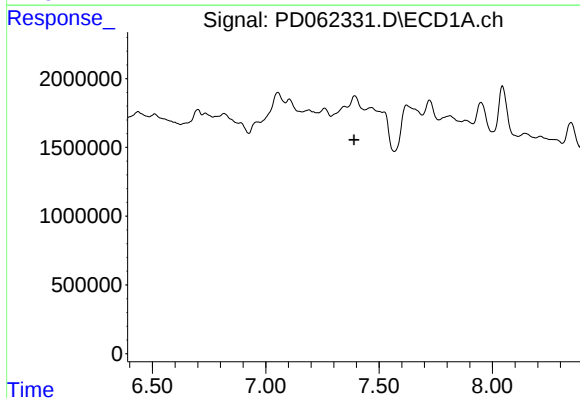


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.390 min
Response: 0
Conc: N.D.

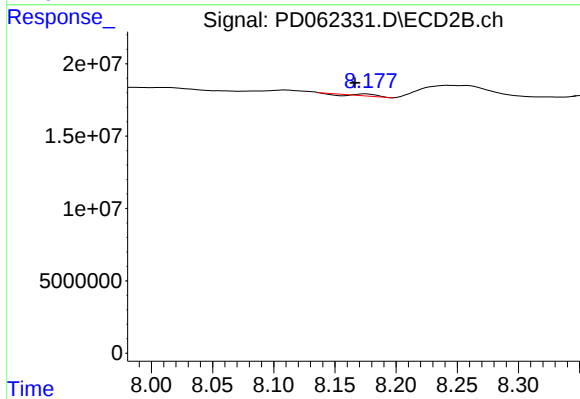


#22 Mirex

R.T.: 8.175 min
Delta R.T.: 0.008 min
Response: 1159195
Conc: 0.19 ng/ml

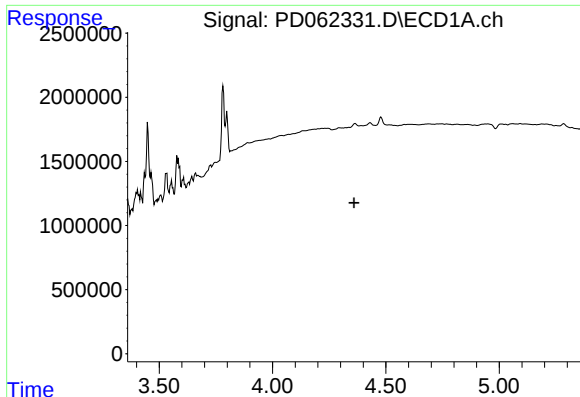


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.360 min
Response: 0
Conc: N.D.

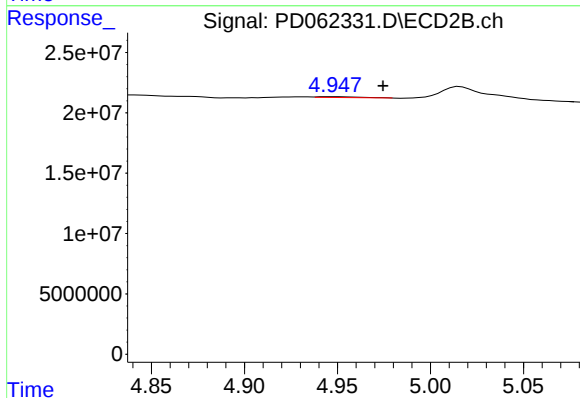


#23 Chlordane-1

R.T.: 4.949 min
Delta R.T.: -0.026 min
Response: 935464
Conc: 1.89 ng/ml

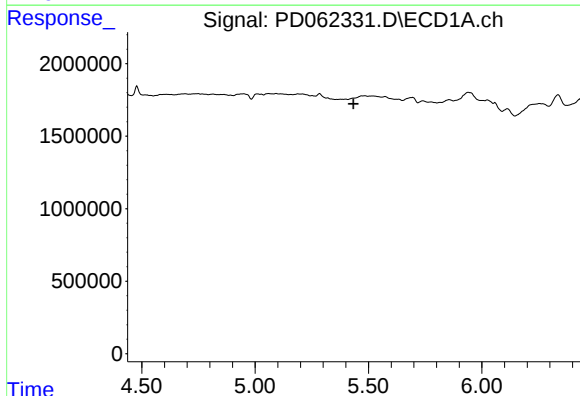


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.434 min
Response: 0
Conc: N.D.

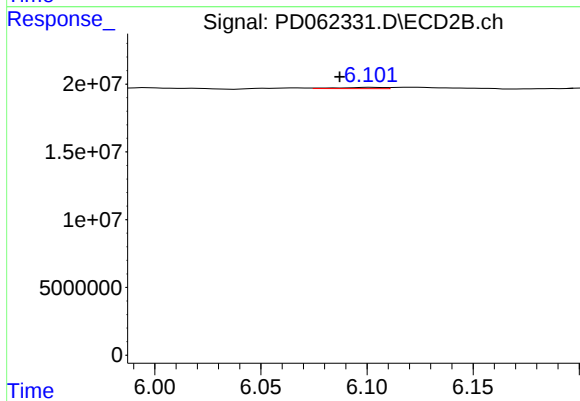


#25 Chlordane-3

R.T.: 6.102 min
Delta R.T.: 0.015 min
Response: 1313814
Conc: 0.67 ng/ml

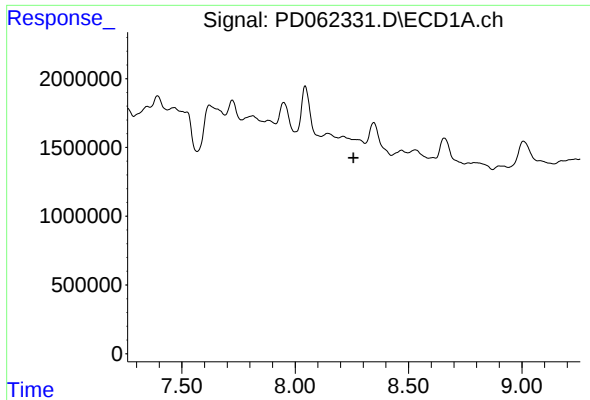

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.258 min
Response: 0
Conc: N.D.

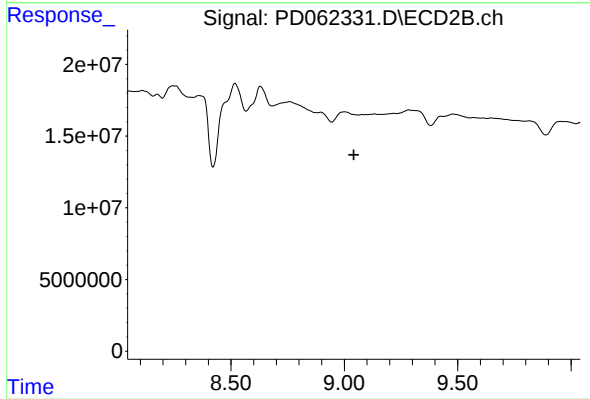

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.042 min
Response: 0
Conc: N.D.