

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
 Data File : PD062353.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2021 13:52
 Operator : AR\AJ
 Sample : M2107-22
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 06:52:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.981	8727834	110.8E6	10.716	10.517
28)	SA Decachlor...	8.255	9.041	35907725	276.4E6	29.602	32.572
Target Compounds							
5)	MB Aldrin	4.746f	5.478	19024591	74963059	15.201	4.987 #
6)	B beta-BHC	4.430f	0.000	2610527	0	4.336	N.D. #
8)	B Heptachlo...	5.225f	0.000	3315508	0	2.700	N.D. #
9)	A Endosulfan I	0.000	6.236f	0	17815632	N.D.	1.360 #
15)	B Endosulfa...	0.000	6.884	0	6178056	N.D.	0.537 #
16)	A 4,4'-DDD	0.000	6.810	0	15518345	N.D.	1.393 #
17)	MA 4,4'-DDT	0.000	7.127f	0	4778419	N.D.	0.479 #
19)	B Endosulfa...	6.696	0.000	1281335	0	1.085	N.D. #
21)	B Endrin ke...	7.222f	0.000	934209	0	0.767	N.D. #
22)	Mirex	7.386	8.188f	2569403	31500985	2.570	5.040 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
Data File : PD062353.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2021 13:52
Operator : AR\AJ
Sample : M2107-22
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 06:52:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

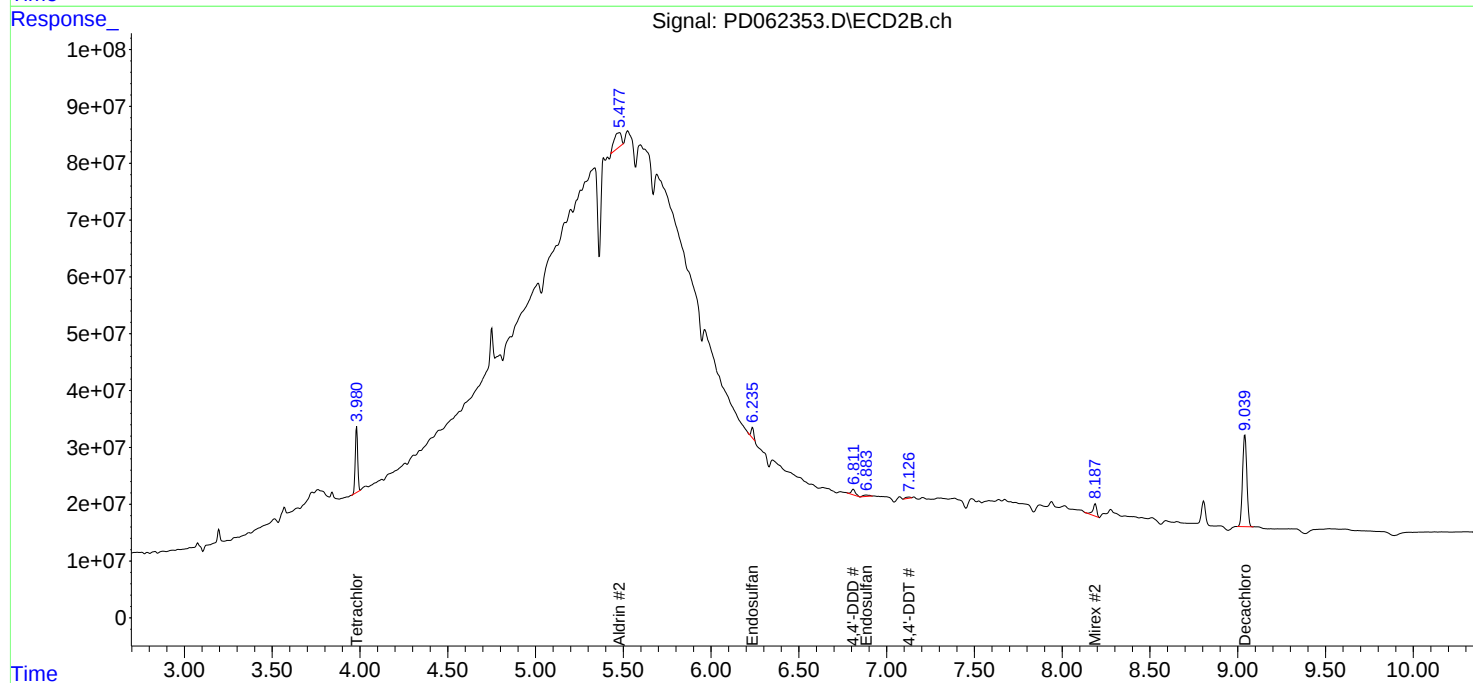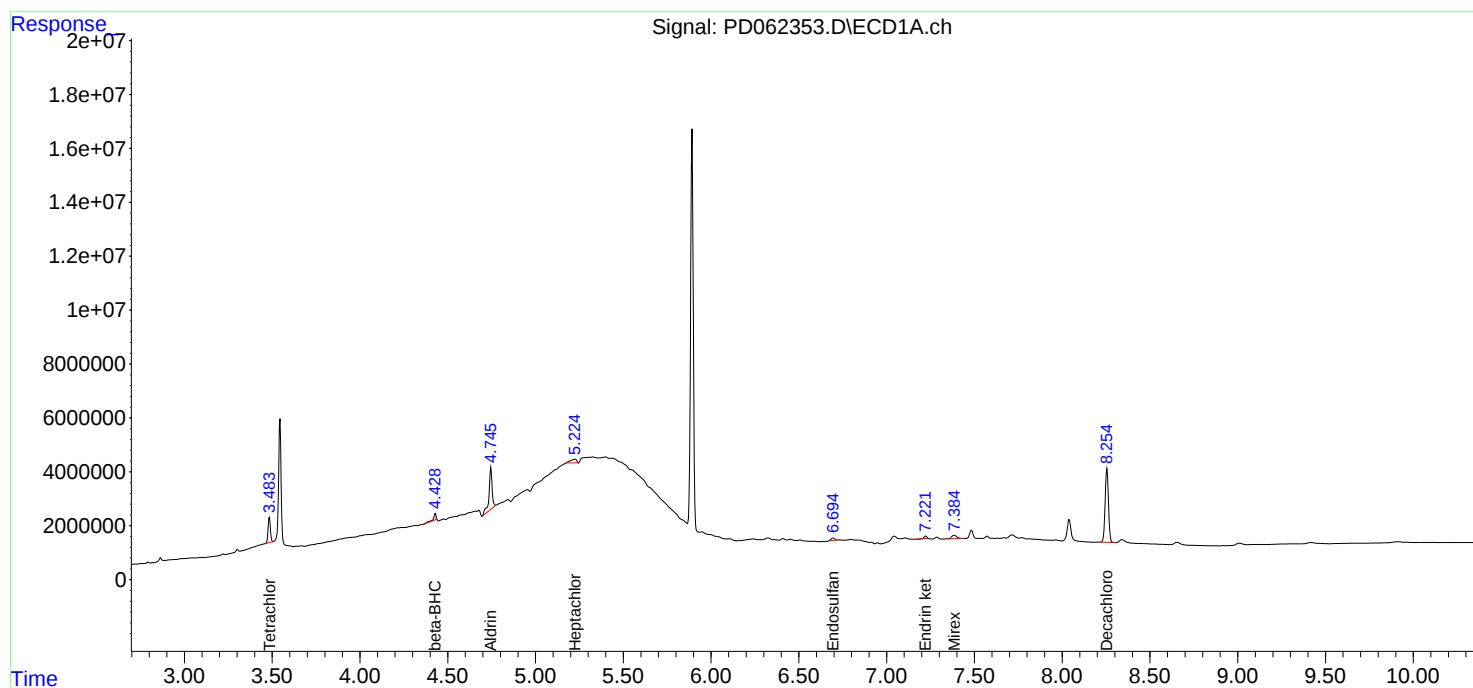

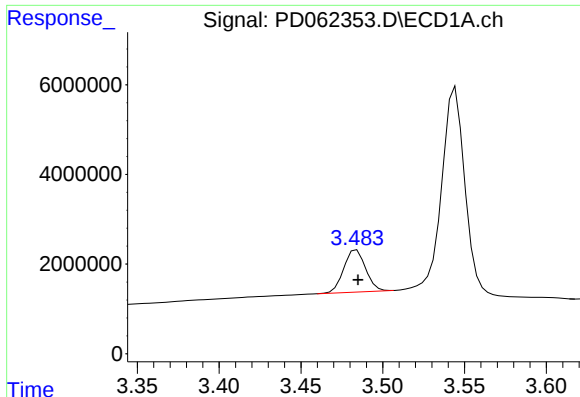


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 8727834
Conc: 10.72 ng/ml

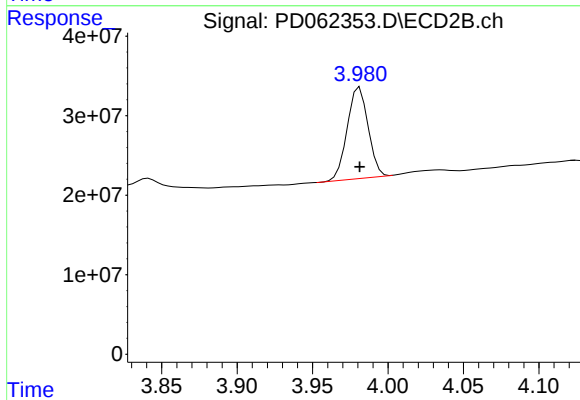


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 110762525
Conc: 10.52 ng/ml

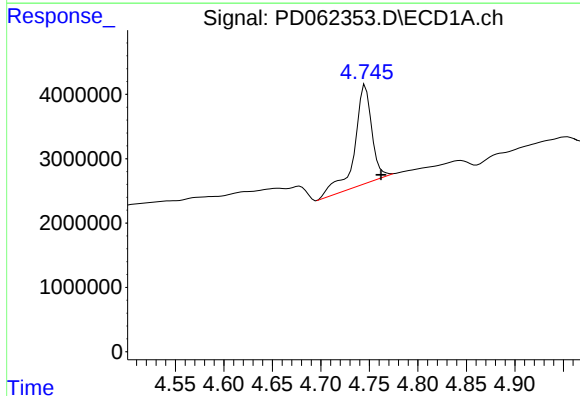


#5 Aldrin

R.T.: 4.746 min
Delta R.T.: -0.016 min
Response: 19024591
Conc: 15.20 ng/ml

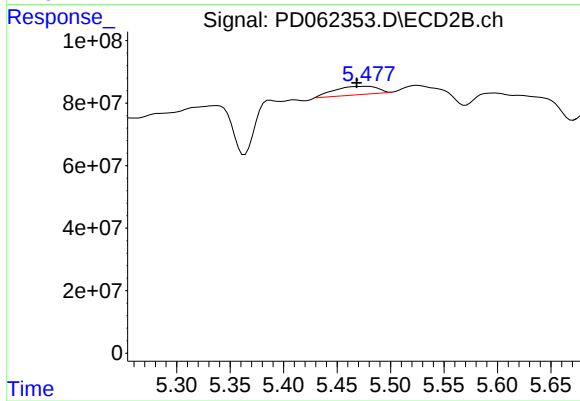


#5 Aldrin

R.T.: 5.478 min
Delta R.T.: 0.010 min
Response: 74963059
Conc: 4.99 ng/ml

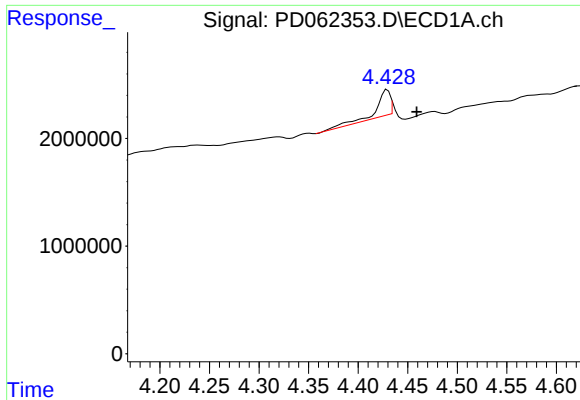


#6 beta-BHC

R.T.: 4.430 min
Delta R.T.: -0.030 min
Response: 2610527
Conc: 4.34 ng/ml

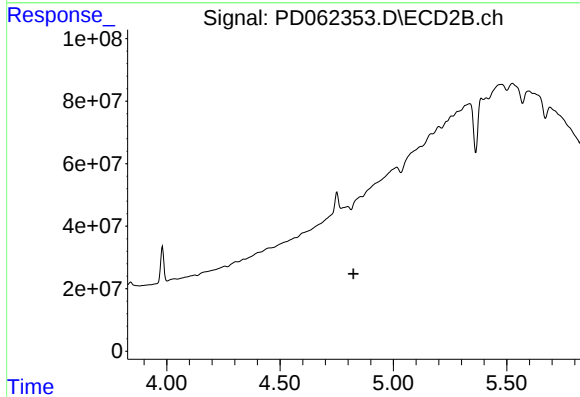


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.824 min
Response: 0
Conc: N.D.

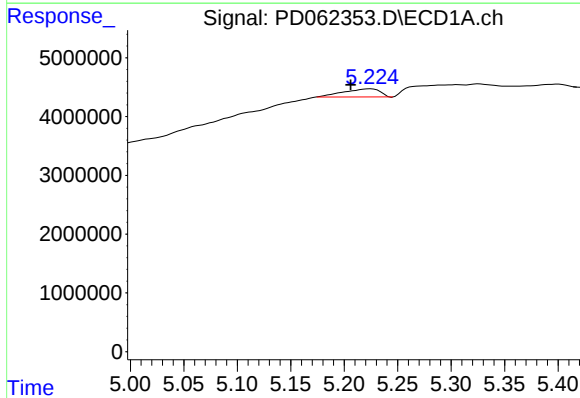


#8 Heptachlor epoxide

R.T.: 5.225 min
Delta R.T.: 0.019 min
Response: 3315508
Conc: 2.70 ng/ml

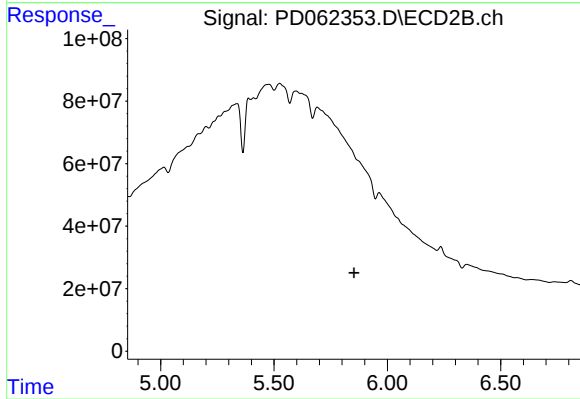


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.854 min
Response: 0
Conc: N.D.

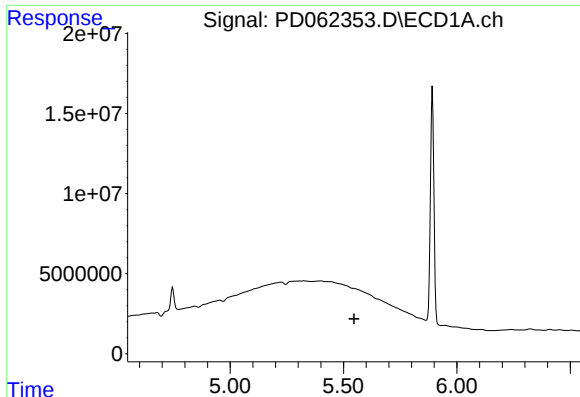


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.547 min
Response: 0
Conc: N.D.

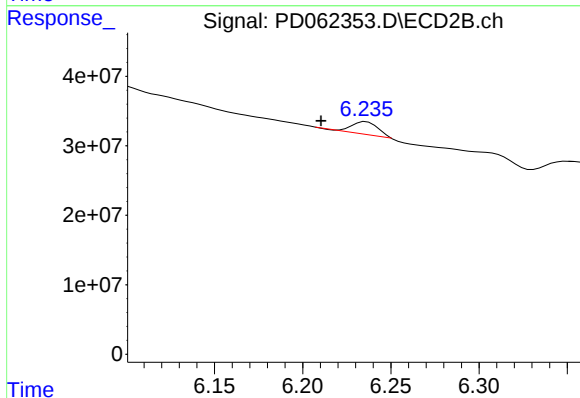


#9 Endosulfan I

R.T.: 6.236 min
Delta R.T.: 0.026 min
Response: 17815632
Conc: 1.36 ng/ml

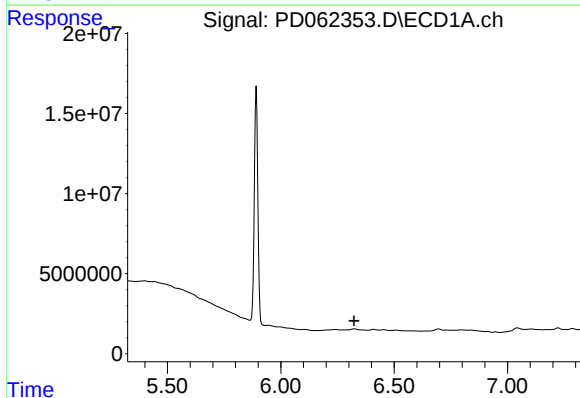


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.323 min
Response: 0
Conc: N.D.

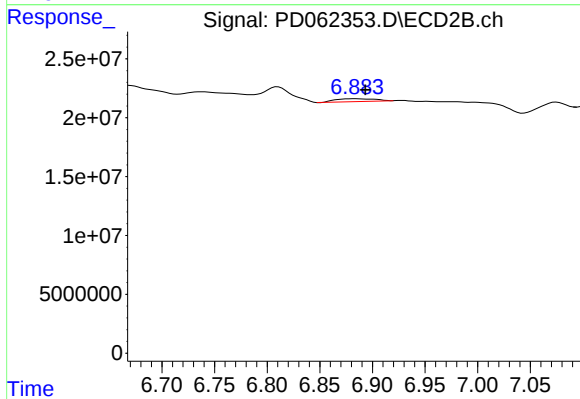


#15 Endosulfan II

R.T.: 6.884 min
Delta R.T.: -0.009 min
Response: 6178056
Conc: 0.54 ng/ml

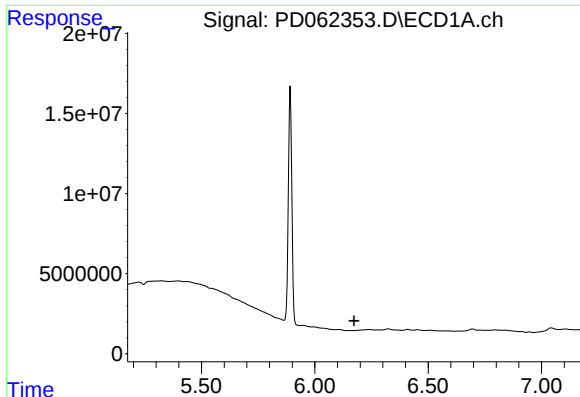


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.173 min
Response: 0
Conc: N.D.

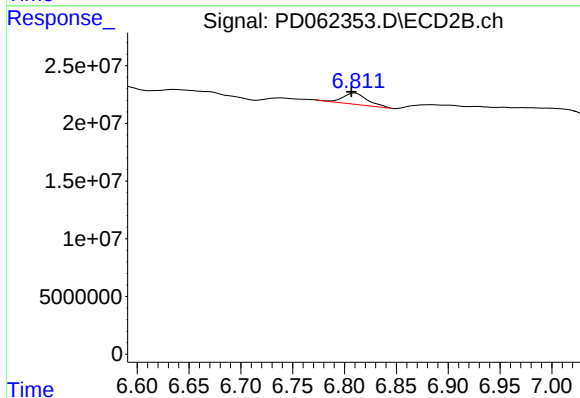


#16 4,4'-DDD

R.T.: 6.810 min
Delta R.T.: 0.004 min
Response: 15518345
Conc: 1.39 ng/ml

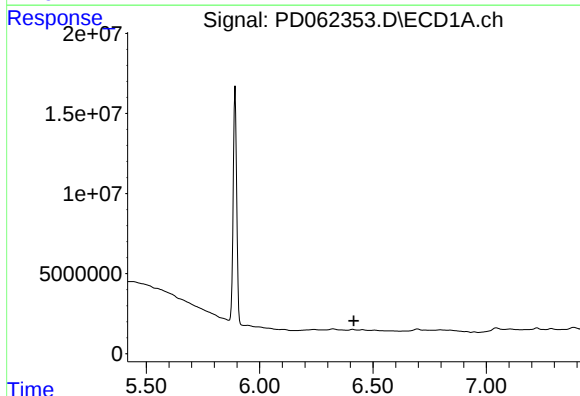


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.415 min
Response: 0
Conc: N.D.

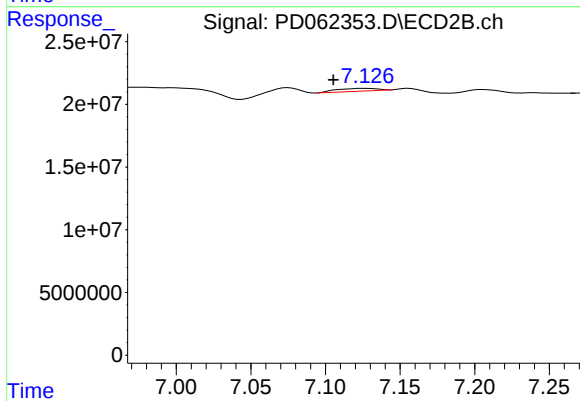


#17 4,4'-DDT

R.T.: 7.127 min
Delta R.T.: 0.021 min
Response: 4778419
Conc: 0.48 ng/ml

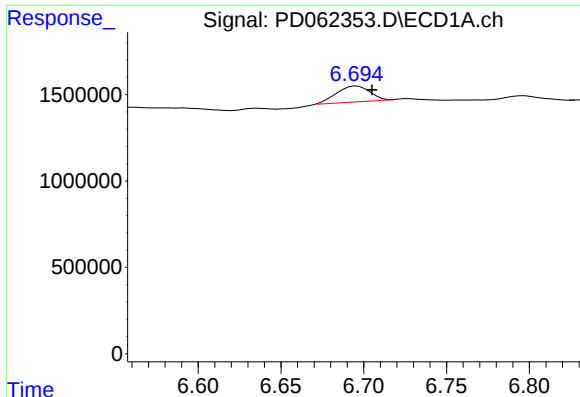


#19 Endosulfan Sulfate

R.T.: 6.696 min
Delta R.T.: -0.009 min
Response: 1281335
Conc: 1.09 ng/ml

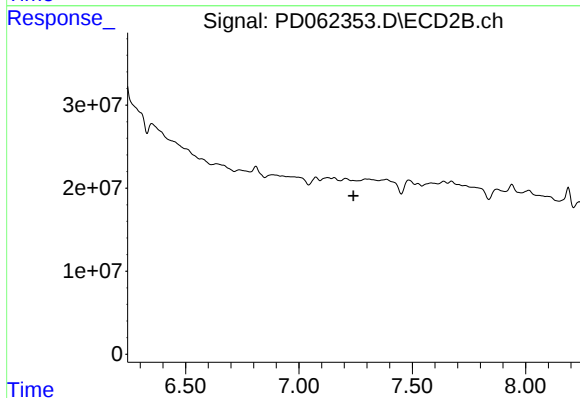


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 7.241 min
Response: 0
Conc: N.D.

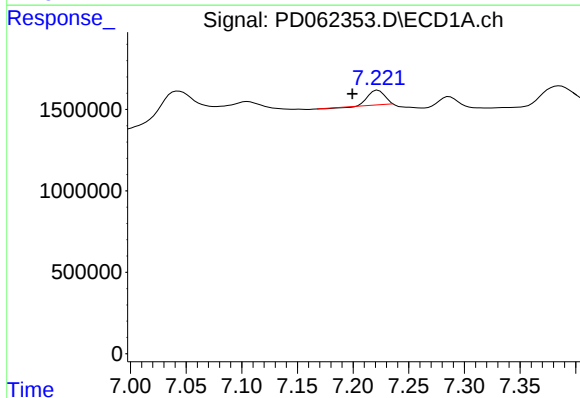


#21 Endrin ketone

R.T.: 7.222 min
Delta R.T.: 0.023 min
Response: 934209
Conc: 0.77 ng/ml

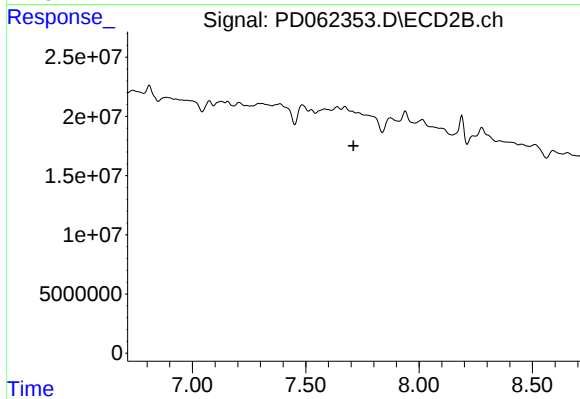


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.711 min
Response: 0
Conc: N.D.

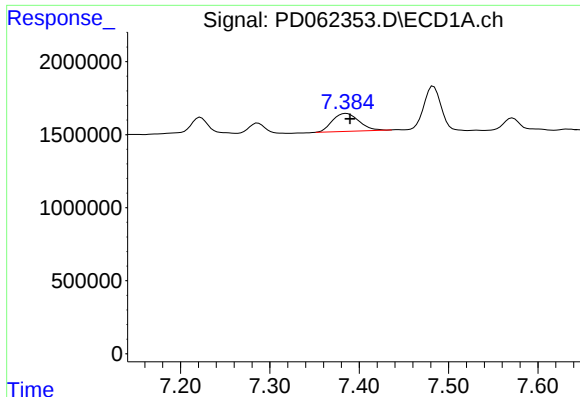


#22 Mirex

R.T.: 7.386 min
Delta R.T.: -0.004 min
Response: 2569403
Conc: 2.57 ng/ml

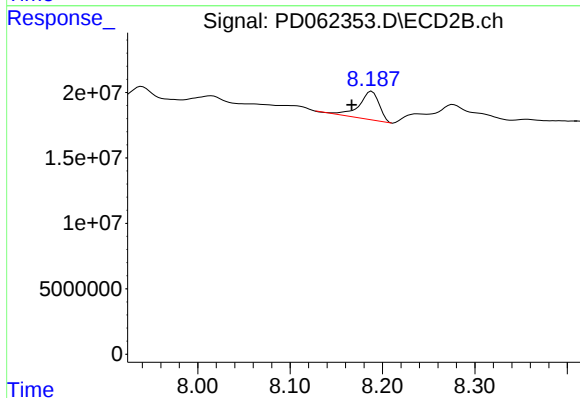


#22 Mirex

R.T.: 8.188 min
Delta R.T.: 0.022 min
Response: 31500985
Conc: 5.04 ng/ml

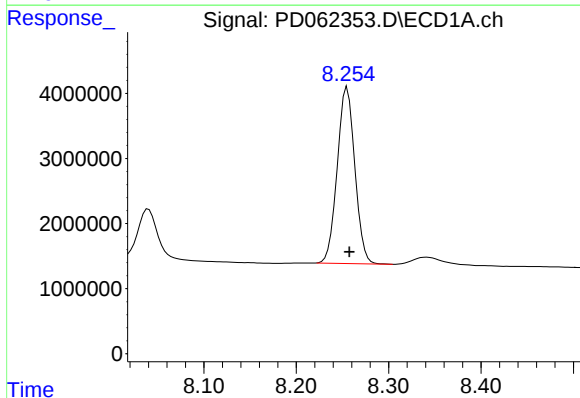

#28 Decachlorobiphenyl

R.T.: 8.255 min
Delta R.T.: -0.002 min
Response: 35907725
Conc: 29.60 ng/ml

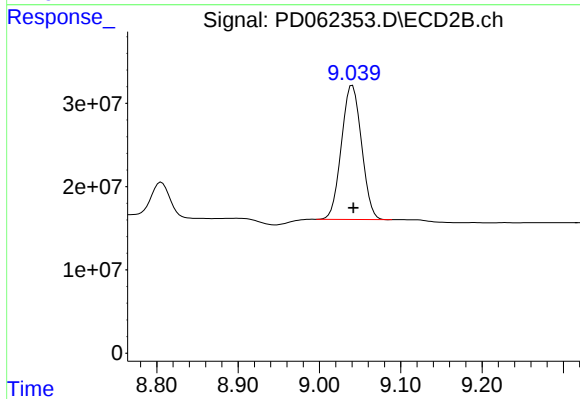

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: -0.001 min
Response: 276373064
Conc: 32.57 ng/ml