

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
 Data File : PD062354.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2021 14:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 06:52:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.981	17281408	222.6E6	21.218	21.136
28)	SA Decachlor...	8.255	9.041	24035572	180.6E6	19.815	21.284
Target Compounds							
3)	MA gamma-BHC...	0.000	4.656	0	638654	N.D.	0.041 #
8)	B Heptachlo...	0.000	5.860	0	15586676	N.D.	1.135 #
9)	A Endosulfan I	0.000	6.202	0	307096	N.D.	0.023 #
11)	B alpha-Chl...	0.000	6.163	0	137895	N.D.	0.010 #
15)	B Endosulfa...	0.000	6.906	0	1595565	N.D.	0.139 #
17)	MA 4,4'-DDT	0.000	7.111	0	845851	N.D.	0.085 #
20)	A Methoxychlor	0.000	7.562	0	389863	N.D.	0.080 #
21)	B Endrin ke...	0.000	7.732f	0	2521124	N.D.	0.251 #
23)	Chlordane-1	0.000	4.961	0	84687	N.D.	0.172 #
26)	Chlordane-4	0.000	6.163	0	137895	N.D.	0.061 #
27)	Chlordane-5	0.000	6.954	0	330046	N.D.	0.802 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
Data File : PD062354.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2021 14:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 06:52:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

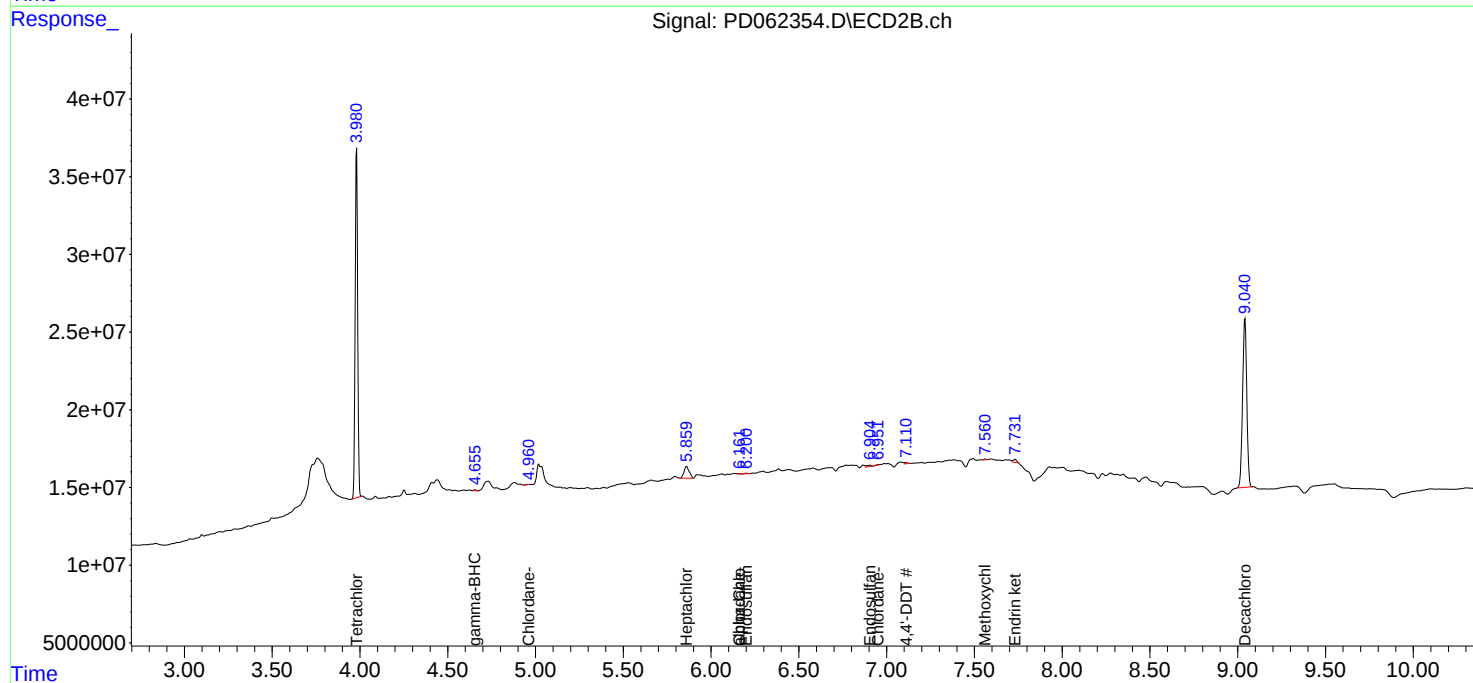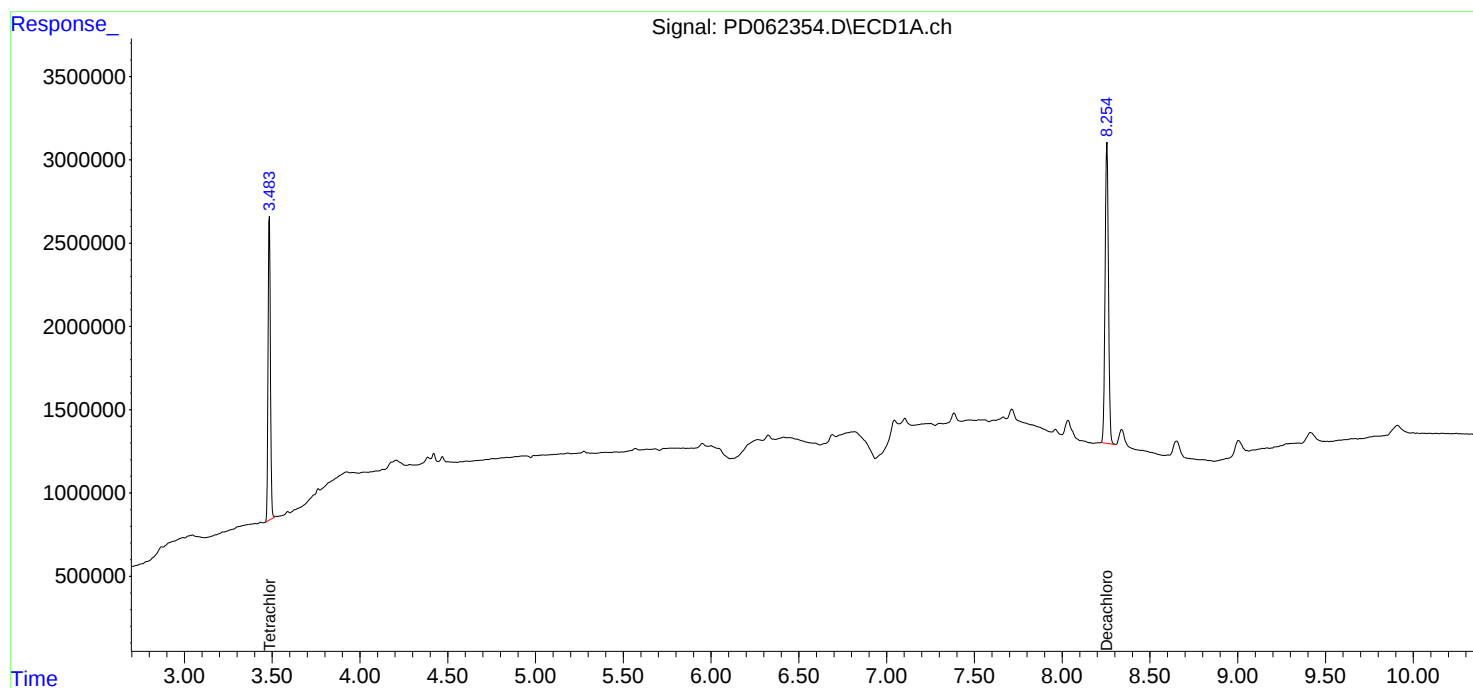

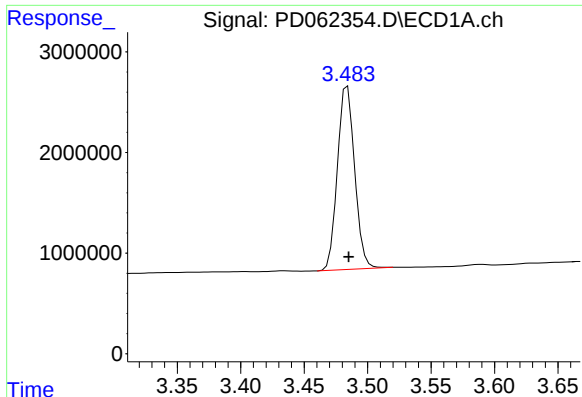


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 17281408
Conc: 21.22 ng/ml

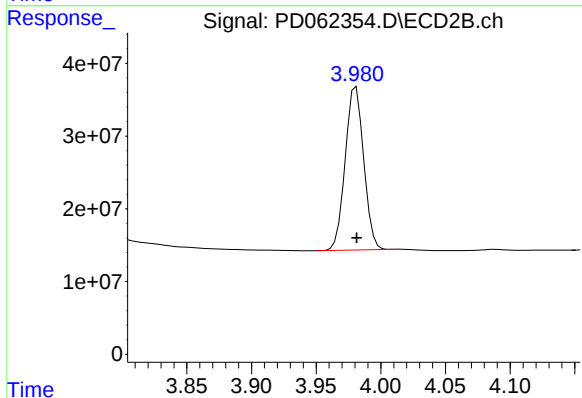


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 222588533
Conc: 21.14 ng/ml

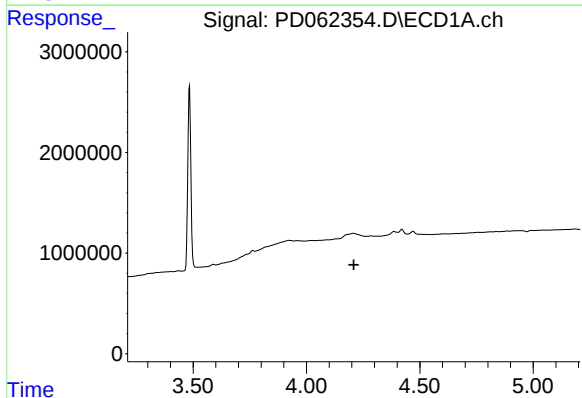


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.209 min
Response: 0
Conc: N.D.

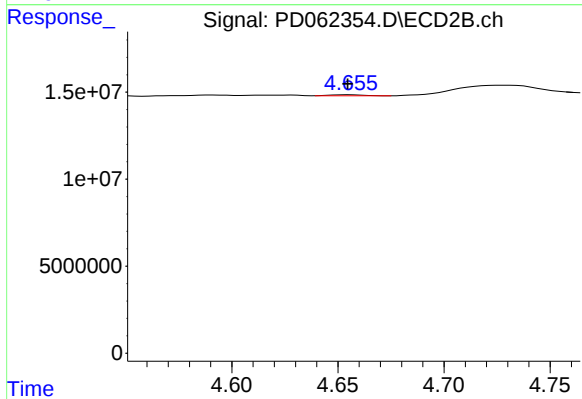


#3 gamma-BHC (Lindane)

R.T.: 4.656 min
Delta R.T.: 0.001 min
Response: 638654
Conc: 0.04 ng/ml

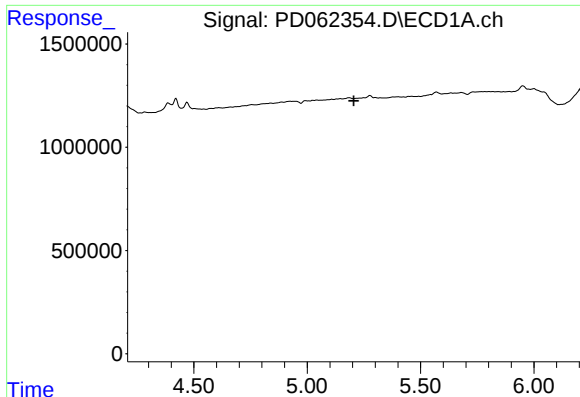


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.206 min
Response: 0
Conc: N.D.

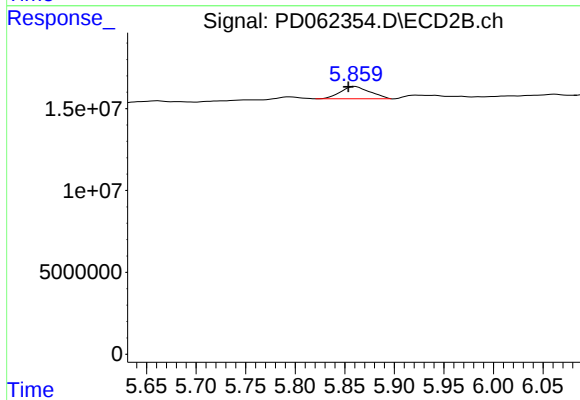


#8 Heptachlor epoxide

R.T.: 5.860 min
Delta R.T.: 0.006 min
Response: 15586676
Conc: 1.13 ng/ml

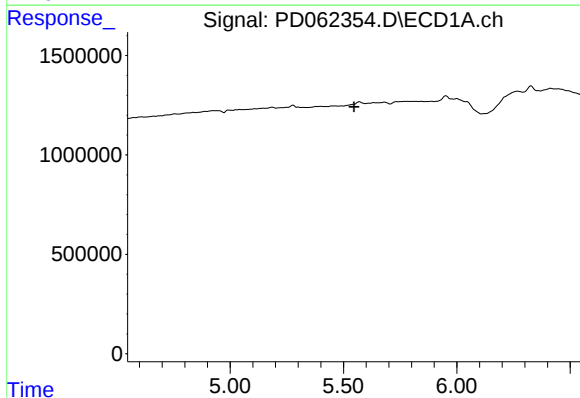


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.547 min
Response: 0
Conc: N.D.

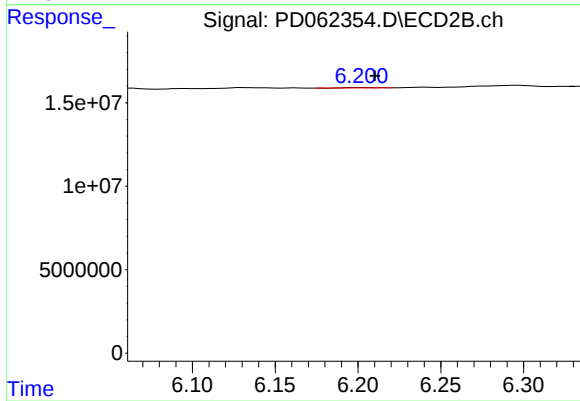


#9 Endosulfan I

R.T.: 6.202 min
Delta R.T.: -0.009 min
Response: 307096
Conc: 0.02 ng/ml

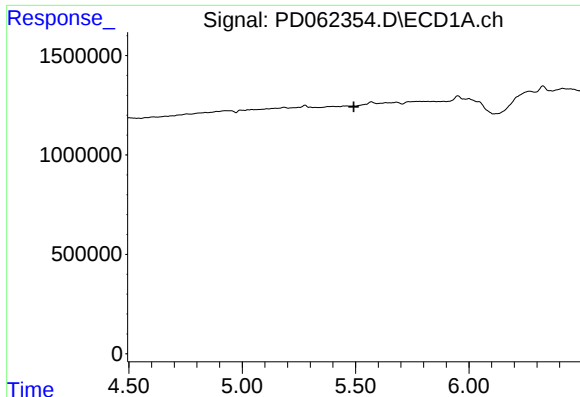


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.492 min
Response: 0
Conc: N.D.

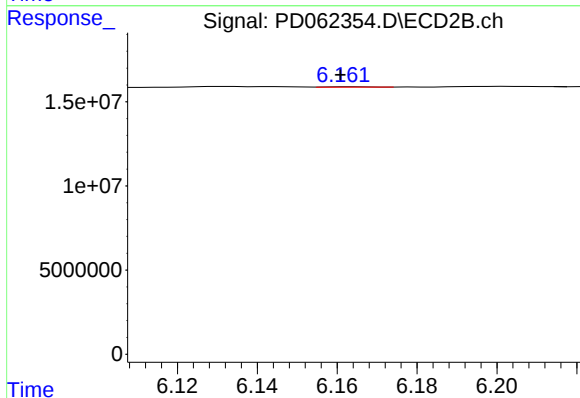


#11 alpha-Chlordane

R.T.: 6.163 min
Delta R.T.: 0.002 min
Response: 137895
Conc: 0.01 ng/ml

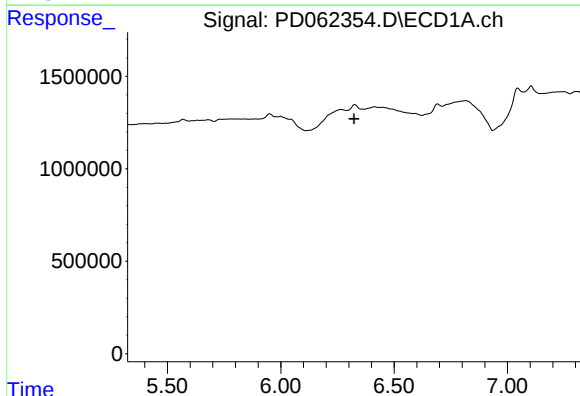


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.323 min
Response: 0
Conc: N.D.

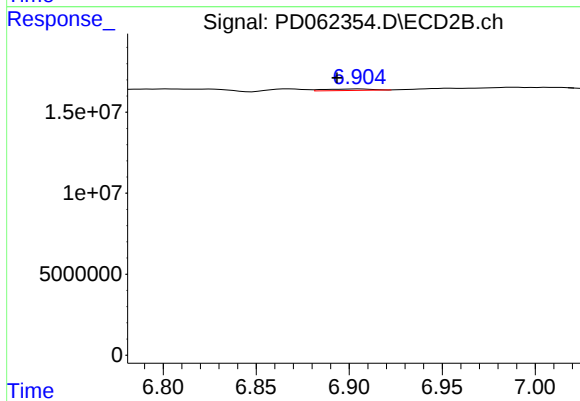


#15 Endosulfan II

R.T.: 6.906 min
Delta R.T.: 0.012 min
Response: 1595565
Conc: 0.14 ng/ml

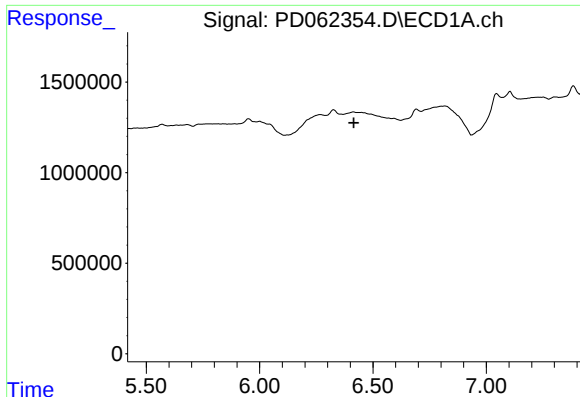


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.415 min
Response: 0
Conc: N.D.

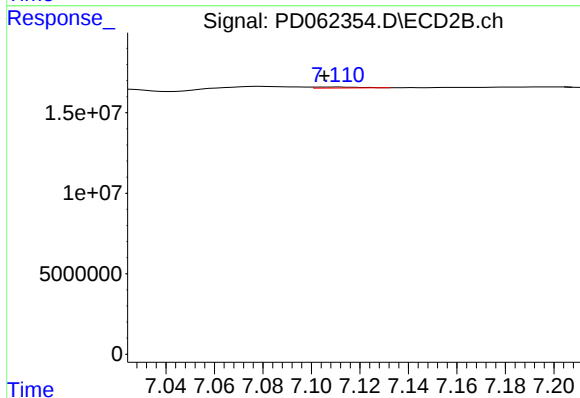


#17 4,4'-DDT

R.T.: 7.111 min
Delta R.T.: 0.006 min
Response: 845851
Conc: 0.08 ng/ml

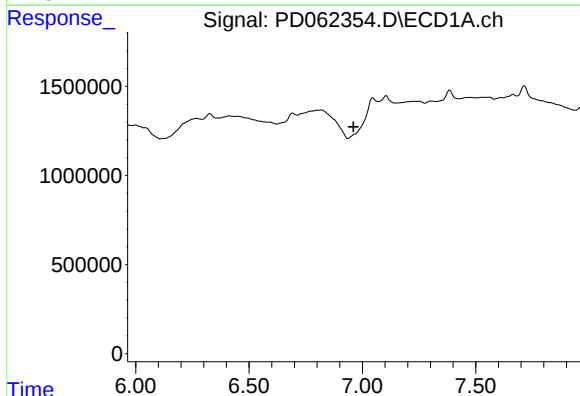


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.962 min
Response: 0
Conc: N.D.

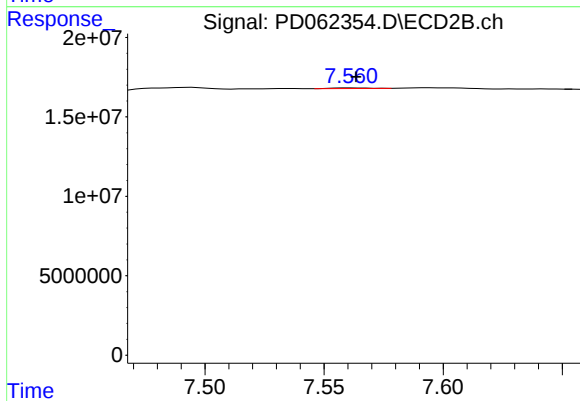


#20 Methoxychlor

R.T.: 7.562 min
Delta R.T.: -0.002 min
Response: 389863
Conc: 0.08 ng/ml

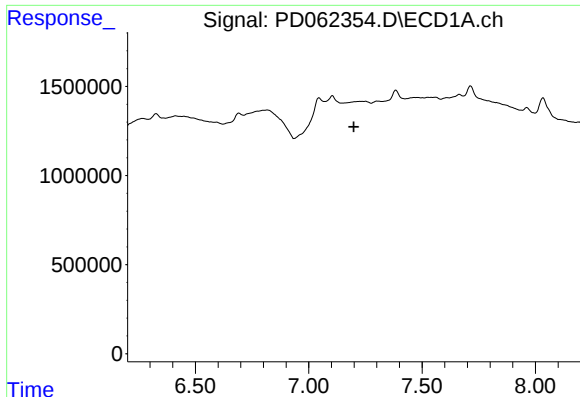


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

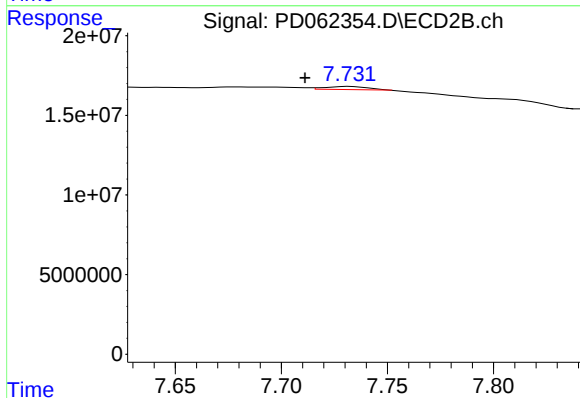


#21 Endrin ketone

R.T.: 7.732 min
Delta R.T.: 0.021 min
Response: 2521124
Conc: 0.25 ng/ml

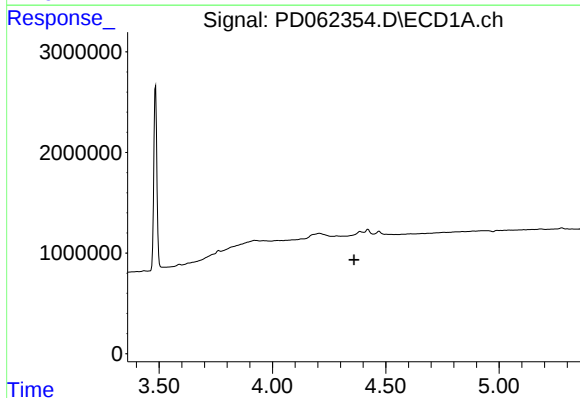


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.360 min
Response: 0
Conc: N.D.

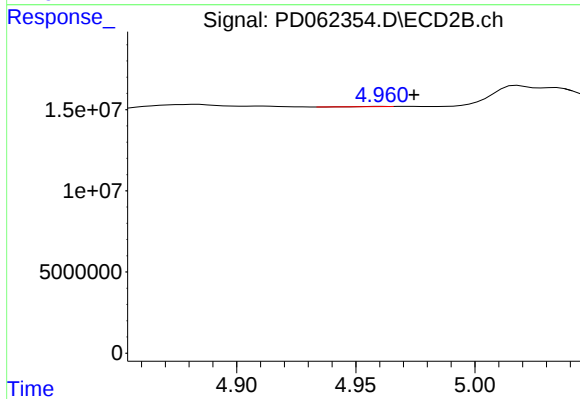


#23 Chlordane-1

R.T.: 4.961 min
Delta R.T.: -0.014 min
Response: 84687
Conc: 0.17 ng/ml

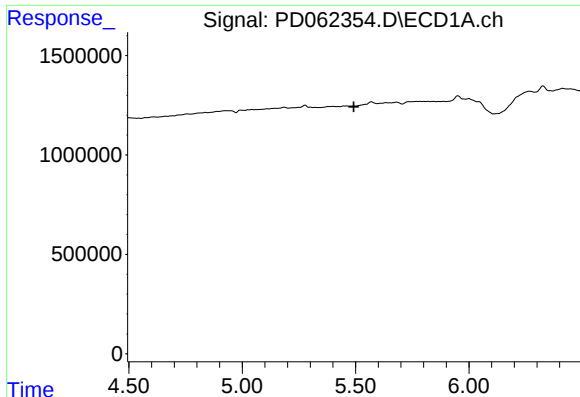


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.493 min
Response: 0
Conc: N.D.

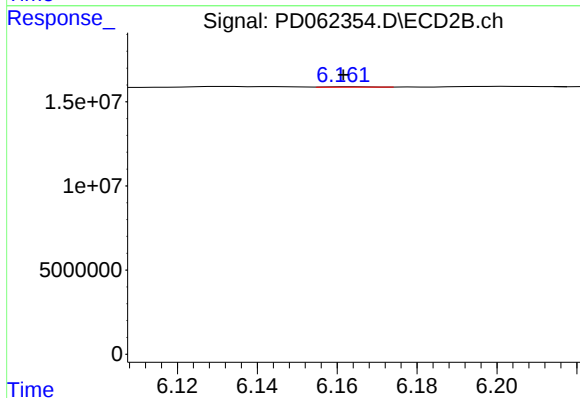


#26 Chlordane-4

R.T.: 6.163 min
Delta R.T.: 0.001 min
Response: 137895
Conc: 0.06 ng/ml

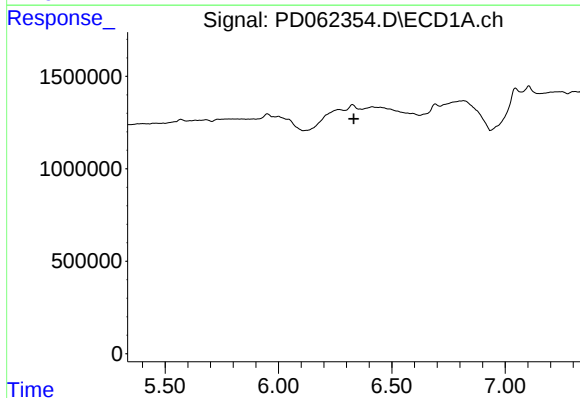


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.333 min
Response: 0
Conc: N.D.

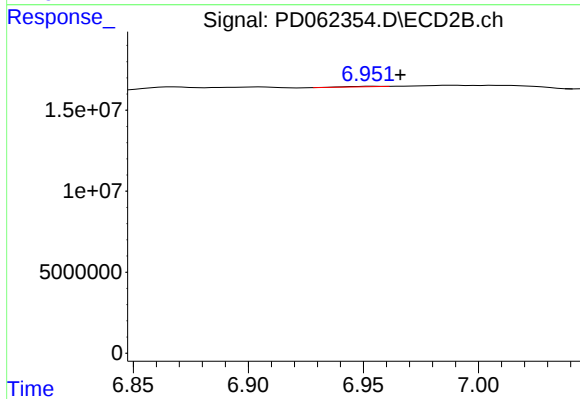


#27 Chlordane-5

R.T.: 6.954 min
Delta R.T.: -0.012 min
Response: 330046
Conc: 0.80 ng/ml

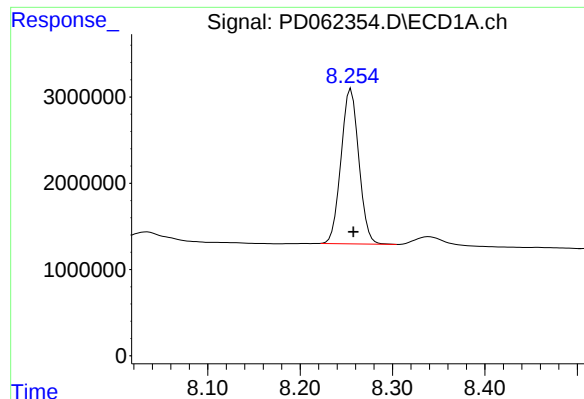

#28 Decachlorobiphenyl

R.T.: 8.255 min
Delta R.T.: -0.002 min
Response: 24035572
Conc: 19.81 ng/ml

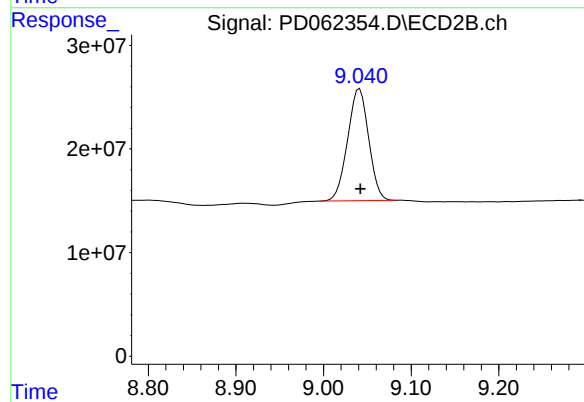

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 180591167
Conc: 21.28 ng/ml