

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
 Data File : PD062362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2021 16:11
 Operator : AR\AJ
 Sample : M2132-06
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 06:54:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.981	11849884	145.0E6	14.549	13.770
28)	SA Decachlor...	8.256	9.041	14229567	106.5E6	11.731	12.547
Target Compounds							
5)	MB Aldrin	4.746f	5.487f	4210352	873058	3.364	0.058 #
9)	A Endosulfan I	0.000	6.236f	0	6122910	N.D.	0.468 #
12)	B 4,4'-DDE	0.000	6.313	0	1768231	N.D.	0.125 #
14)	MA Endrin	0.000	6.703f	0	666053	N.D.	0.055 #
16)	A 4,4'-DDD	0.000	6.810	0	3022073	N.D.	0.271 #
17)	MA 4,4'-DDT	0.000	7.113	0	317631	N.D.	0.032 #
19)	B Endosulfa...	0.000	7.263f	0	231858	N.D.	0.021 #
21)	B Endrin ke...	0.000	7.737f	0	359734	N.D.	0.036 #
22)	Mirex	0.000	8.142f	0	2529230	N.D.	0.405 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
Data File : PD062362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2021 16:11
Operator : AR\AJ
Sample : M2132-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 06:54:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

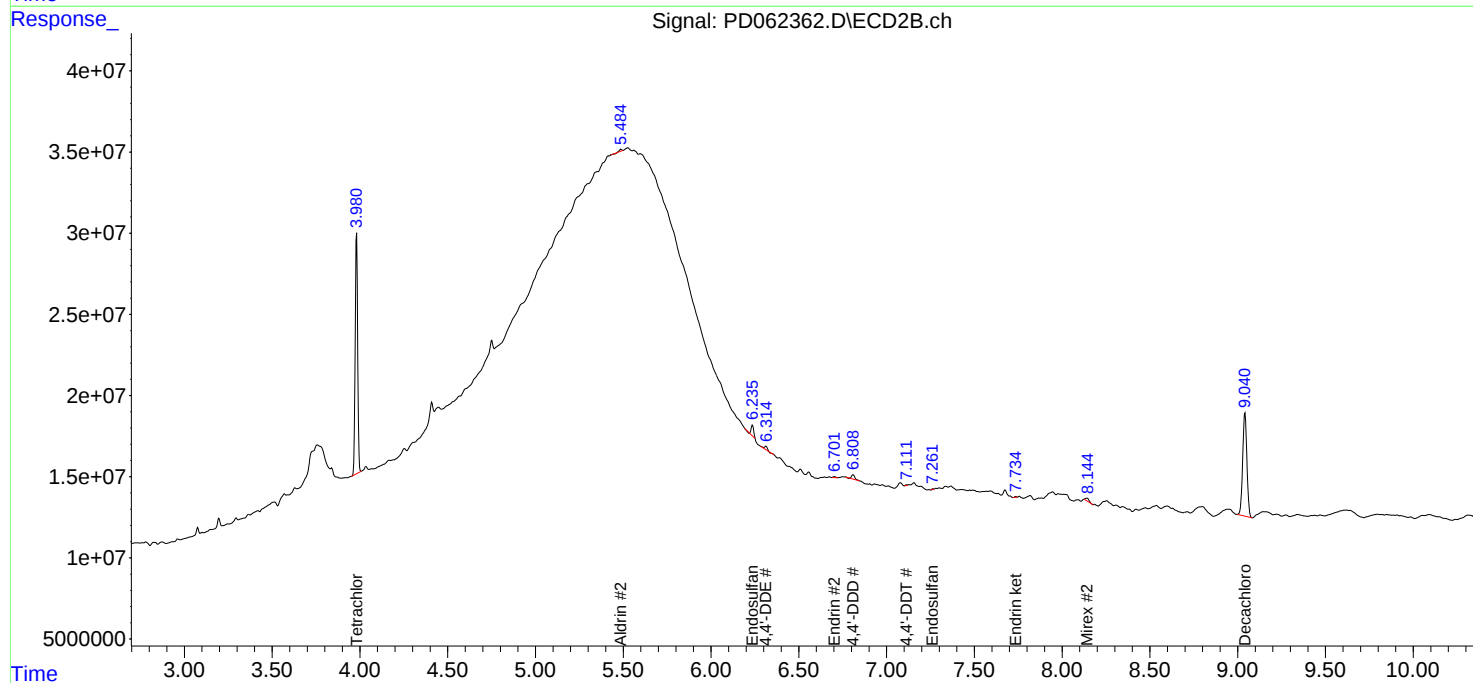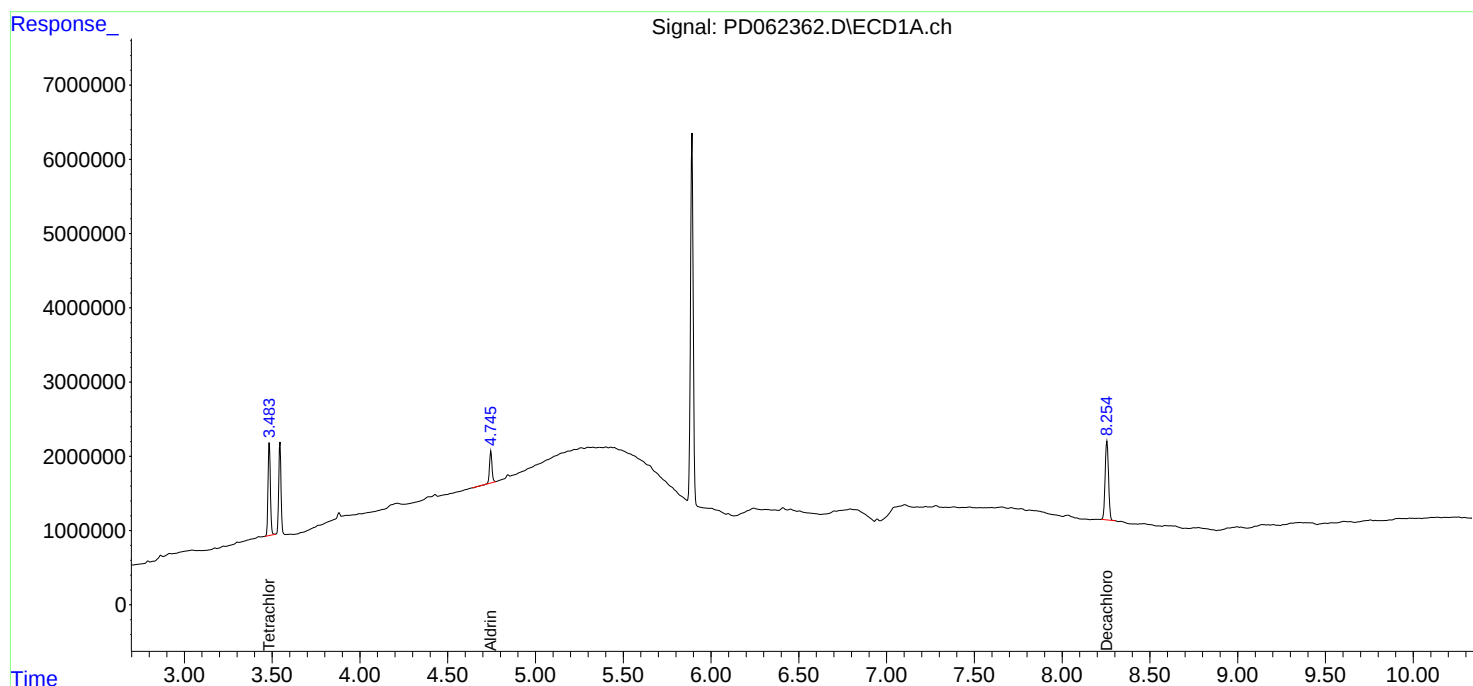

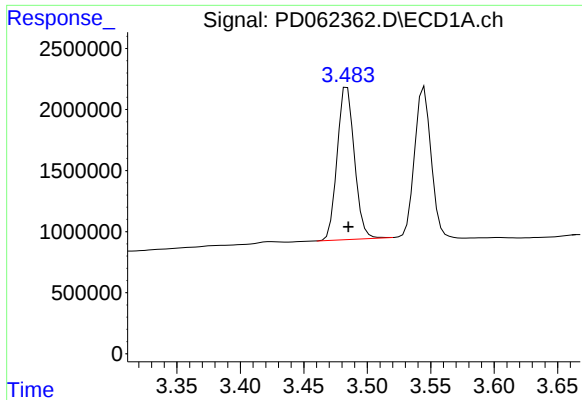


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 11849884
Conc: 14.55 ng/ml

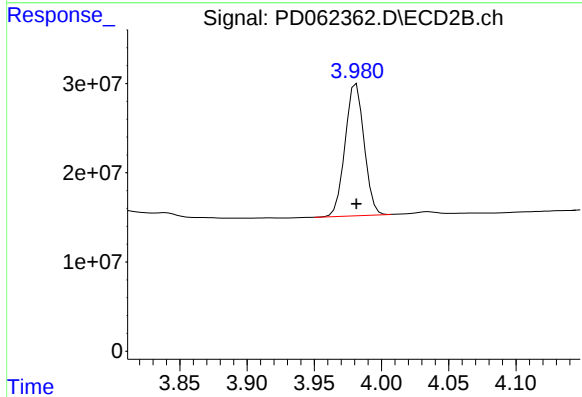


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 145014975
Conc: 13.77 ng/ml

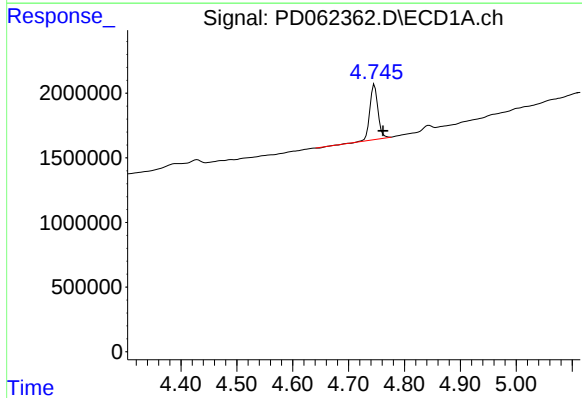


#5 Aldrin

R.T.: 4.746 min
Delta R.T.: -0.016 min
Response: 4210352
Conc: 3.36 ng/ml

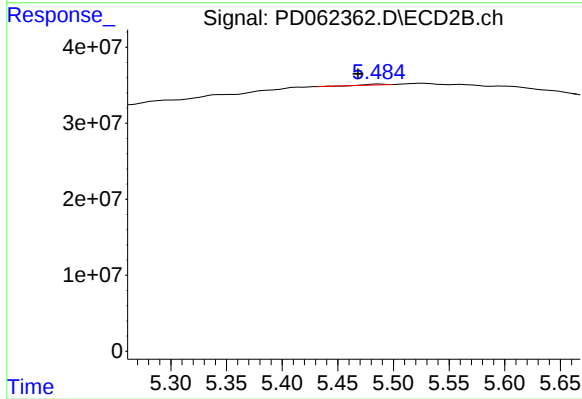


#5 Aldrin

R.T.: 5.487 min
Delta R.T.: 0.018 min
Response: 873058
Conc: 0.06 ng/ml

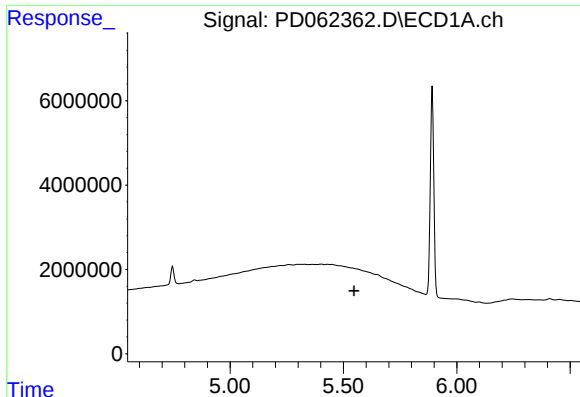


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.547 min
Response: 0
Conc: N.D.

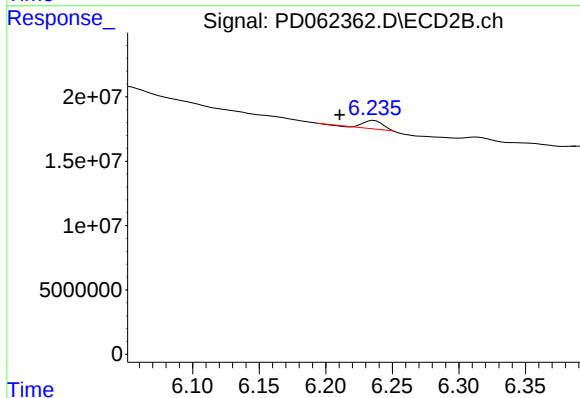


#9 Endosulfan I

R.T.: 6.236 min
Delta R.T.: 0.026 min
Response: 6122910
Conc: 0.47 ng/ml

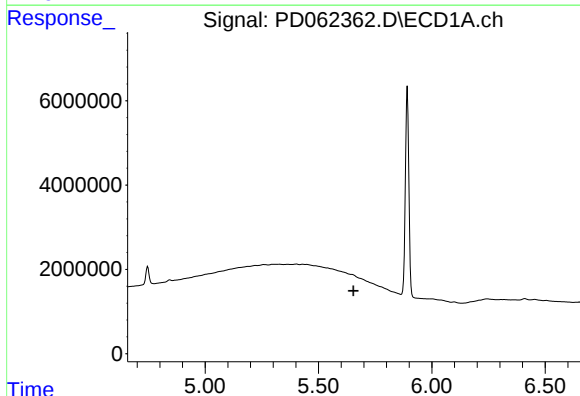


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.655 min
Response: 0
Conc: N.D.

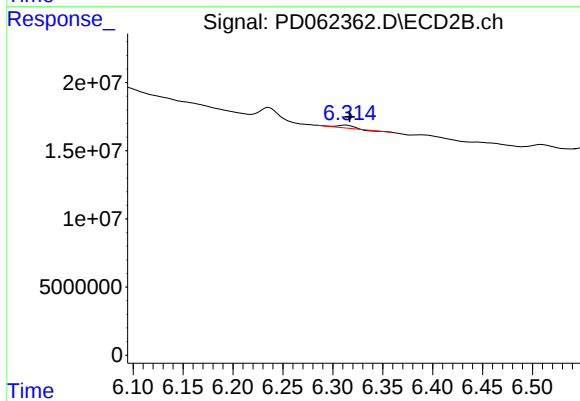


#12 4,4'-DDE

R.T.: 6.313 min
Delta R.T.: -0.004 min
Response: 1768231
Conc: 0.13 ng/ml

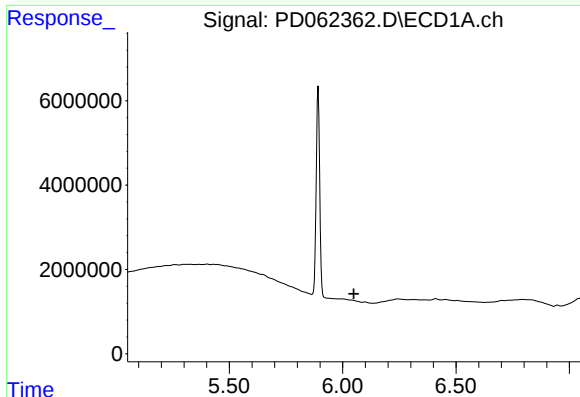


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

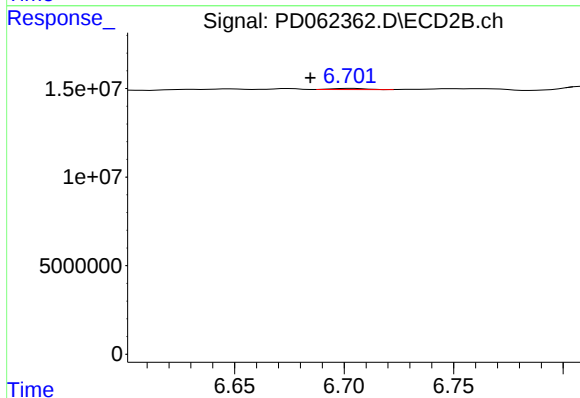


#14 Endrin

R.T.: 6.703 min
Delta R.T.: 0.018 min
Response: 666053
Conc: 0.05 ng/ml

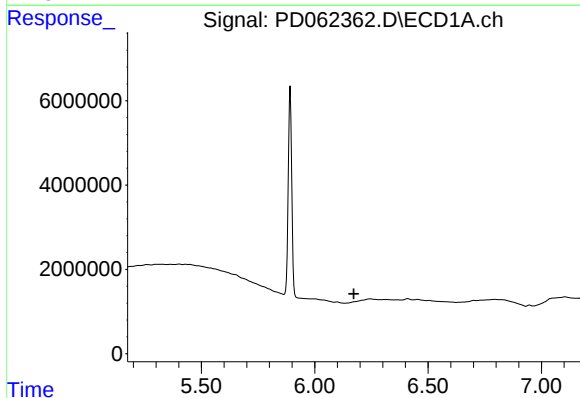


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.173 min
Response: 0
Conc: N.D.

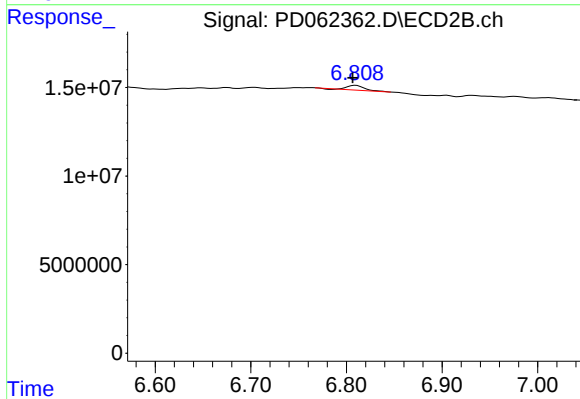


#16 4,4'-DDD

R.T.: 6.810 min
Delta R.T.: 0.003 min
Response: 3022073
Conc: 0.27 ng/ml

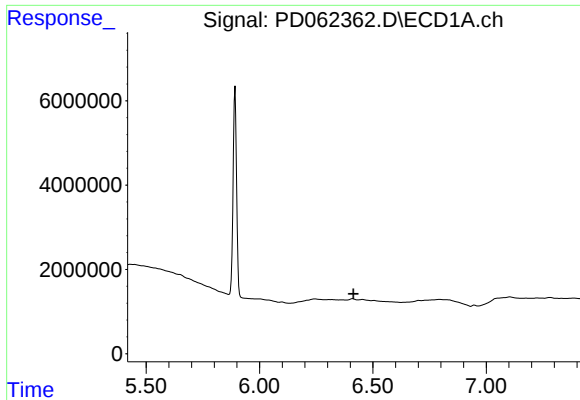


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.415 min
Response: 0
Conc: N.D.

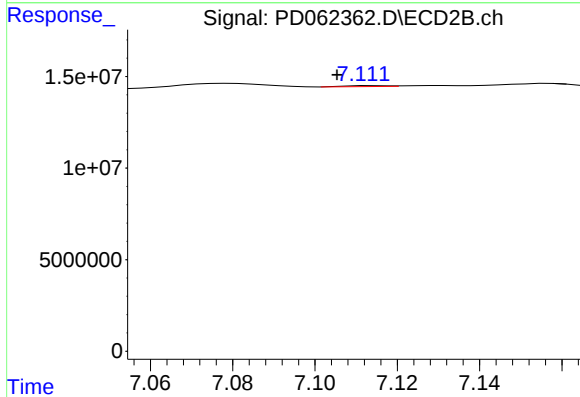


#17 4,4'-DDT

R.T.: 7.113 min
Delta R.T.: 0.008 min
Response: 317631
Conc: 0.03 ng/ml

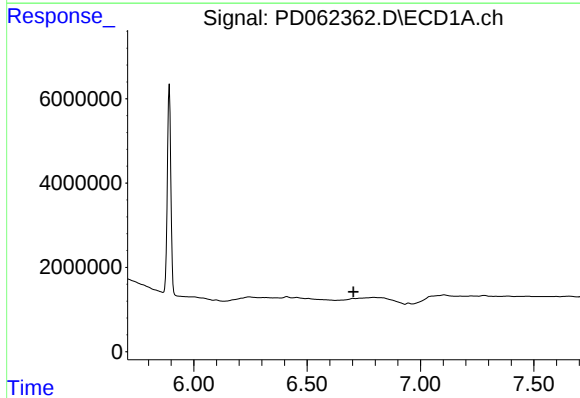


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.705 min
Response: 0
Conc: N.D.

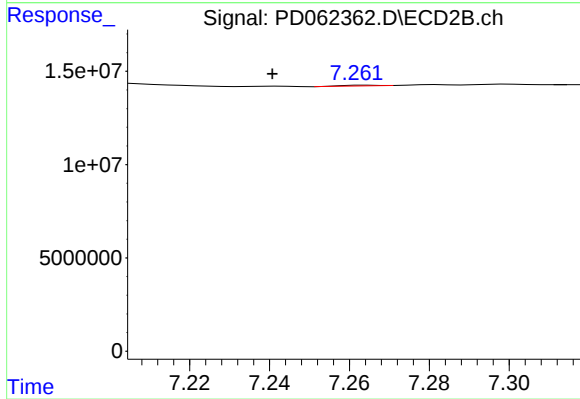


#19 Endosulfan Sulfate

R.T.: 7.263 min
Delta R.T.: 0.023 min
Response: 231858
Conc: 0.02 ng/ml

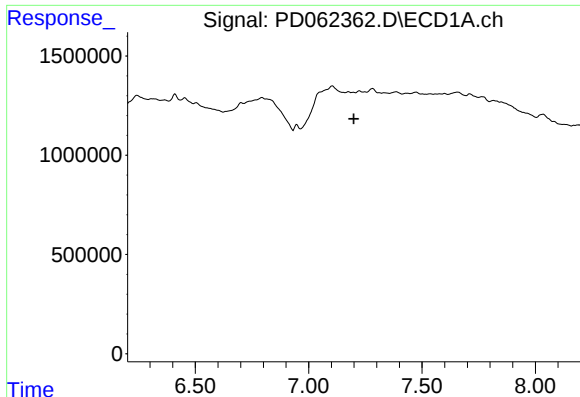


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

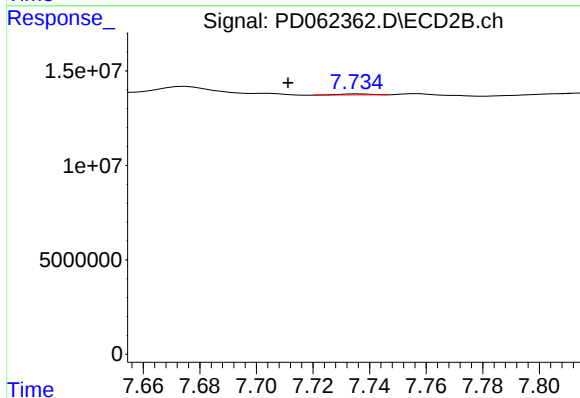


#21 Endrin ketone

R.T.: 7.737 min
Delta R.T.: 0.025 min
Response: 359734
Conc: 0.04 ng/ml

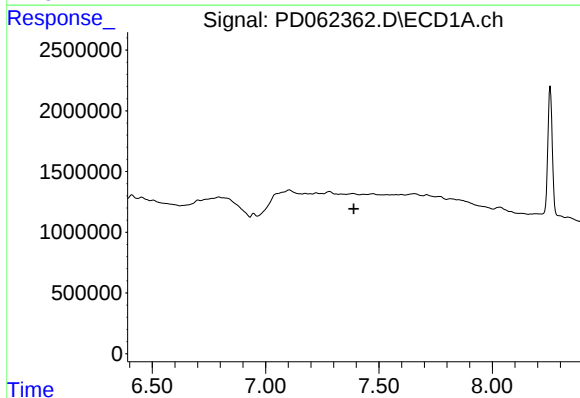


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.390 min
Response: 0
Conc: N.D.

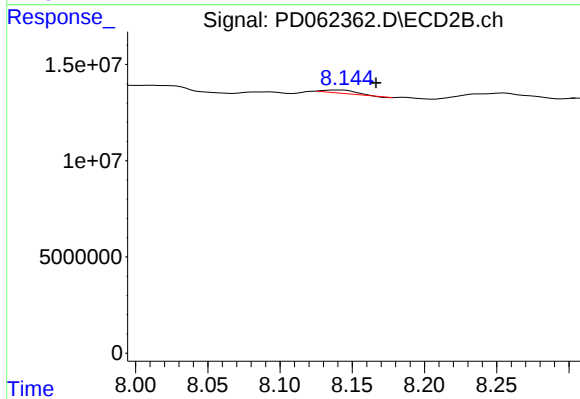


#22 Mirex

R.T.: 8.142 min
Delta R.T.: -0.024 min
Response: 2529230
Conc: 0.40 ng/ml

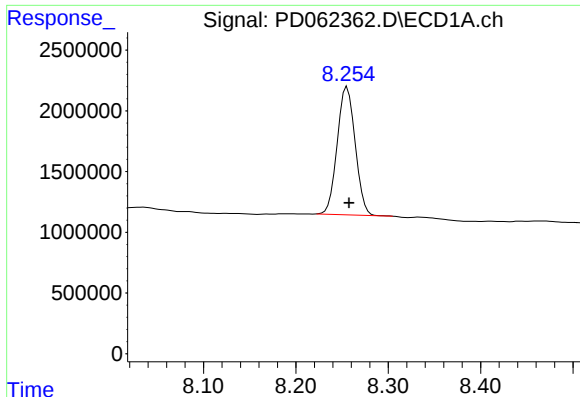

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.002 min
Response: 14229567
Conc: 11.73 ng/ml

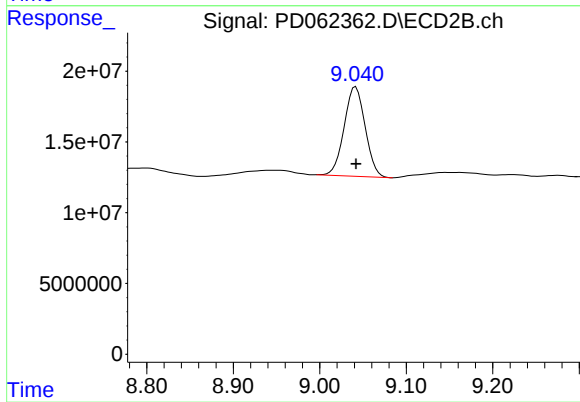

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 106463612
Conc: 12.55 ng/ml