

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
 Data File : PD062365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2021 16:53
 Operator : AR\AJ
 Sample : M2148-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 06:55:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	9600893	122.0E6	11.788	11.587
28)	SA Decachlor...	8.256	9.042	12765507	88368023	10.524	10.415
Target Compounds							
3)	MA gamma-BHC...	0.000	4.654	0	671983	N.D.	0.043 #
8)	B Heptachlo...	0.000	5.861	0	9407820	N.D.	0.685 #
11)	B alpha-Chl...	0.000	6.160	0	1274706	N.D.	0.093 #
12)	B 4,4'-DDE	0.000	6.310	0	2540179	N.D.	0.180 #
15)	B Endosulfa...	0.000	6.906	0	664604	N.D.	0.058 #
16)	A 4,4'-DDD	0.000	6.820	0	541189	N.D.	0.049 #
17)	MA 4,4'-DDT	0.000	7.108	0	1047767	N.D.	0.105 #
21)	B Endrin ke...	0.000	7.736f	0	1183720	N.D.	0.118 #
23)	Chlordane-1	0.000	4.949f	0	51916	N.D.	0.105 #
26)	Chlordane-4	0.000	6.160	0	1274706	N.D.	0.560 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
Data File : PD062365.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2021 16:53
Operator : AR\AJ
Sample : M2148-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 06:55:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

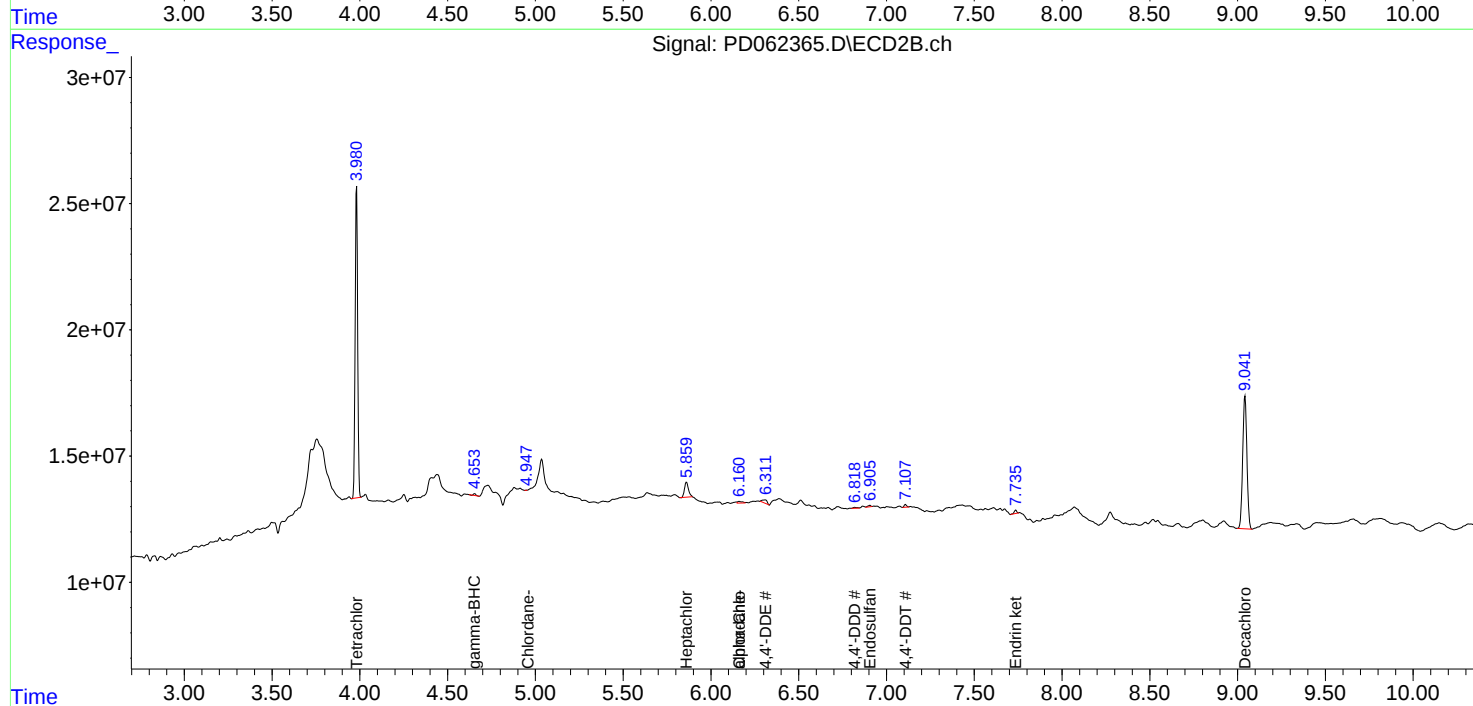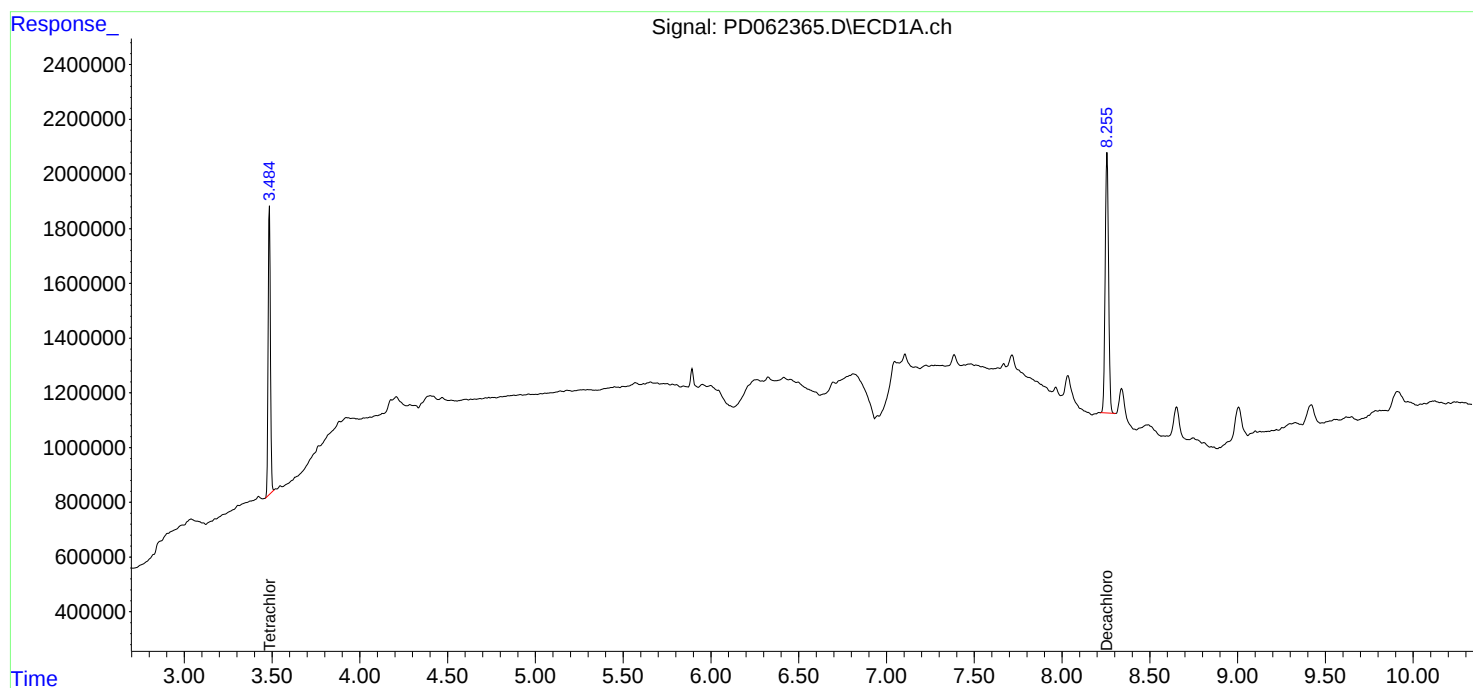

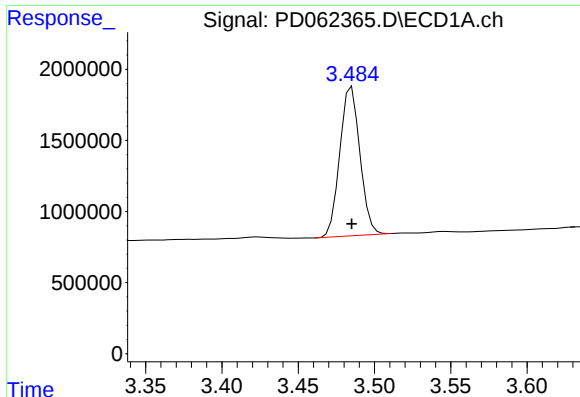


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 9600893
Conc: 11.79 ng/ml

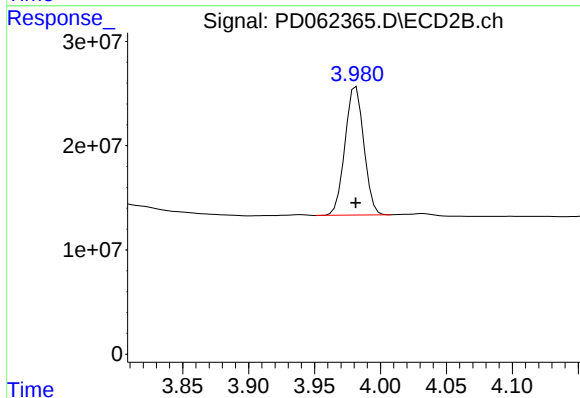


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 122028666
Conc: 11.59 ng/ml

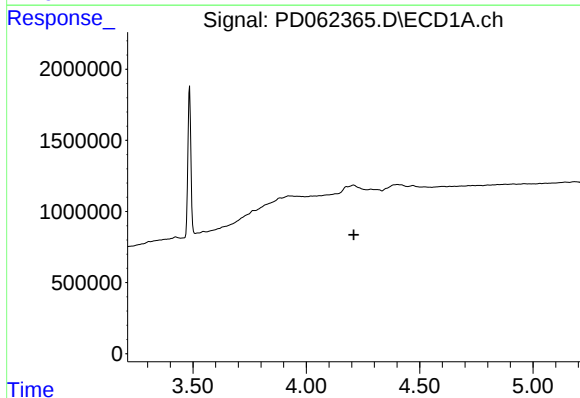


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.209 min
Response: 0
Conc: N.D.

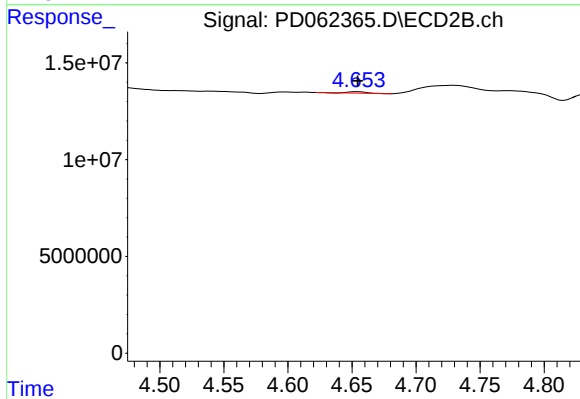


#3 gamma-BHC (Lindane)

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 671983
Conc: 0.04 ng/ml

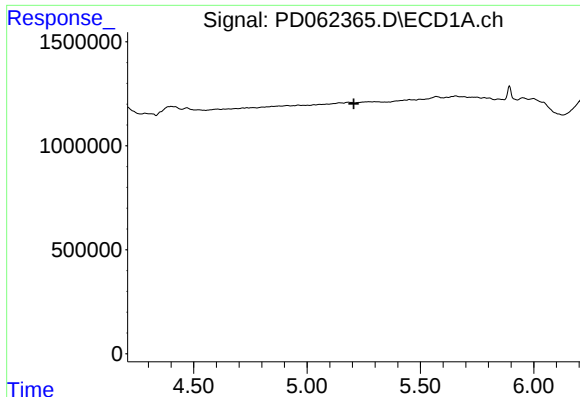


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.206 min
Response: 0
Conc: N.D.

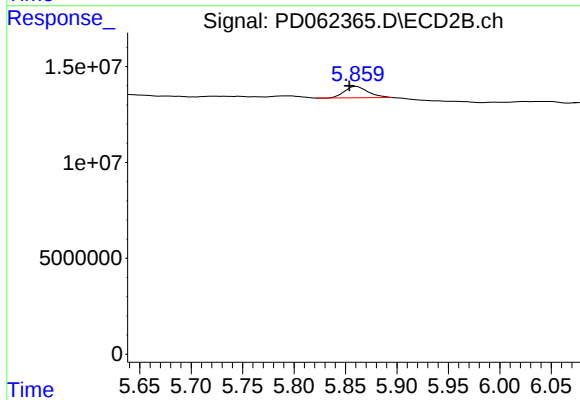


#8 Heptachlor epoxide

R.T.: 5.861 min
Delta R.T.: 0.007 min
Response: 9407820
Conc: 0.68 ng/ml

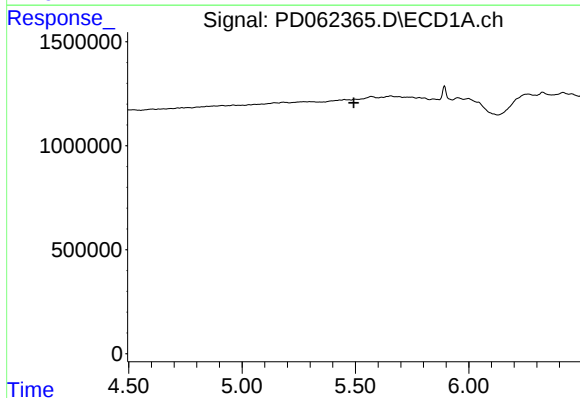


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.492 min
Response: 0
Conc: N.D.

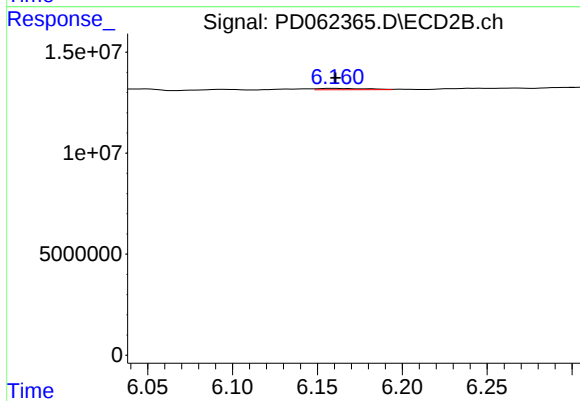


#11 alpha-Chlordane

R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 1274706
Conc: 0.09 ng/ml

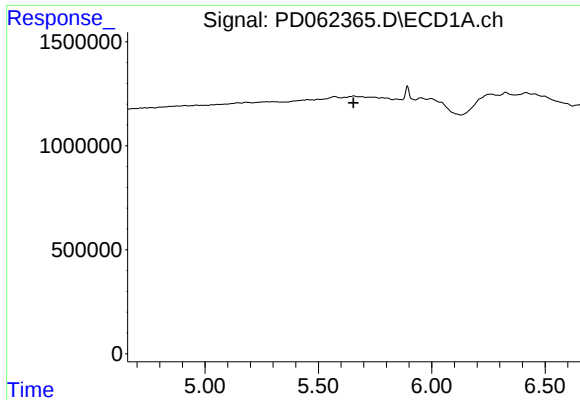


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.655 min
Response: 0
Conc: N.D.

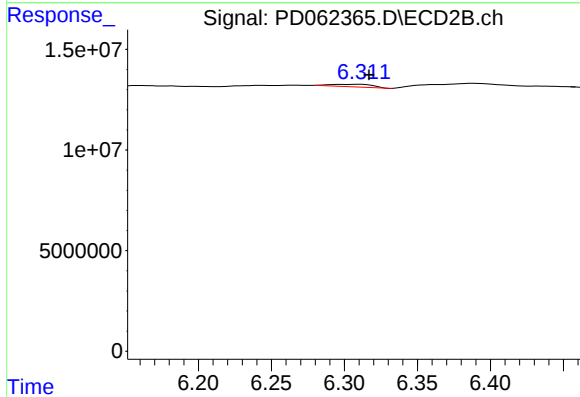


#12 4,4'-DDE

R.T.: 6.310 min
Delta R.T.: -0.007 min
Response: 2540179
Conc: 0.18 ng/ml

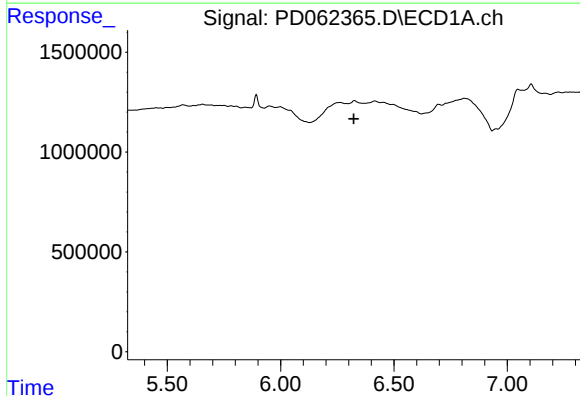


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

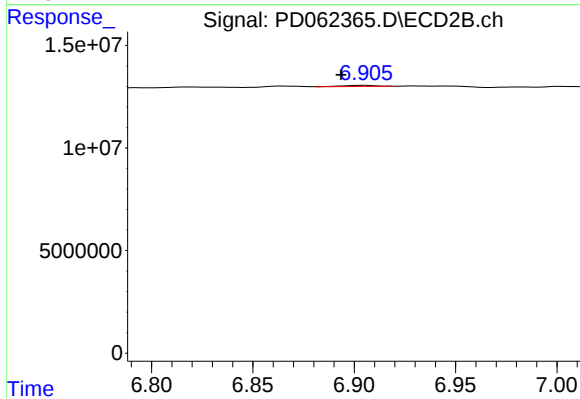


#15 Endosulfan II

R.T.: 6.906 min
Delta R.T.: 0.013 min
Response: 664604
Conc: 0.06 ng/ml

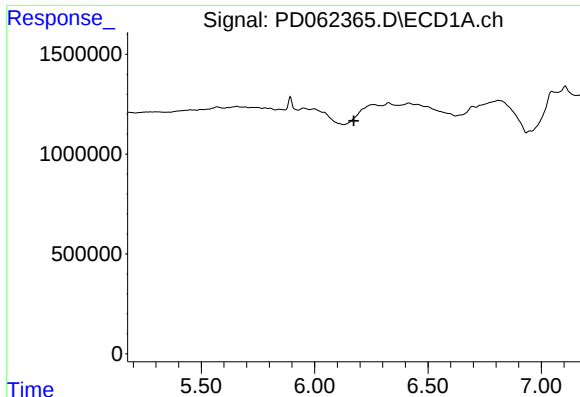


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.173 min
Response: 0
Conc: N.D.

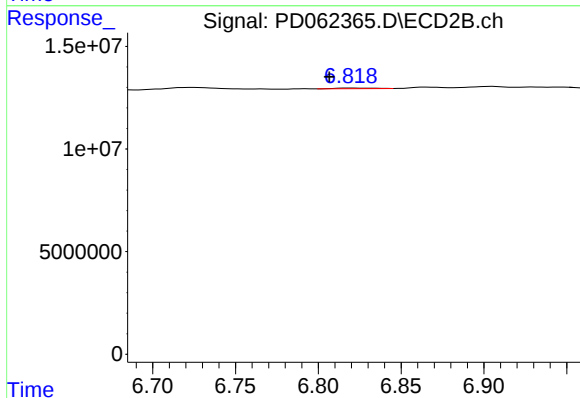


#16 4,4'-DDD

R.T.: 6.820 min
Delta R.T.: 0.013 min
Response: 541189
Conc: 0.05 ng/ml

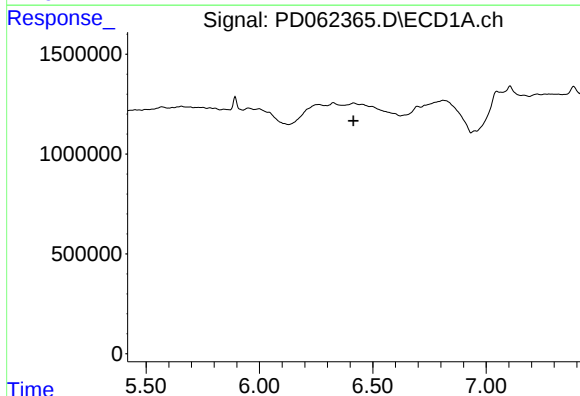


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.415 min
Response: 0
Conc: N.D.

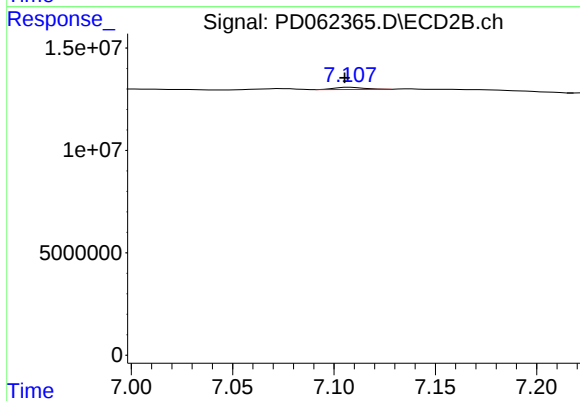


#17 4,4'-DDT

R.T.: 7.108 min
Delta R.T.: 0.003 min
Response: 1047767
Conc: 0.11 ng/ml

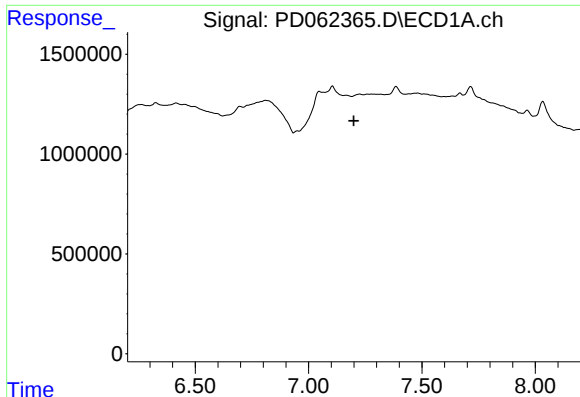


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

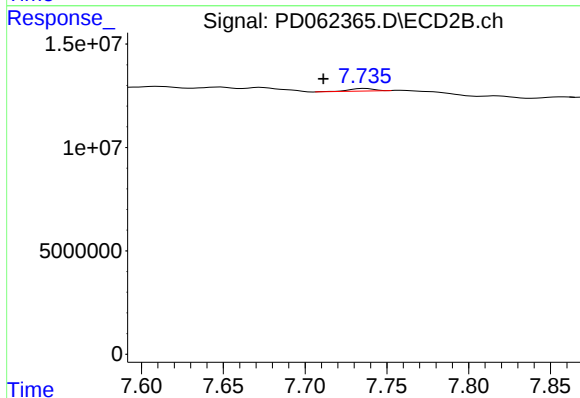


#21 Endrin ketone

R.T.: 7.736 min
Delta R.T.: 0.025 min
Response: 1183720
Conc: 0.12 ng/ml

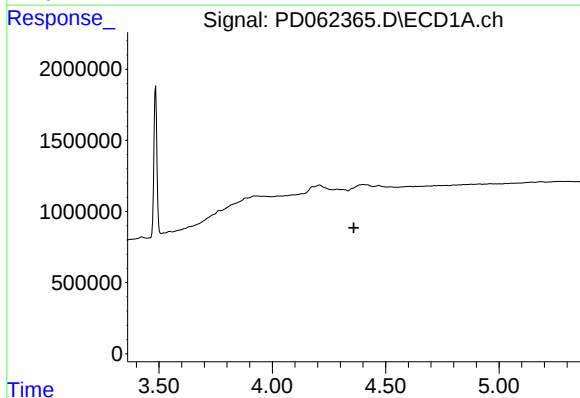


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.360 min
Response: 0
Conc: N.D.

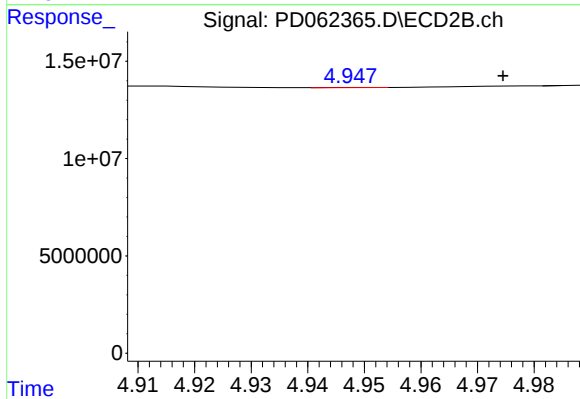


#23 Chlordane-1

R.T.: 4.949 min
Delta R.T.: -0.026 min
Response: 51916
Conc: 0.11 ng/ml

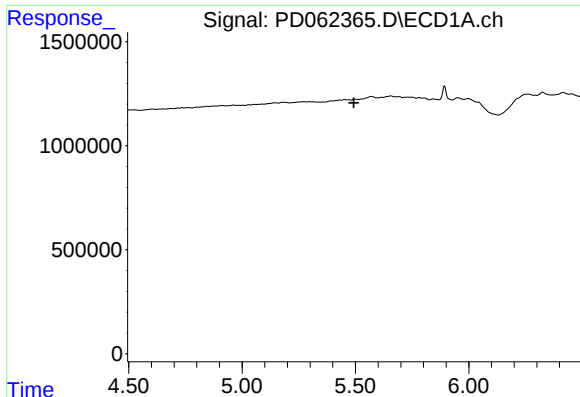


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.493 min
Response: 0
Conc: N.D.

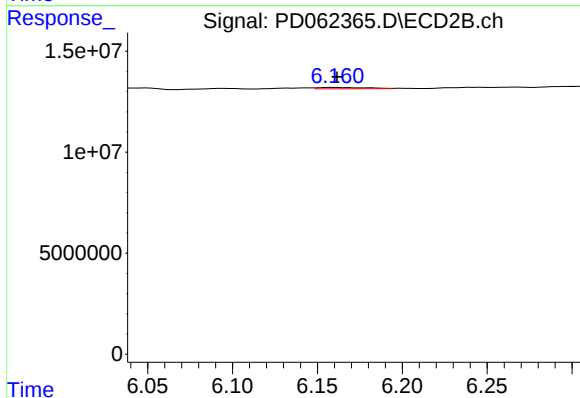


#26 Chlordane-4

R.T.: 6.160 min
Delta R.T.: -0.002 min
Response: 1274706
Conc: 0.56 ng/ml

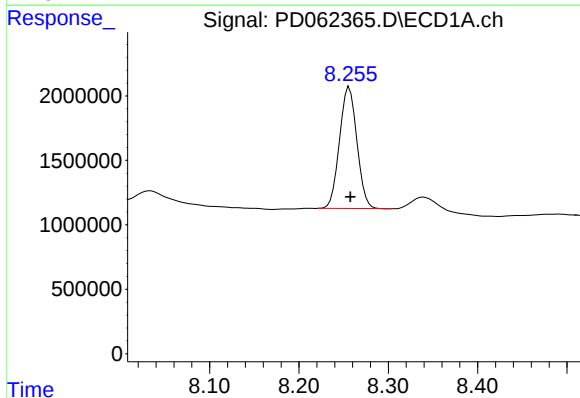

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.001 min
Response: 12765507
Conc: 10.52 ng/ml

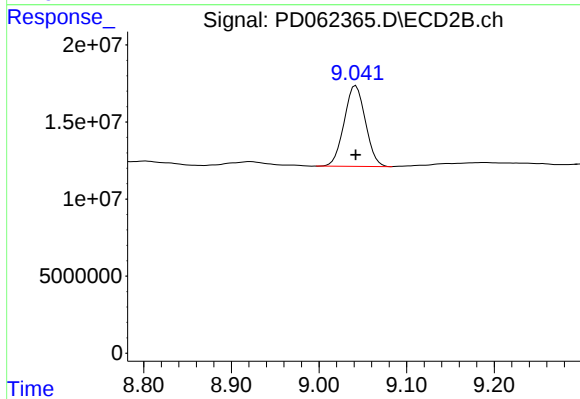

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 88368023
Conc: 10.41 ng/ml