

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
 Data File : PD062367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2021 17:21
 Operator : AR\AJ
 Sample : M2149-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 06:55:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	8484540	114.3E6	10.417	10.854
28)	SA Decachlor...	8.256	9.042	13559818	92487438	11.178	10.900
Target Compounds							
5)	MB Aldrin	4.747f	5.473	101.9E6	937.9E6	81.410	62.395
7)	B delta-BHC	4.656	5.021f	1307369	102.4E6	1.032	2.583 #
8)	B Heptachlo...	5.235f	0.000	32568109	0	26.527	N.D. #
10)	B gamma-Chl...	5.445	6.070f	341.6E6	-253700955	268.047	N.D. #
21)	B Endrin ke...	7.223f	0.000	953389	0	0.783	N.D. #
22)	Mirex	0.000	8.184f	0	11696791	N.D.	1.871 #
23)	Chlordane-1	4.349	0.000	2737615	0	78.887	N.D. #
24)	Chlordane-2	4.849	0.000	4583147	0	109.700	N.D. #
25)	Chlordane-3	5.445	6.070f	341.6E6	-253700955	2738.865	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
Data File : PD062367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2021 17:21
Operator : AR\AJ
Sample : M2149-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 06:55:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

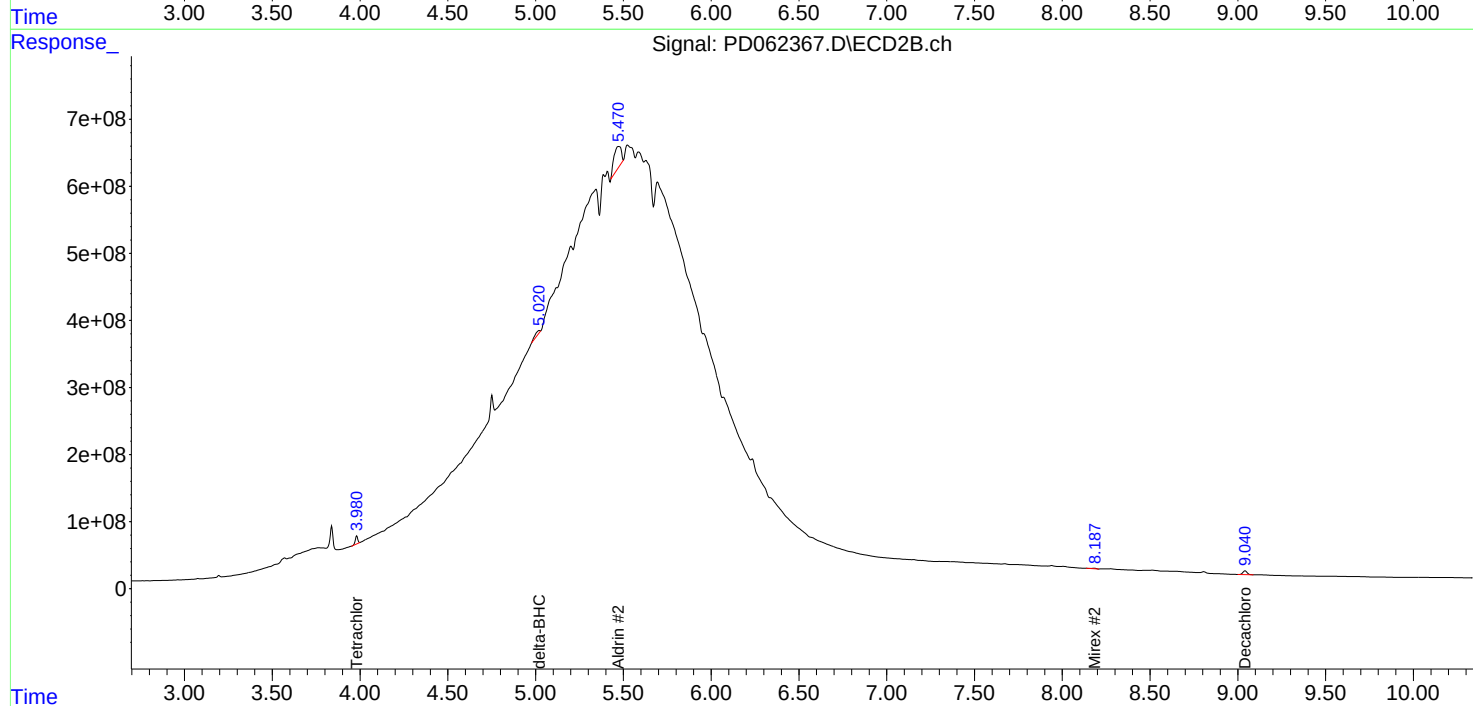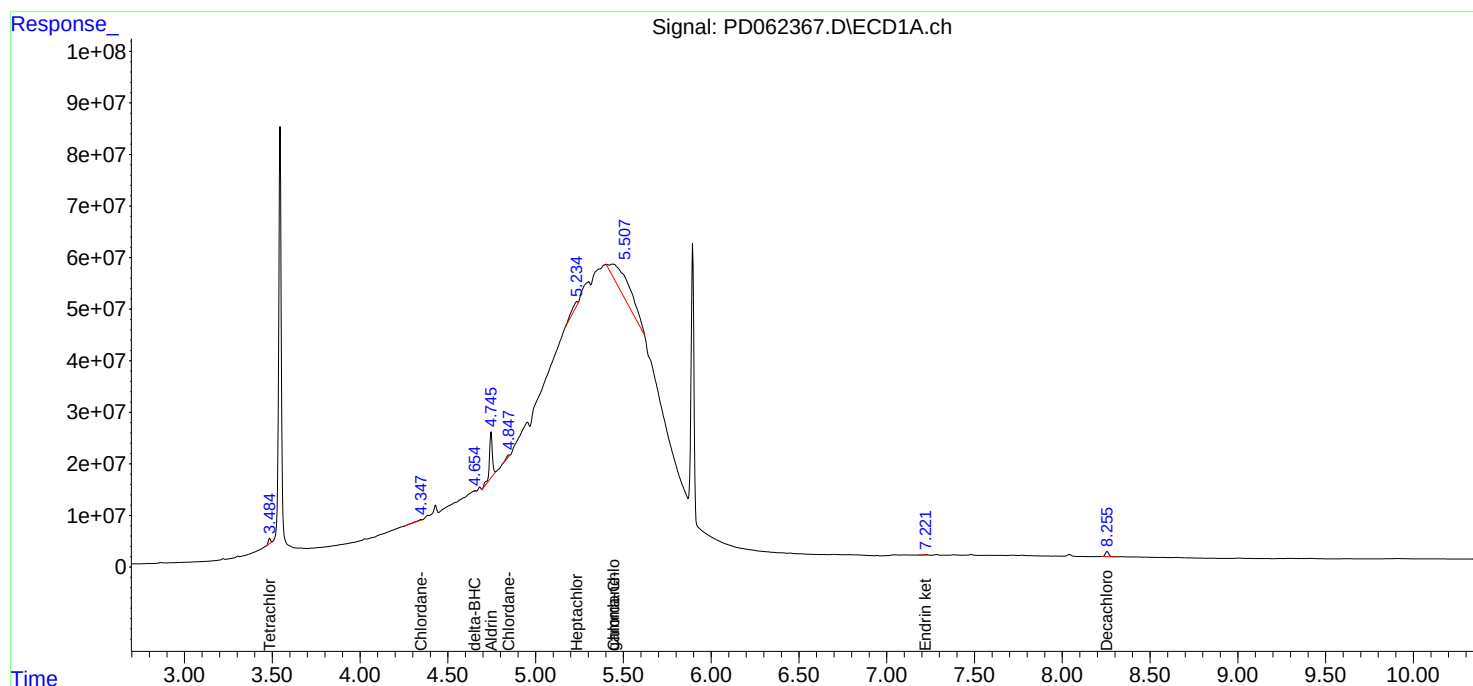

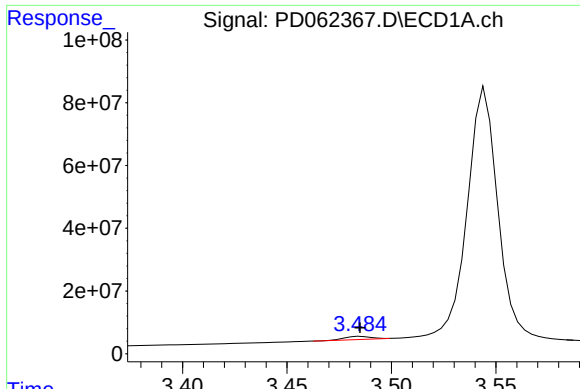


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 8484540
Conc: 10.42 ng/ml

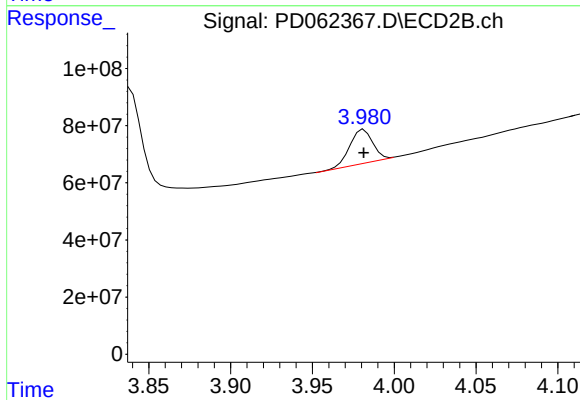


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 114305198
Conc: 10.85 ng/ml

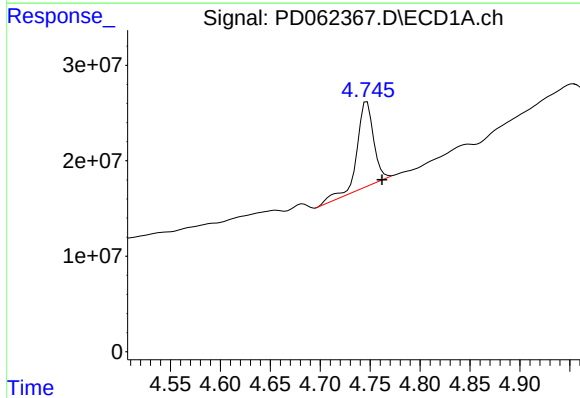


#5 Aldrin

R.T.: 4.747 min
Delta R.T.: -0.015 min
Response: 101891007
Conc: 81.41 ng/ml

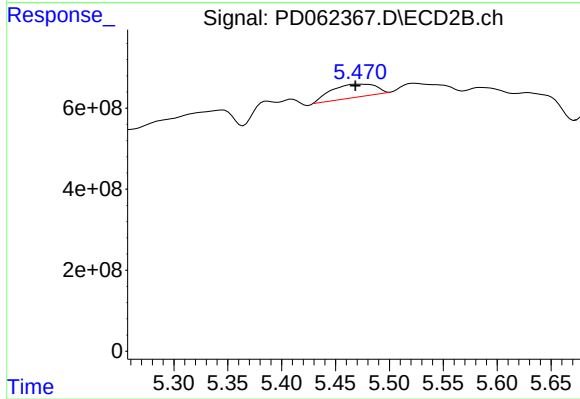


#5 Aldrin

R.T.: 5.473 min
Delta R.T.: 0.005 min
Response: 937929190
Conc: 62.39 ng/ml

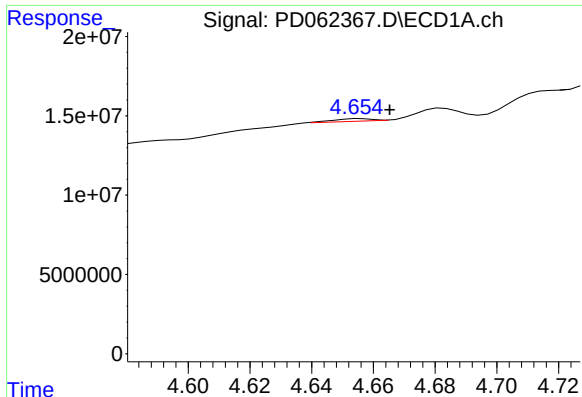


#7 delta-BHC

R.T.: 4.656 min
Delta R.T.: -0.009 min
Response: 1307369
Conc: 1.03 ng/ml

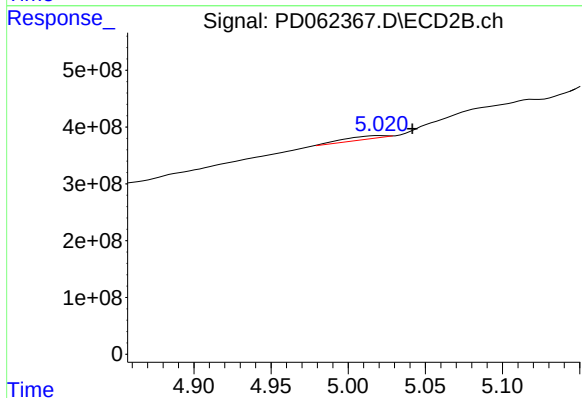


#7 delta-BHC

R.T.: 5.021 min
Delta R.T.: -0.020 min
Response: 102356049
Conc: 2.58 ng/ml

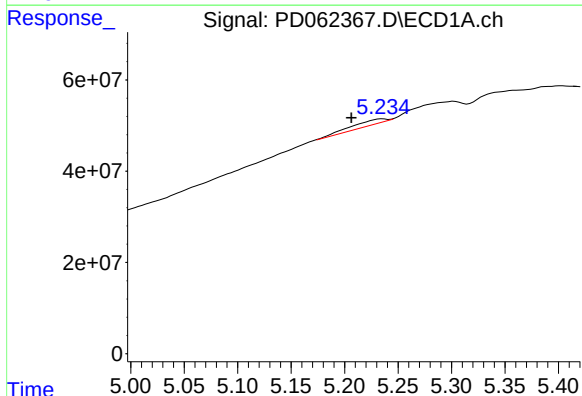


#8 Heptachlor epoxide

R.T.: 5.235 min
Delta R.T.: 0.029 min
Response: 32568109
Conc: 26.53 ng/ml

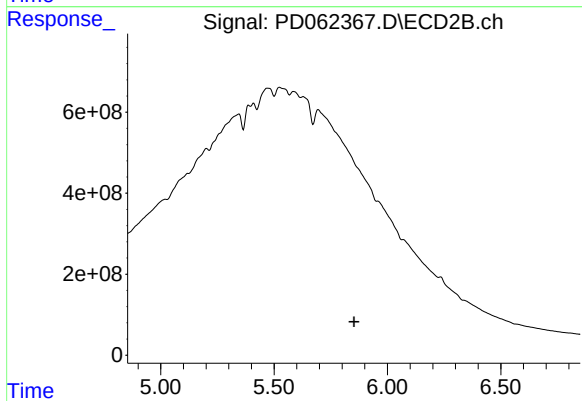


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.854 min
Response: 0
Conc: N.D.

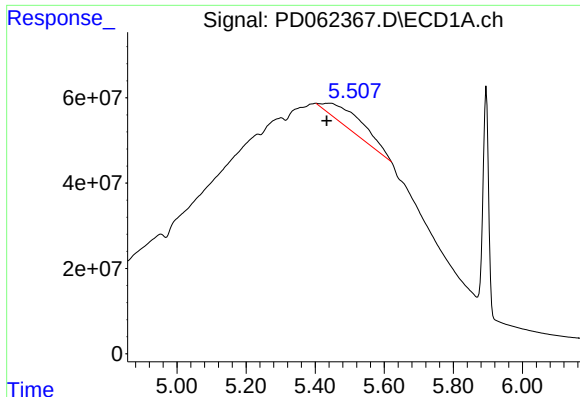


#10 gamma-Chlordane

R.T.: 5.445 min
Delta R.T.: 0.011 min
Response: 341550560
Conc: 268.05 ng/ml

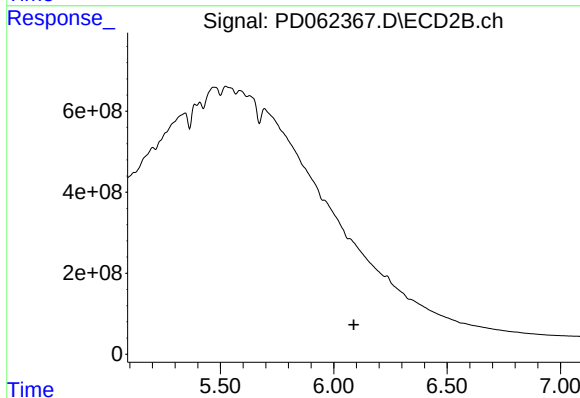


#10 gamma-Chlordane

R.T.: 6.070 min
Delta R.T.: -0.018 min
Response: -253700955
Conc: N.D.

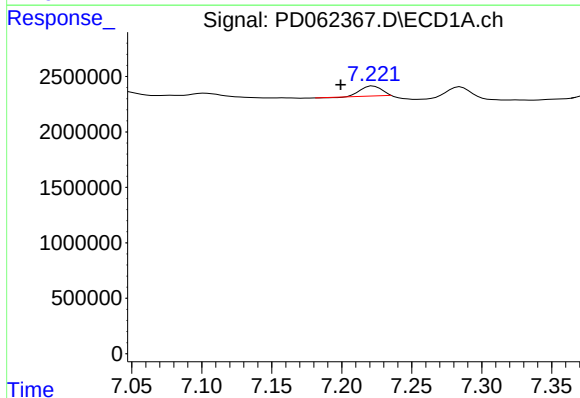


#21 Endrin ketone

R.T.: 7.223 min
Delta R.T.: 0.023 min
Response: 953389
Conc: 0.78 ng/ml

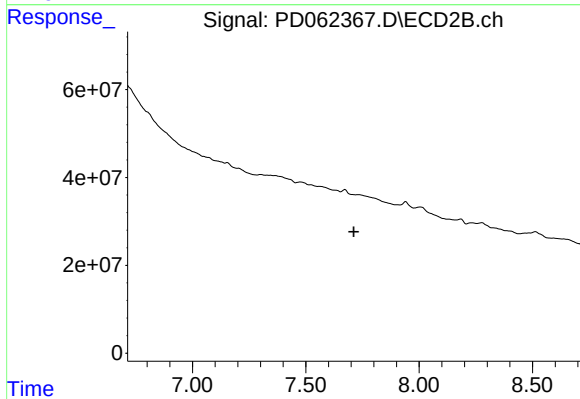


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.711 min
Response: 0
Conc: N.D.

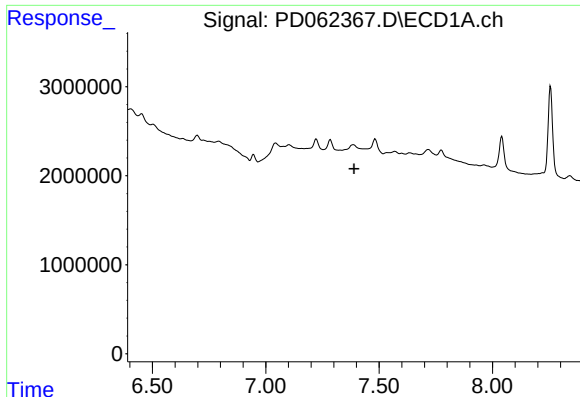


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.390 min
Response: 0
Conc: N.D.

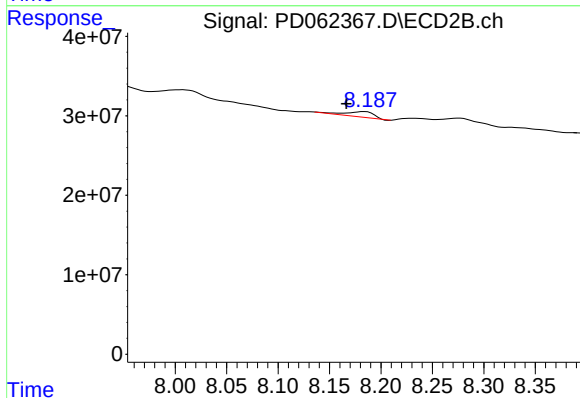


#22 Mirex

R.T.: 8.184 min
Delta R.T.: 0.017 min
Response: 11696791
Conc: 1.87 ng/ml

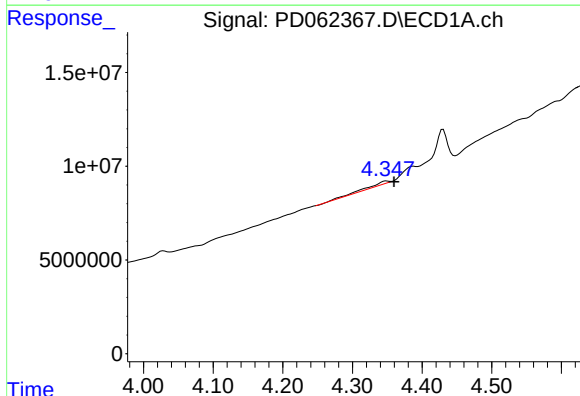


#23 Chlordane-1

R.T.: 4.349 min
Delta R.T.: -0.011 min
Response: 2737615
Conc: 78.89 ng/ml

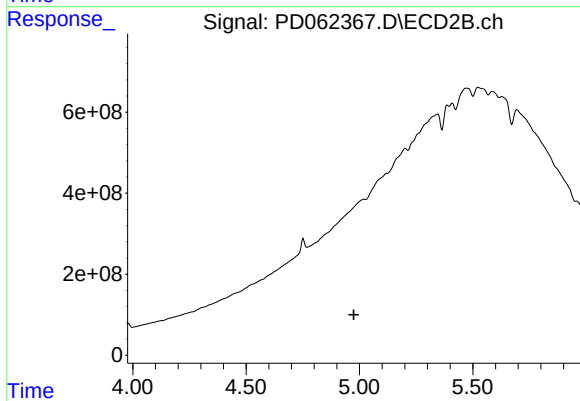


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.974 min
Response: 0
Conc: N.D.

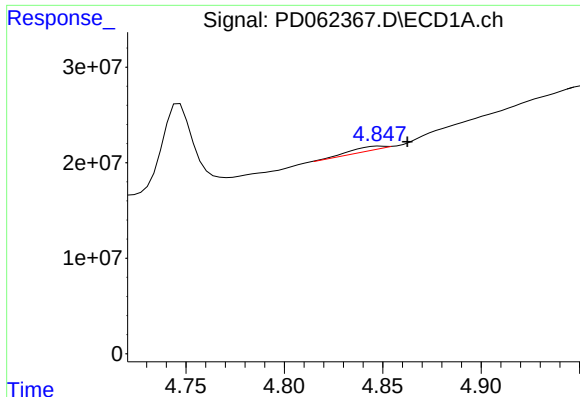


#24 Chlordane-2

R.T.: 4.849 min
Delta R.T.: -0.013 min
Response: 4583147
Conc: 109.70 ng/ml

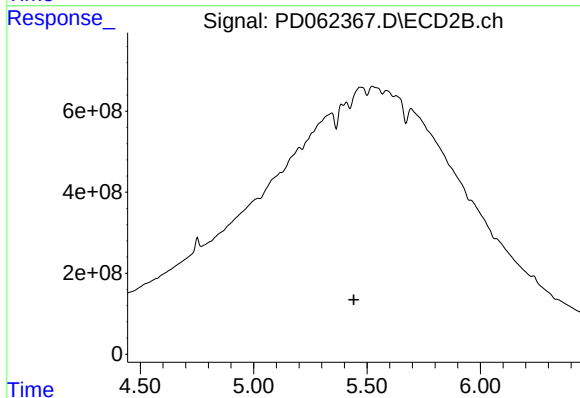


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.442 min
Response: 0
Conc: N.D.

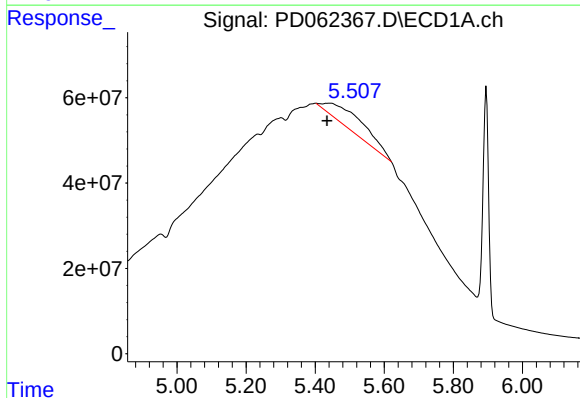


#25 Chlordane-3

R.T.: 5.445 min
Delta R.T.: 0.010 min
Response: 341550560
Conc: 2738.86 ng/ml

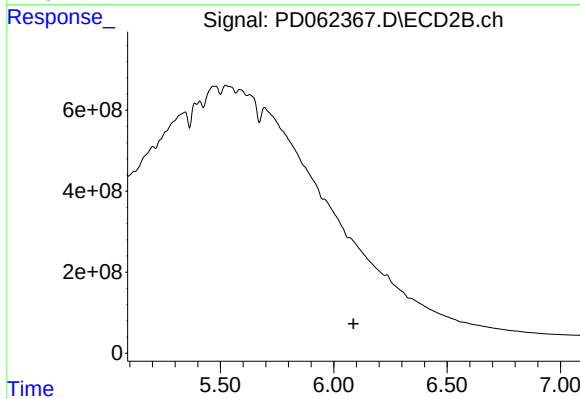


#25 Chlordane-3

R.T.: 6.070 min
Delta R.T.: -0.017 min
Response: -253700955
Conc: N.D.

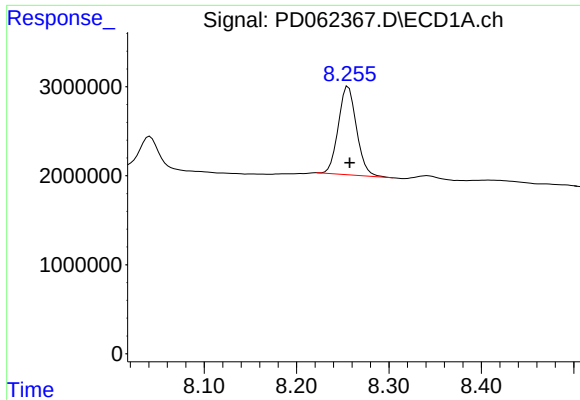

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.002 min
Response: 13559818
Conc: 11.18 ng/ml

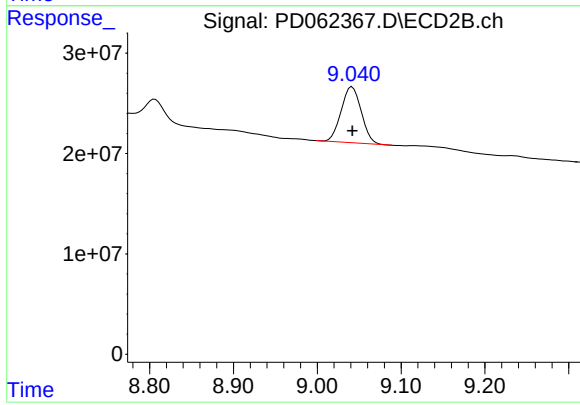

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 92487438
Conc: 10.90 ng/ml