

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
 Data File : PD062390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2021 22:56
 Operator : AR\AJ
 Sample : M2152-06
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 07:01:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.981	17239986	226.6E6	21.167	21.519
2)	SA Decachlor...	8.256	9.042	21470962	159.6E6	17.700	18.806
Target Compounds							
2)	A alpha-BHC	0.000	4.370	0	4012456	N.D.	0.237 #
3)	MA gamma-BHC...	4.212	0.000	909419	0	0.739	N.D. #
5)	MB Aldrin	4.746f	5.474	14657864	11154134	11.712	0.742 #
9)	A Endosulfan I	0.000	6.236f	0	8914299	N.D.	0.681 #
15)	B Endosulfa...	0.000	6.896	0	11607403	N.D.	1.009 #
16)	A 4,4'-DDD	0.000	6.805	0	7467092	N.D.	0.670 #
17)	MA 4,4'-DDT	0.000	7.107	0	2984690	N.D.	0.299 #
18)	B Endrin al...	0.000	7.015	0	5421254	N.D.	0.574 #
19)	B Endosulfa...	0.000	7.240	0	13833998	N.D.	1.275 #
20)	A Methoxychlor	0.000	7.561	0	1856938	N.D.	0.380 #
21)	B Endrin ke...	0.000	7.708	0	14733105	N.D.	1.469 #
27)	Chlordane-5	0.000	6.953	0	675748	N.D.	1.642 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
Data File : PD062390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2021 22:56
Operator : AR\AJ
Sample : M2152-06
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 07:01:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

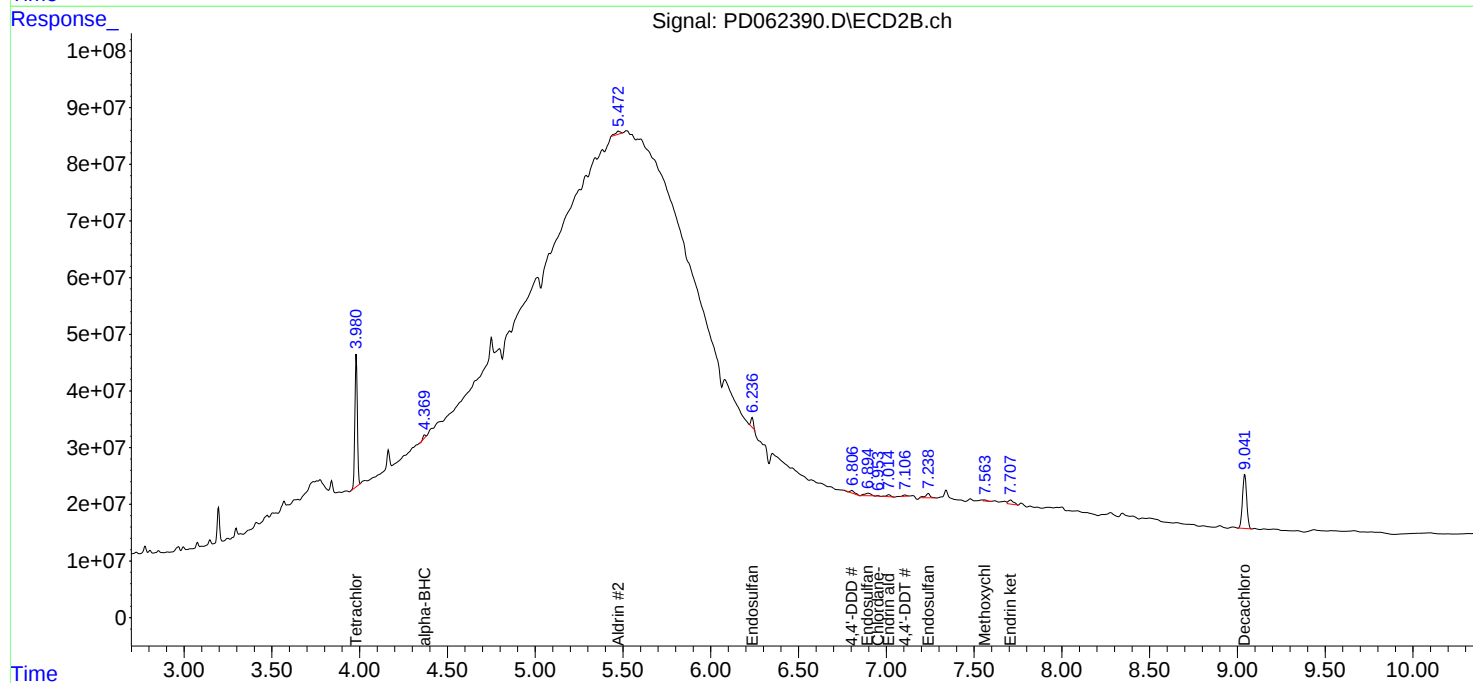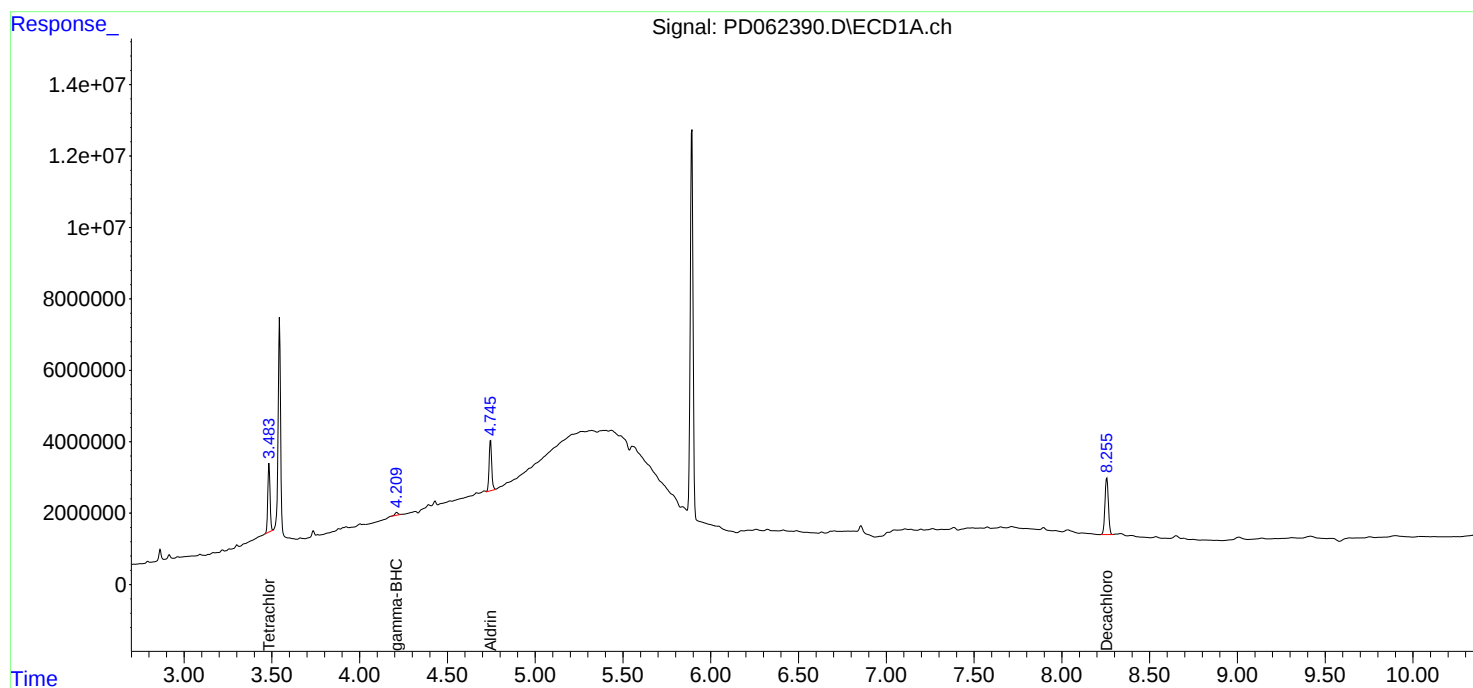

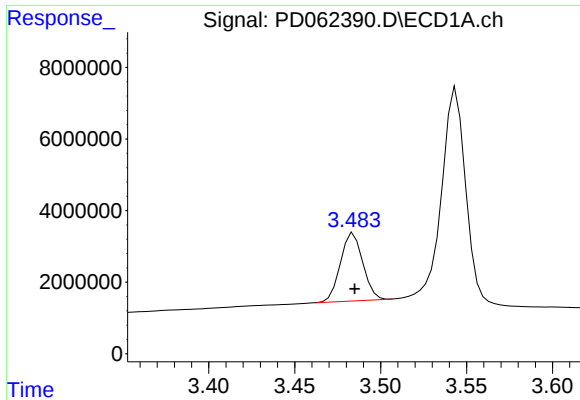


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 17239986
Conc: 21.17 ng/ml

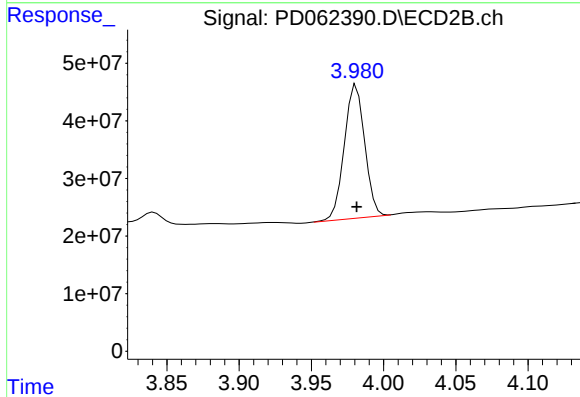


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 226628396
Conc: 21.52 ng/ml

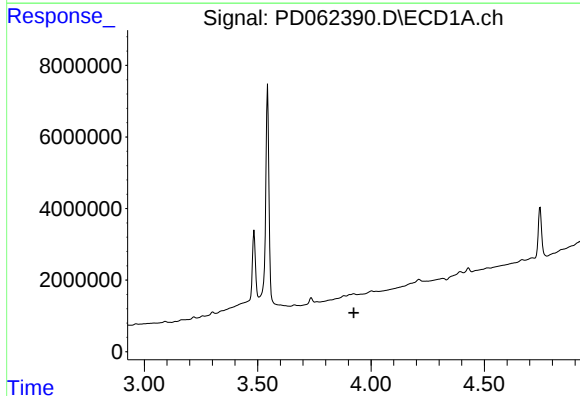


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.924 min
Response: 0
Conc: N.D.

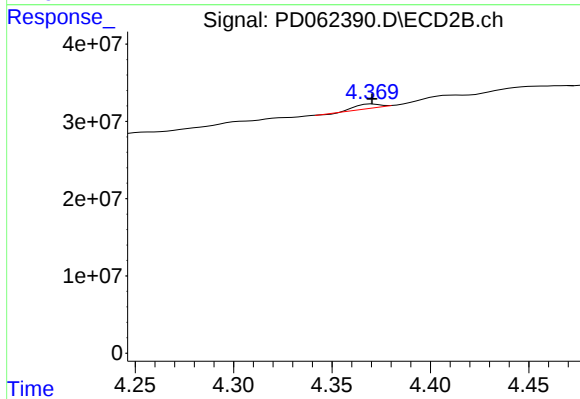


#2 alpha-BHC

R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 4012456
Conc: 0.24 ng/ml

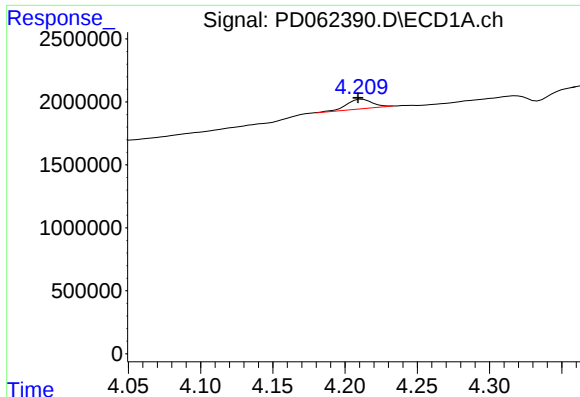


#3 gamma-BHC (Lindane)

R.T.: 4.212 min
Delta R.T.: 0.003 min
Response: 909419
Conc: 0.74 ng/ml

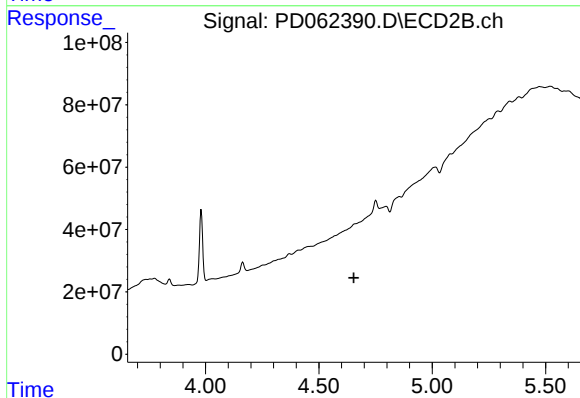


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.655 min
Response: 0
Conc: N.D.

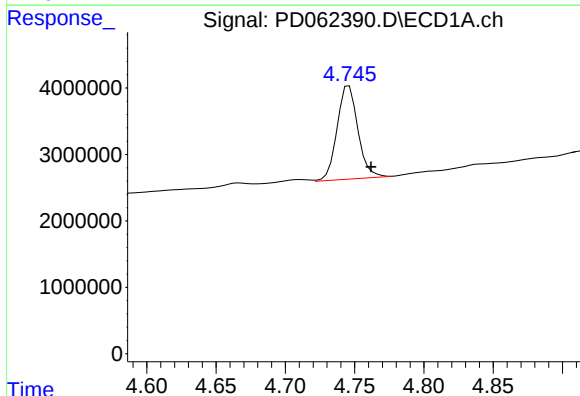


#5 Aldrin

R.T.: 4.746 min
Delta R.T.: -0.016 min
Response: 14657864
Conc: 11.71 ng/ml

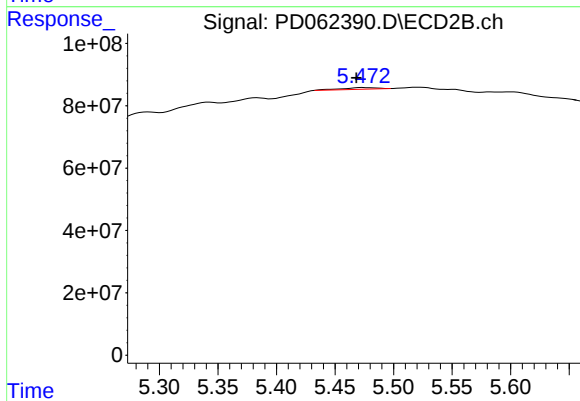


#5 Aldrin

R.T.: 5.474 min
Delta R.T.: 0.005 min
Response: 11154134
Conc: 0.74 ng/ml

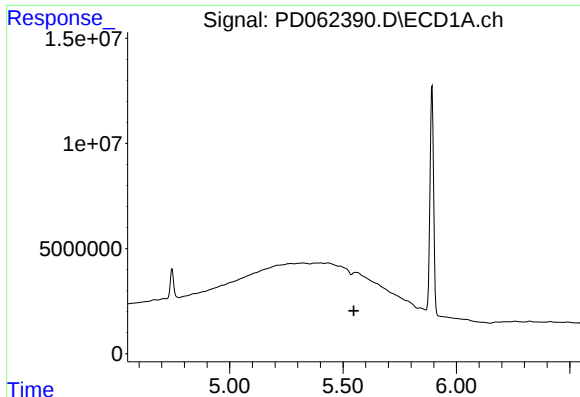


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.547 min
Response: 0
Conc: N.D.

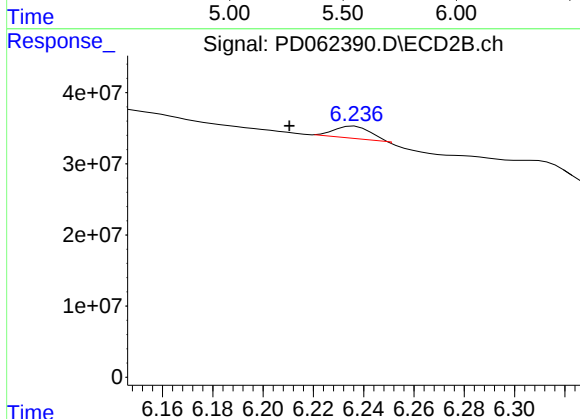


#9 Endosulfan I

R.T.: 6.236 min
Delta R.T.: 0.026 min
Response: 8914299
Conc: 0.68 ng/ml

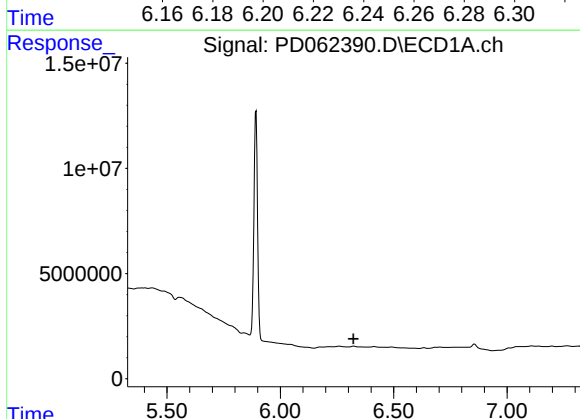


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.323 min
Response: 0
Conc: N.D.

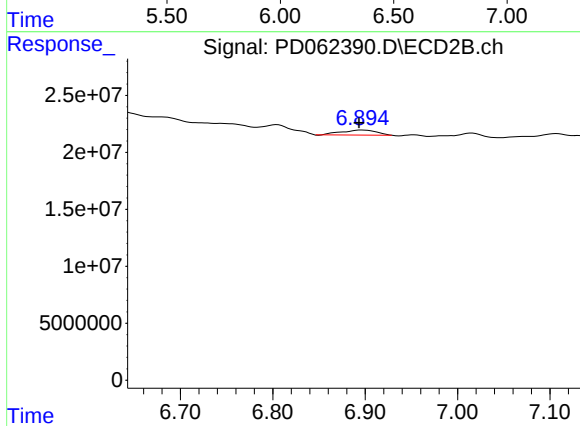


#15 Endosulfan II

R.T.: 6.896 min
Delta R.T.: 0.002 min
Response: 11607403
Conc: 1.01 ng/ml

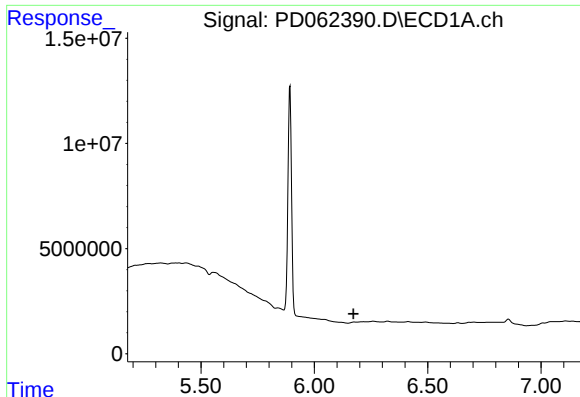


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.173 min
Response: 0
Conc: N.D.

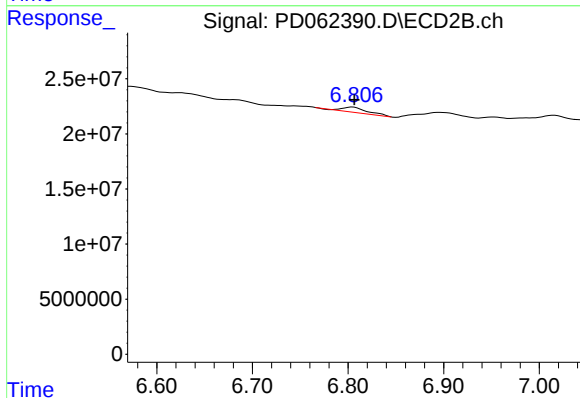


#16 4,4'-DDD

R.T.: 6.805 min
Delta R.T.: -0.002 min
Response: 7467092
Conc: 0.67 ng/ml

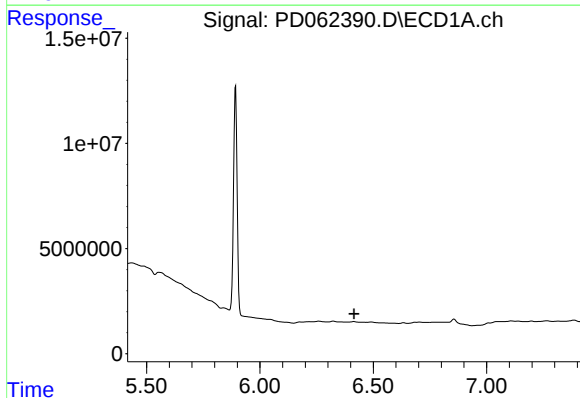


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.415 min
Response: 0
Conc: N.D.

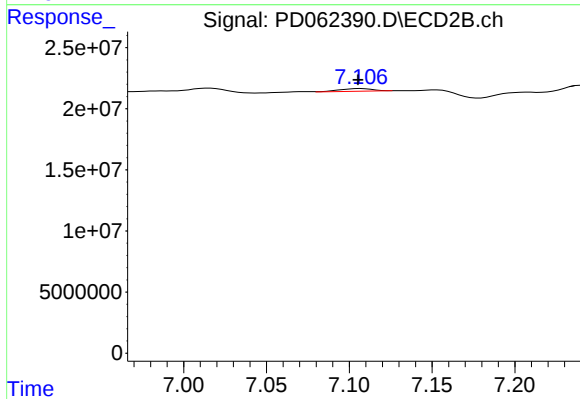


#17 4,4'-DDT

R.T.: 7.107 min
Delta R.T.: 0.002 min
Response: 2984690
Conc: 0.30 ng/ml

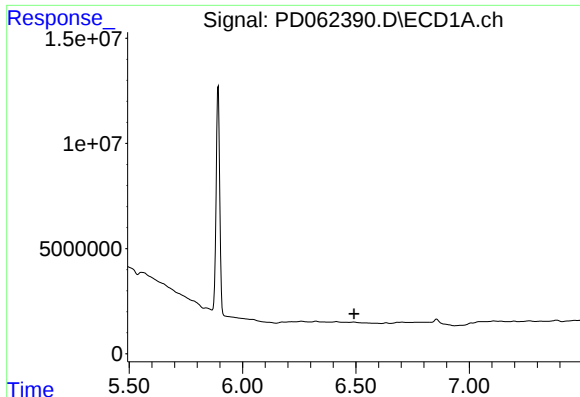


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.492 min
Response: 0
Conc: N.D.

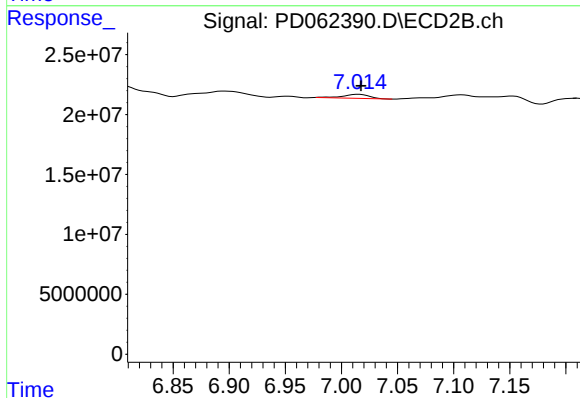


#18 Endrin aldehyde

R.T.: 7.015 min
Delta R.T.: -0.002 min
Response: 5421254
Conc: 0.57 ng/ml

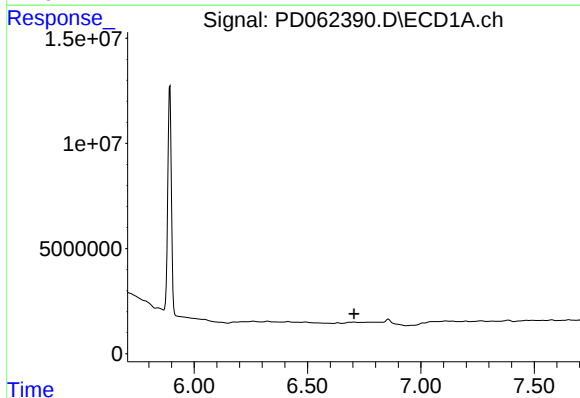


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.705 min
Response: 0
Conc: N.D.

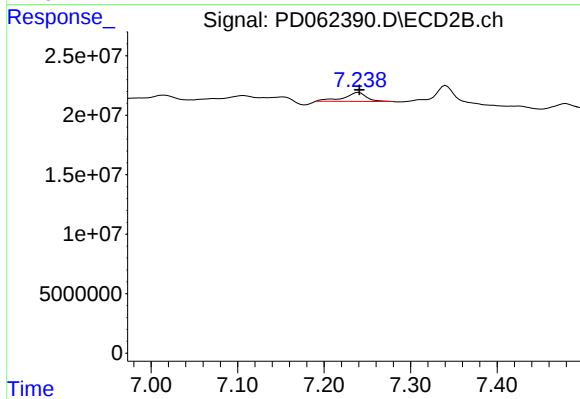


#19 Endosulfan Sulfate

R.T.: 7.240 min
Delta R.T.: 0.000 min
Response: 13833998
Conc: 1.28 ng/ml

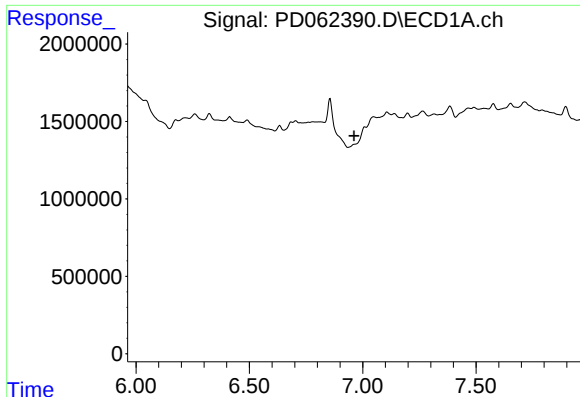


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.962 min
Response: 0
Conc: N.D.

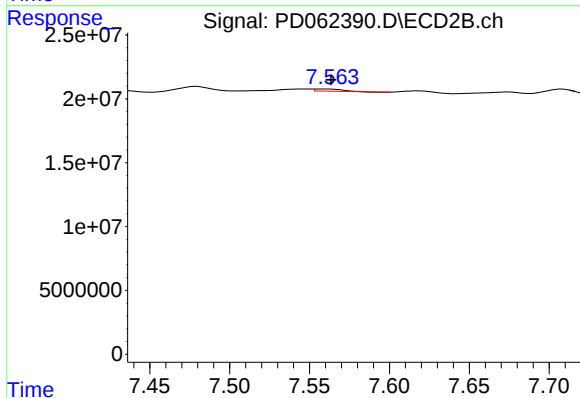


#20 Methoxychlor

R.T.: 7.561 min
Delta R.T.: -0.003 min
Response: 1856938
Conc: 0.38 ng/ml

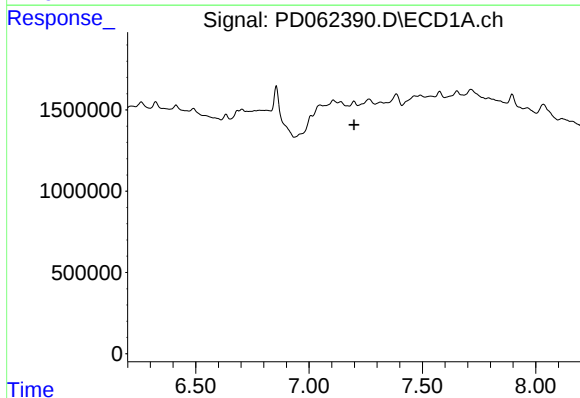


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

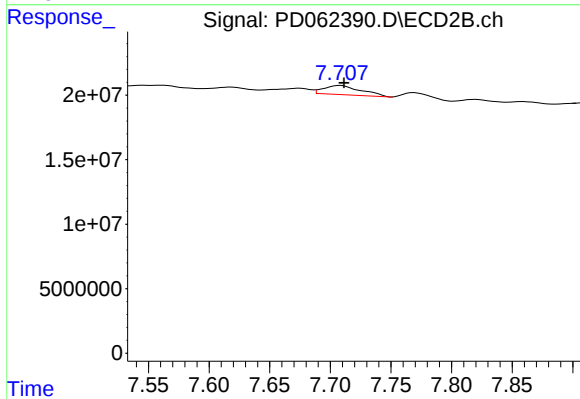


#21 Endrin ketone

R.T.: 7.708 min
Delta R.T.: -0.003 min
Response: 14733105
Conc: 1.47 ng/ml

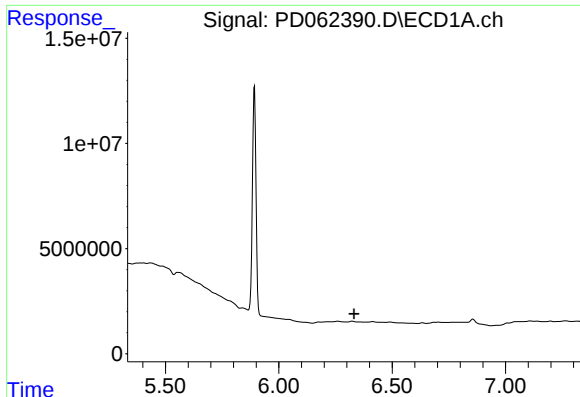


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.333 min
Response: 0
Conc: N.D.

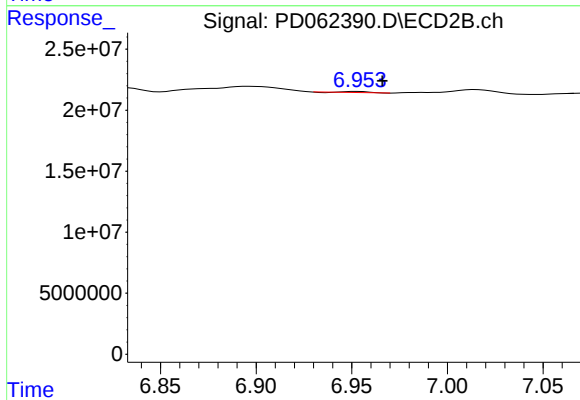


#27 Chlordane-5

R.T.: 6.953 min
Delta R.T.: -0.013 min
Response: 675748
Conc: 1.64 ng/ml

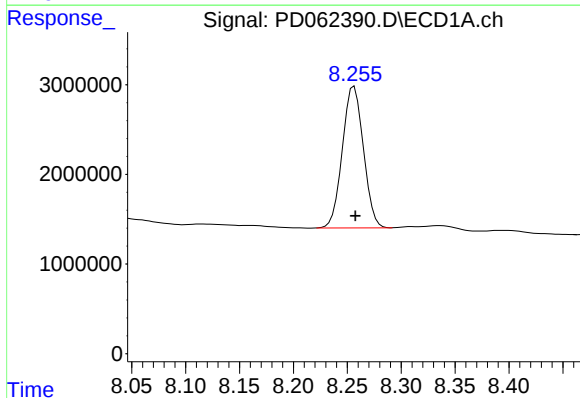

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.001 min
Response: 21470962
Conc: 17.70 ng/ml

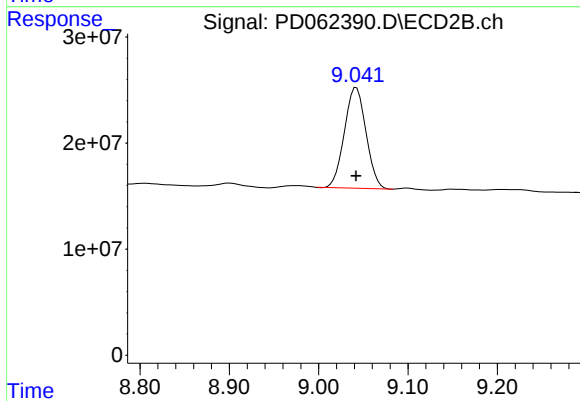

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 159566867
Conc: 18.81 ng/ml