

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
 Data File : PD062394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2021 23:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 07:02:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.981	17479273	230.5E6	21.460	21.887
28)	SA Decachlor...	8.256	9.041	25077321	185.0E6	20.673	21.801
Target Compounds							
3)	MA gamma-BHC...	0.000	4.653	0	434511	N.D.	0.028 #
4)	MA Heptachlor	0.000	5.156	0	974590	N.D.	0.062 #
5)	MB Aldrin	0.000	5.468	0	291646	N.D.	0.019 #
8)	B Heptachlo...	0.000	5.854	0	23200132	N.D.	1.689 #
9)	A Endosulfan I	0.000	6.204	0	1312655	N.D.	0.100 #
15)	B Endosulfa...	0.000	6.881	0	3480725	N.D.	0.302 #
17)	MA 4,4'-DDT	0.000	7.108	0	2842705	N.D.	0.285 #
21)	B Endrin ke...	0.000	7.734f	0	2833122	N.D.	0.282 #
22)	Mirex	0.000	8.187f	0	700135	N.D.	0.112 #
24)	Chlordane-2	0.000	5.468f	0	291646	N.D.	0.613 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
Data File : PD062394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2021 23:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 07:02:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

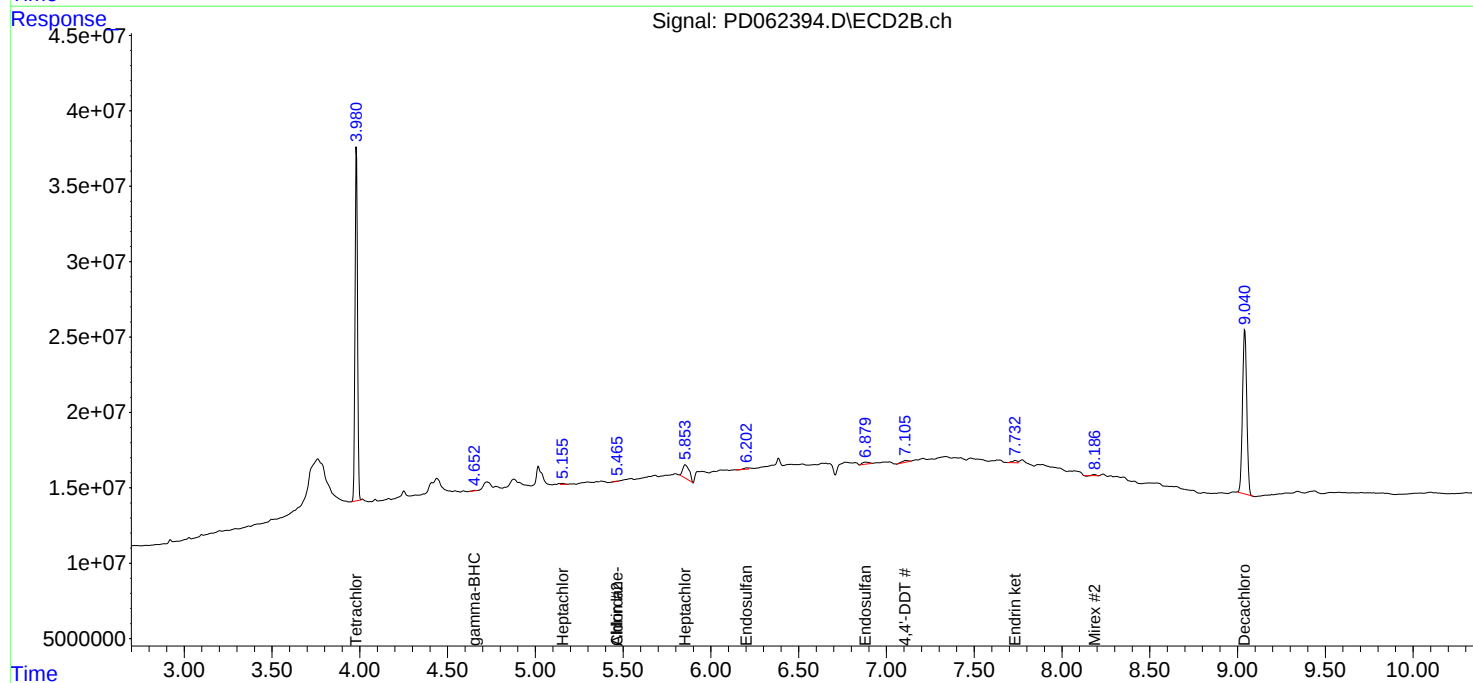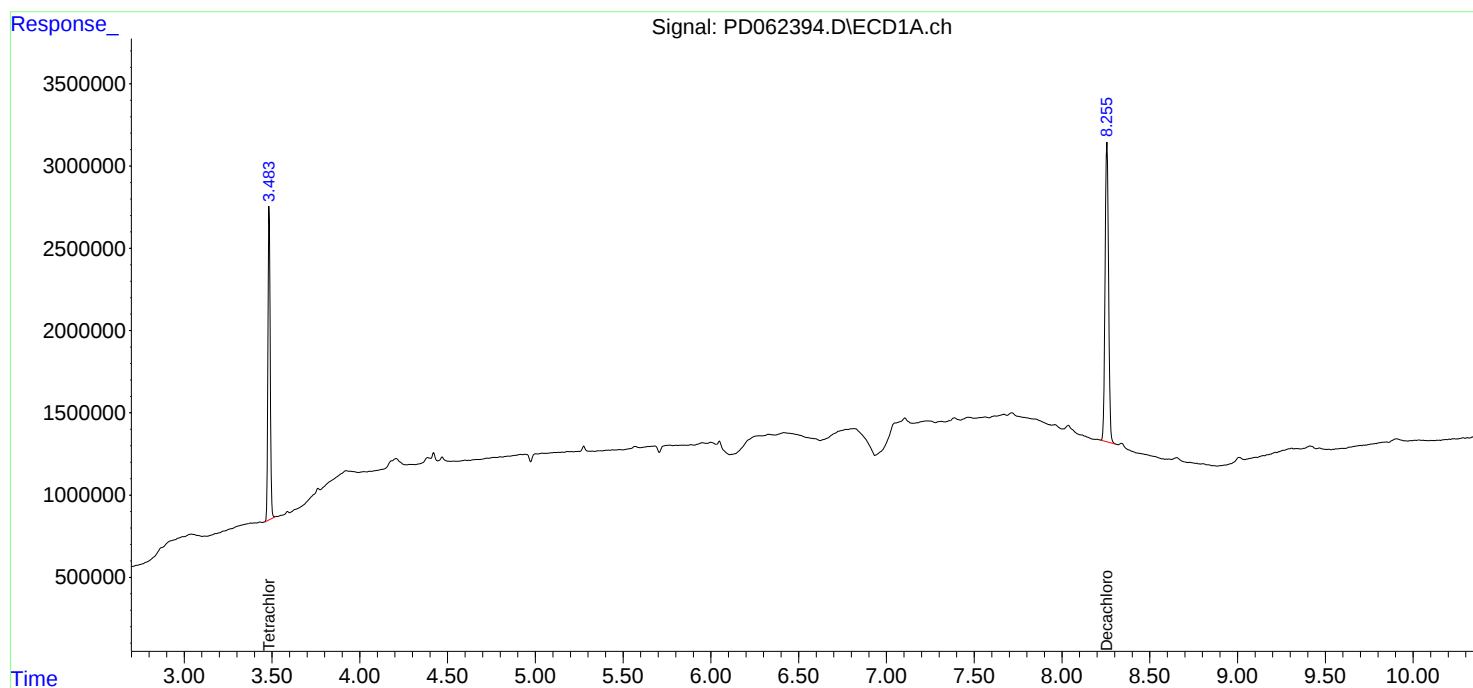

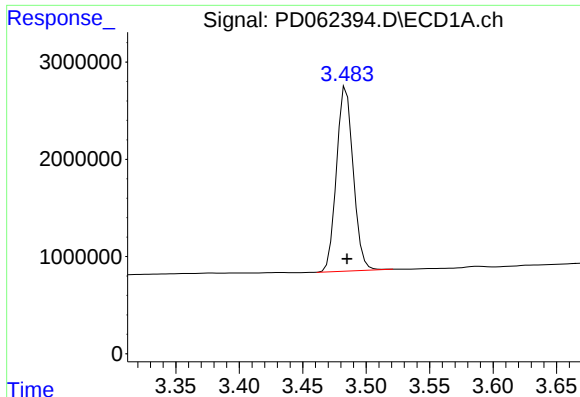


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 17479273
Conc: 21.46 ng/ml

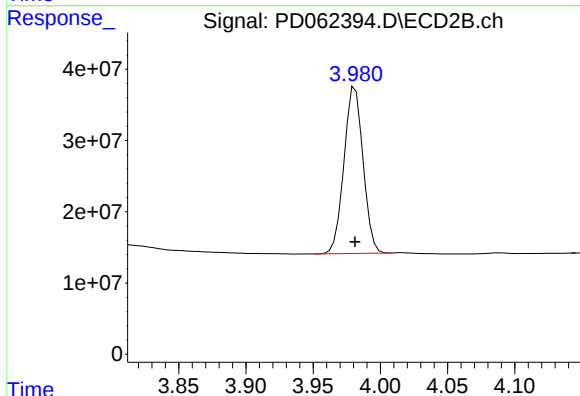


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 230502735
Conc: 21.89 ng/ml

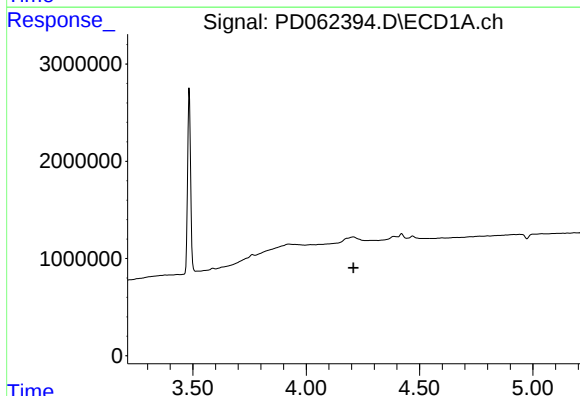


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.209 min
Response: 0
Conc: N.D.

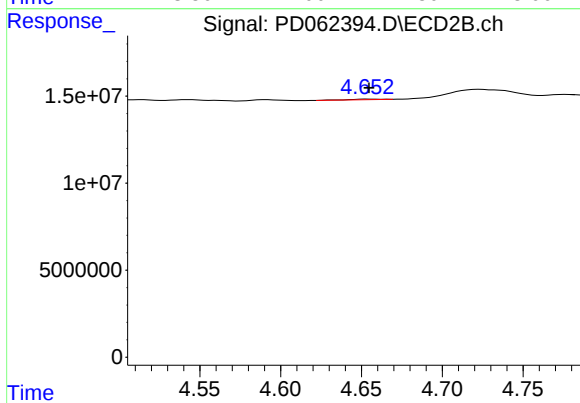


#3 gamma-BHC (Lindane)

R.T.: 4.653 min
Delta R.T.: -0.001 min
Response: 434511
Conc: 0.03 ng/ml

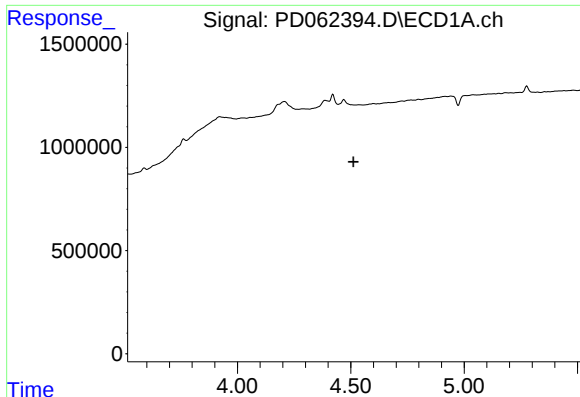


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.512 min
Response: 0
Conc: N.D.

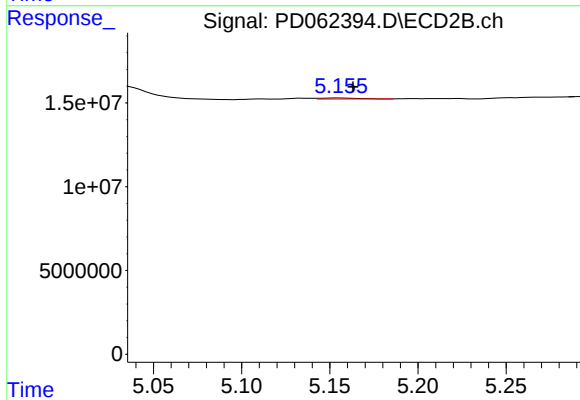


#4 Heptachlor

R.T.: 5.156 min
Delta R.T.: -0.007 min
Response: 974590
Conc: 0.06 ng/ml

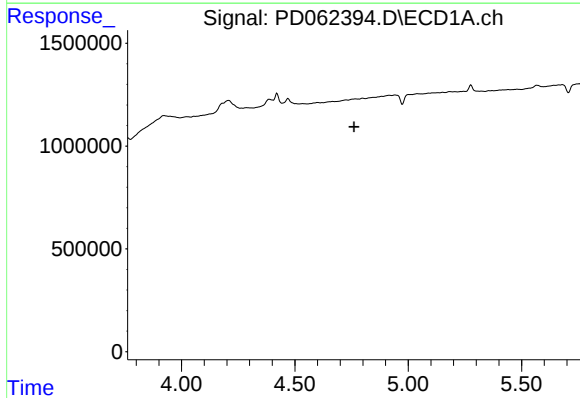


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.762 min
Response: 0
Conc: N.D.

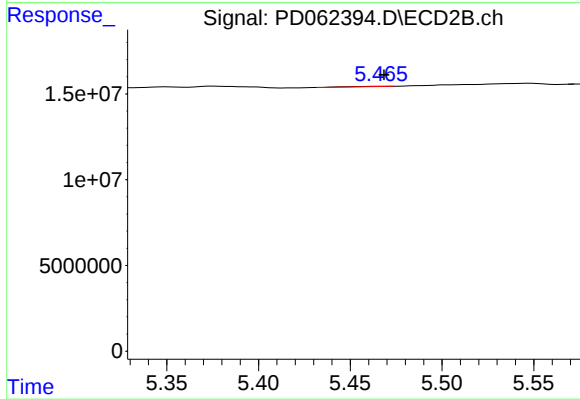


#5 Aldrin

R.T.: 5.468 min
Delta R.T.: 0.000 min
Response: 291646
Conc: 0.02 ng/ml

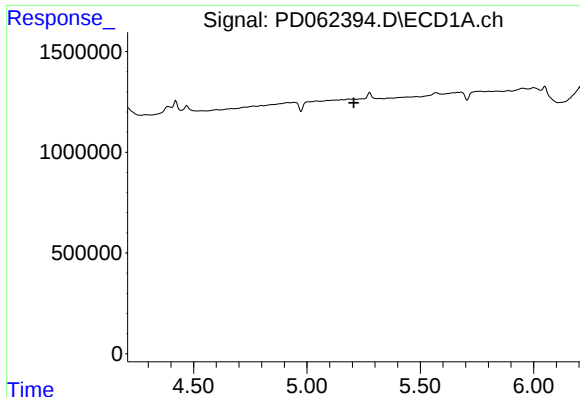


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.206 min
Response: 0
Conc: N.D.

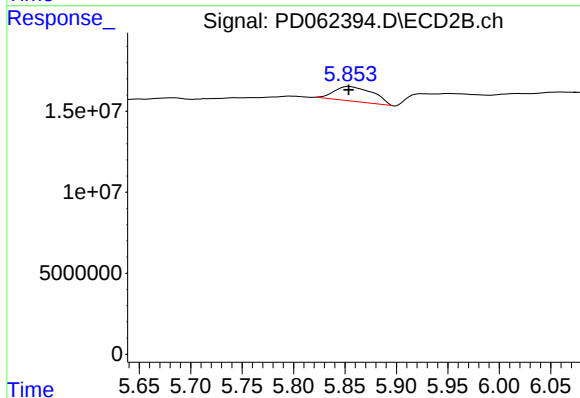


#8 Heptachlor epoxide

R.T.: 5.854 min
Delta R.T.: 0.000 min
Response: 23200132
Conc: 1.69 ng/ml

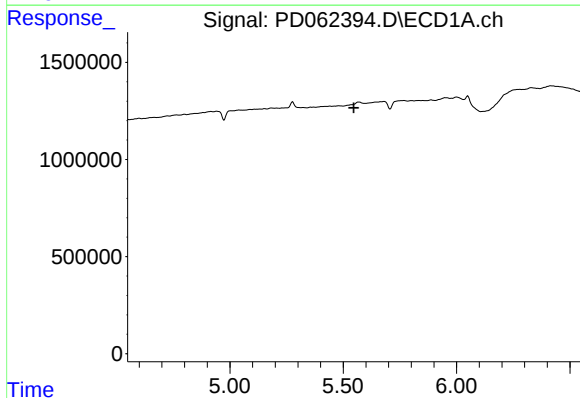


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.547 min
Response: 0
Conc: N.D.

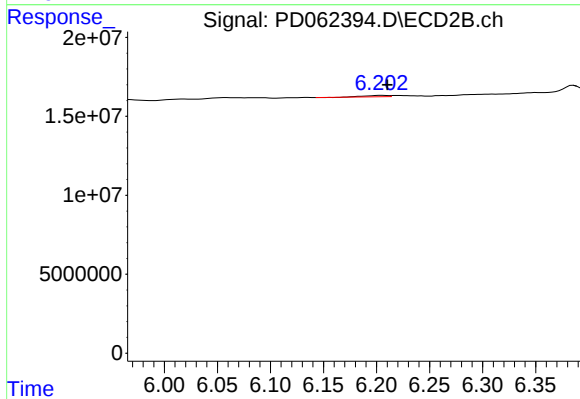


#9 Endosulfan I

R.T.: 6.204 min
Delta R.T.: -0.006 min
Response: 1312655
Conc: 0.10 ng/ml

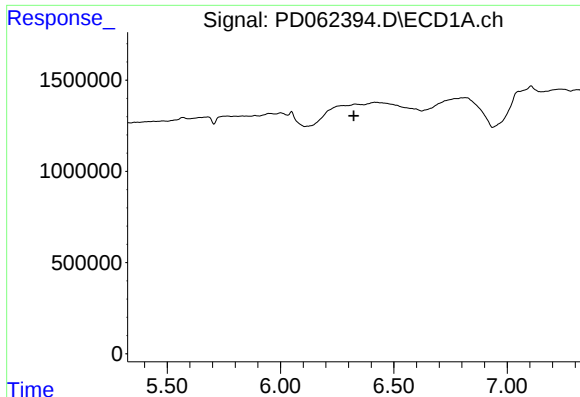


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

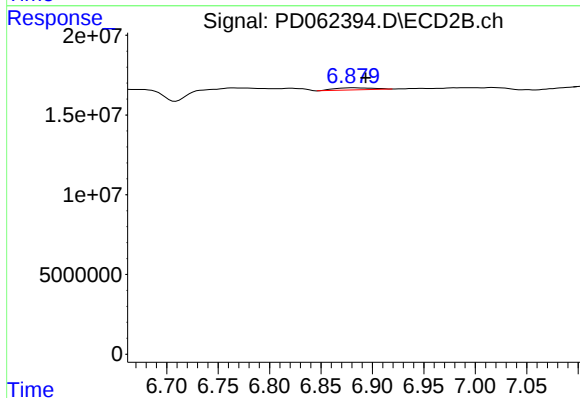


#15 Endosulfan II

R.T.: 6.881 min
Delta R.T.: -0.012 min
Response: 3480725
Conc: 0.30 ng/ml

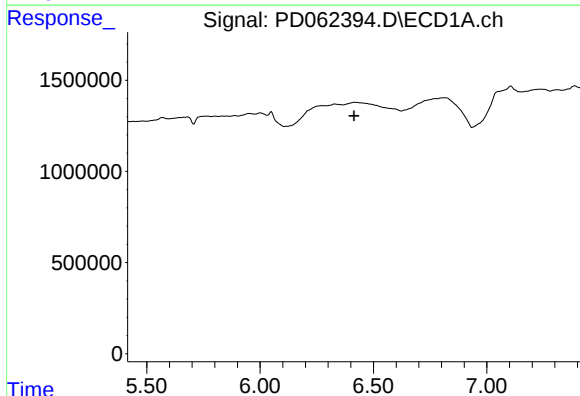


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.415 min
Response: 0
Conc: N.D.

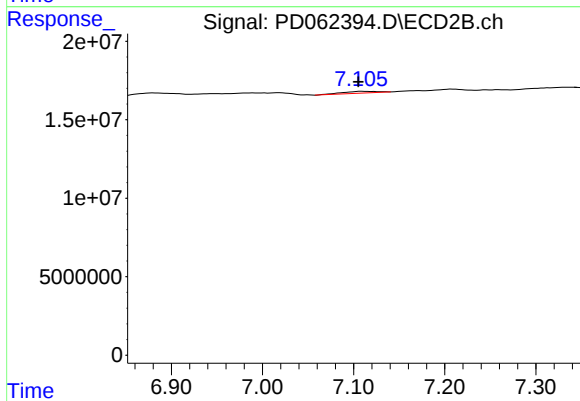


#17 4,4'-DDT

R.T.: 7.108 min
Delta R.T.: 0.003 min
Response: 2842705
Conc: 0.29 ng/ml

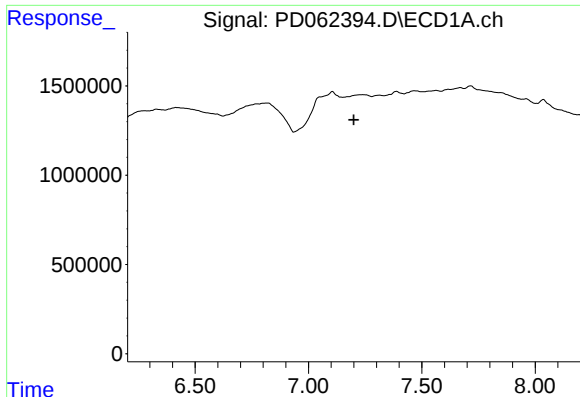


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

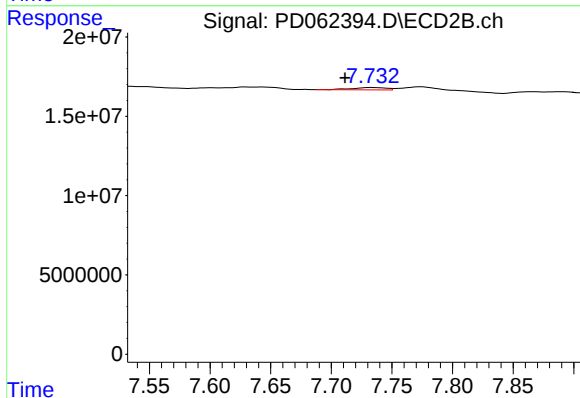


#21 Endrin ketone

R.T.: 7.734 min
Delta R.T.: 0.022 min
Response: 2833122
Conc: 0.28 ng/ml

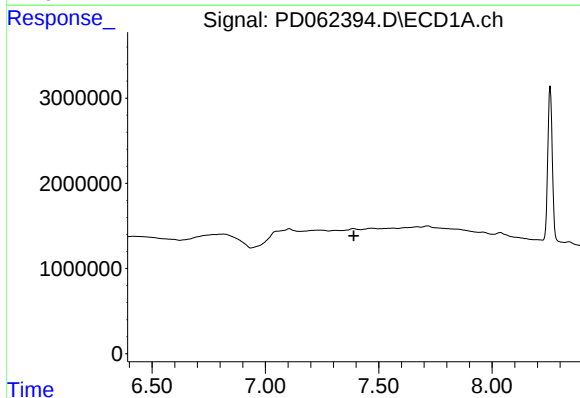


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.390 min
Response: 0
Conc: N.D.

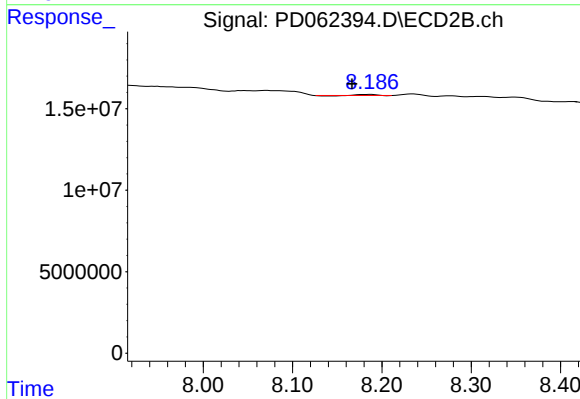


#22 Mirex

R.T.: 8.187 min
Delta R.T.: 0.021 min
Response: 700135
Conc: 0.11 ng/ml

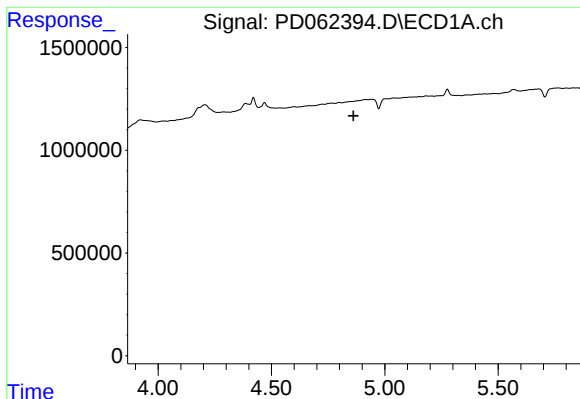


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.862 min
Response: 0
Conc: N.D.

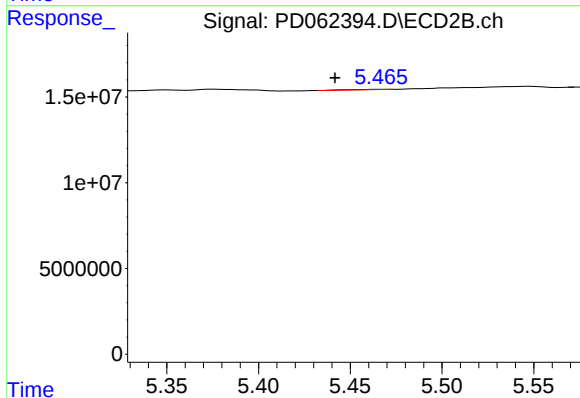


#24 Chlordane-2

R.T.: 5.468 min
Delta R.T.: 0.027 min
Response: 291646
Conc: 0.61 ng/ml

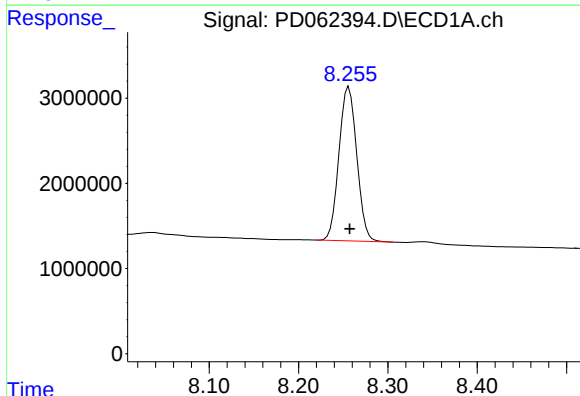

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.001 min
Response: 25077321
Conc: 20.67 ng/ml

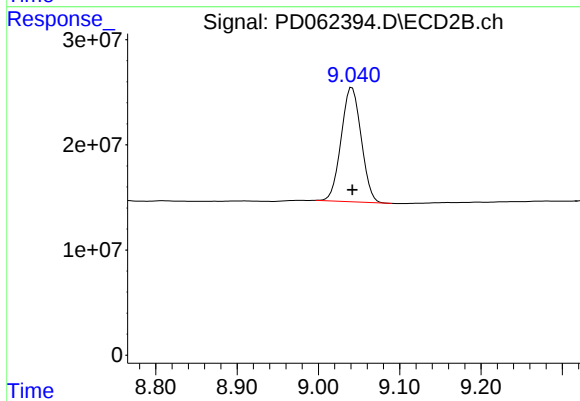

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 184985113
Conc: 21.80 ng/ml