

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042621\
 Data File : PL066464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2021 15:43
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 02:44:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 27 02:36:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds



Target Compounds						
8) B	Heptachlo...	0.000	6.068	0	5242846	N.D. 1.417 #
13) MA	Dieldrin	5.694	0.000	4940430	0	1.018 N.D. #
14) MA	Endrin	5.956	0.000	3637574	0	0.835 N.D. #
21) B	Endrin ke...	0.000	7.972	0	1219943	N.D. 0.344 #
23)	Chlordane-1	4.292	0.000	1486018	0	10.485 N.D. #
24)	Chlordane-2	0.000	5.647	0	18941965	N.D. 112.796 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042621\
Data File : PL066464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2021 15:43
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 02:44:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Tue Apr 27 02:36:03 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

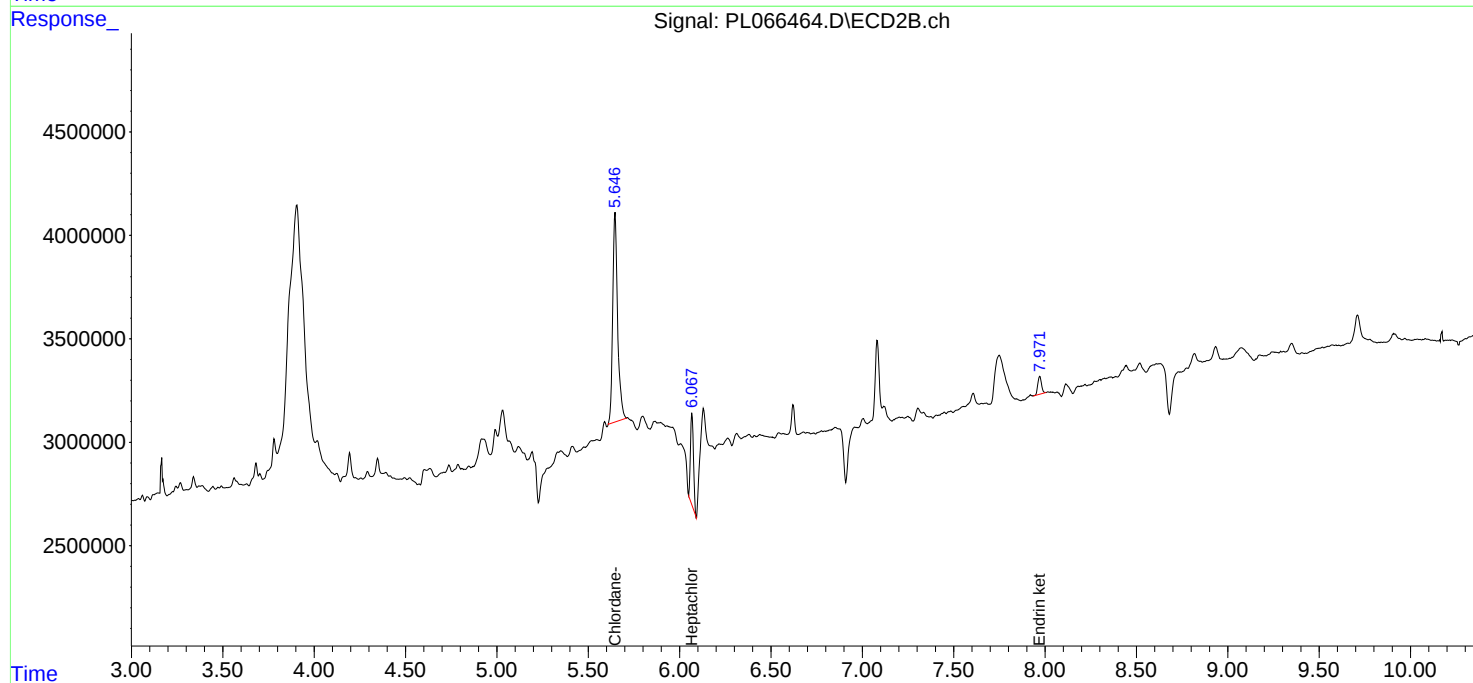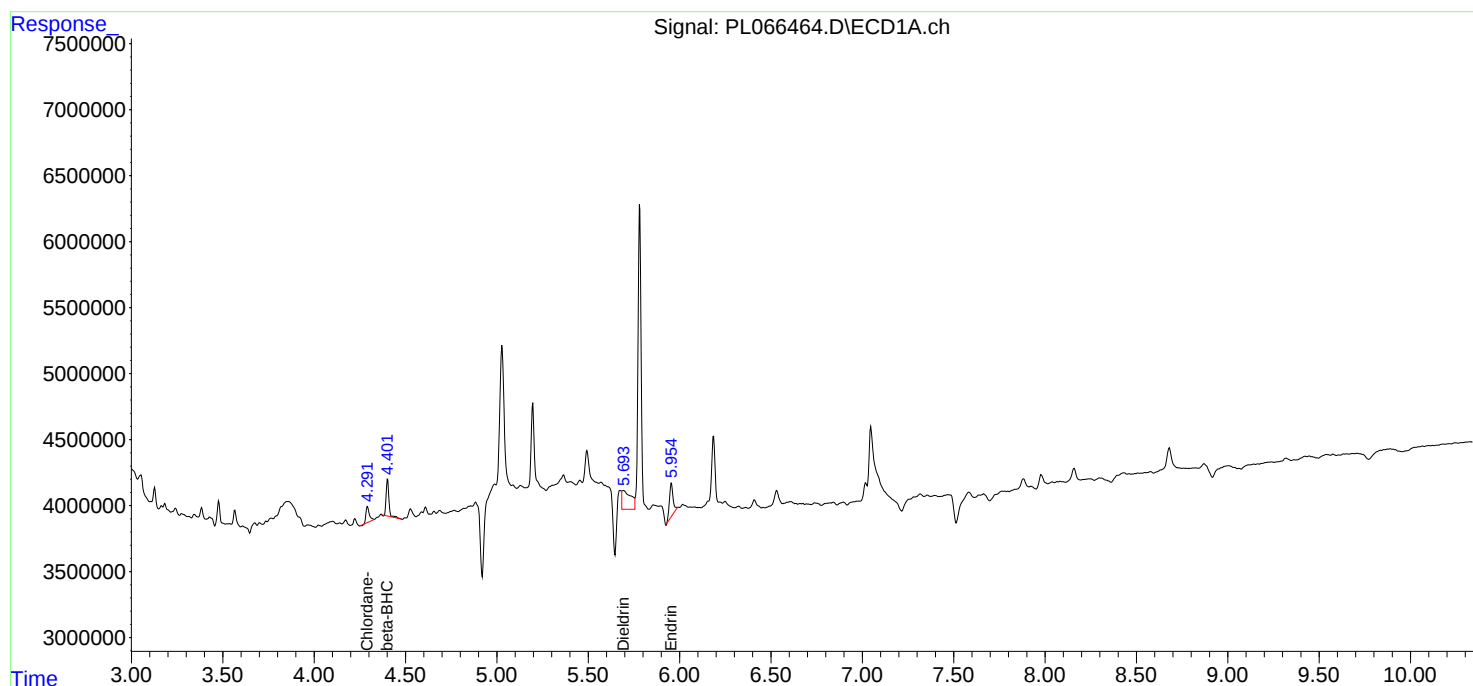

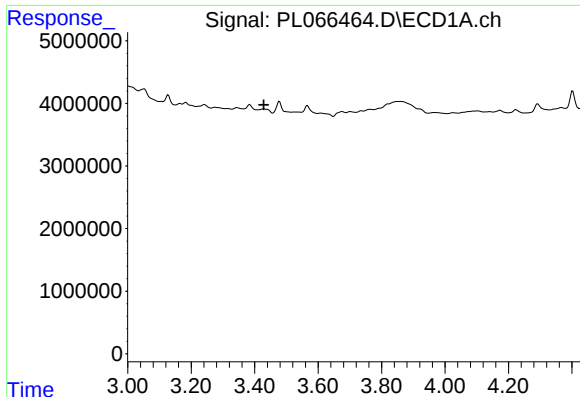


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.429 min
Response: 0
Conc: N.D.

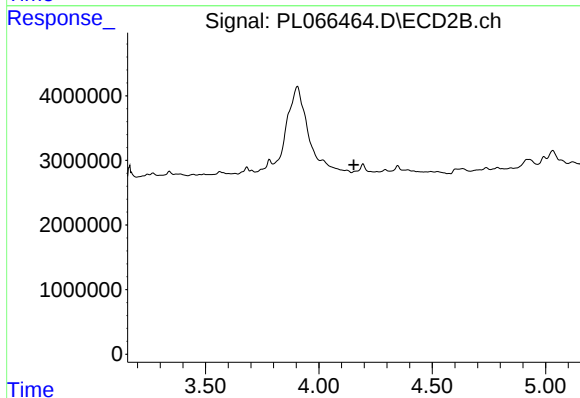


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.154 min
Response: 0
Conc: N.D.

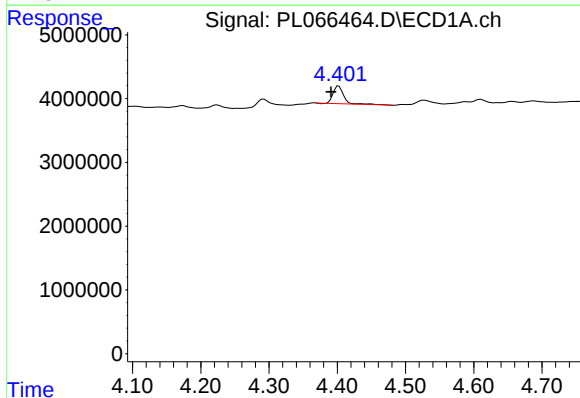


#6 beta-BHC

R.T.: 4.402 min
Delta R.T.: 0.011 min
Response: 2989145
Conc: 1.13 ng/ml

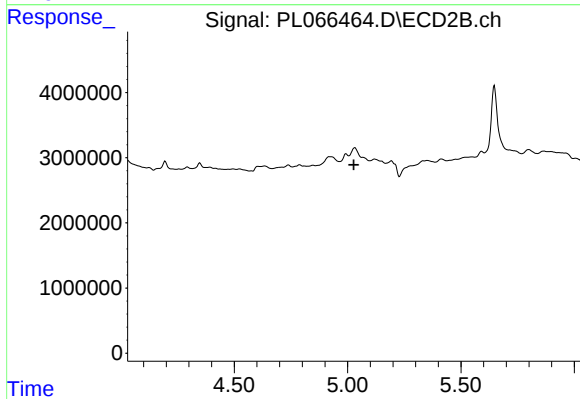


#6 beta-BHC

R.T.: 5.032 min
Delta R.T.: 0.005 min
Response: 1812242
Conc: N.D.

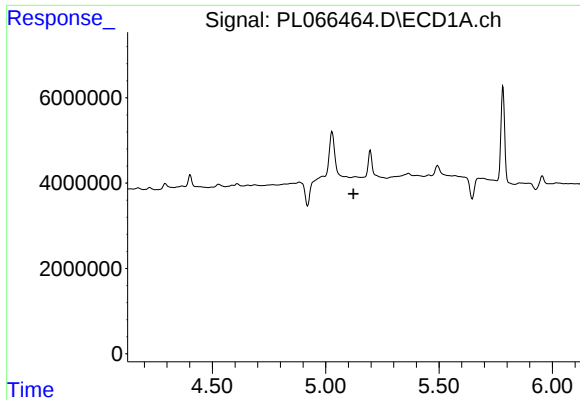


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.123 min
Response: 0
Conc: N.D.

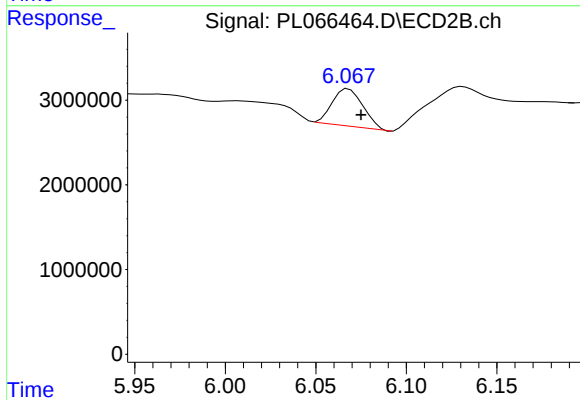


#8 Heptachlor epoxide

R.T.: 6.068 min
Delta R.T.: -0.007 min
Response: 5242846
Conc: 1.42 ng/ml

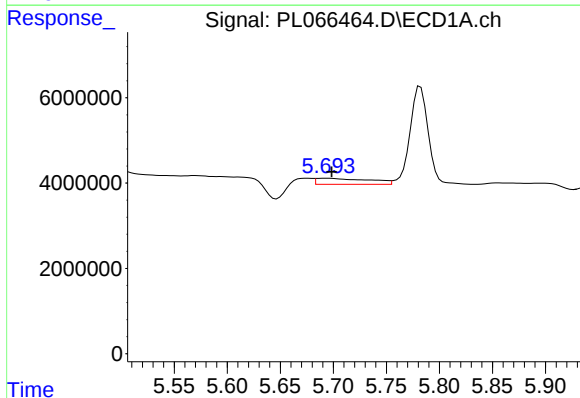


#13 Dieldrin

R.T.: 5.694 min
Delta R.T.: -0.004 min
Response: 4940430
Conc: 1.02 ng/ml

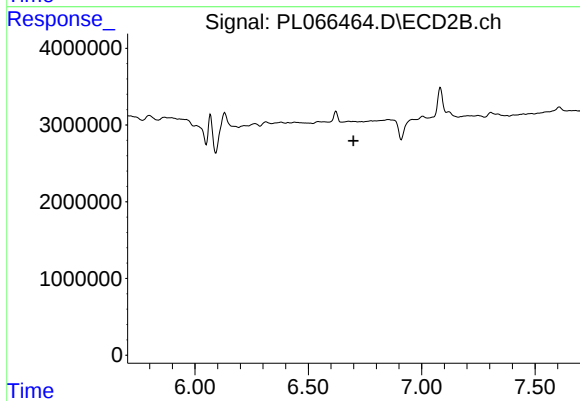


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.700 min
Response: 0
Conc: N.D.

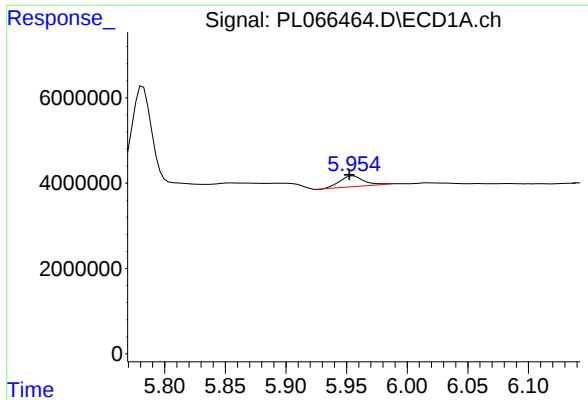


#14 Endrin

R.T.: 5.956 min
Delta R.T.: 0.003 min
Response: 3637574
Conc: 0.84 ng/ml

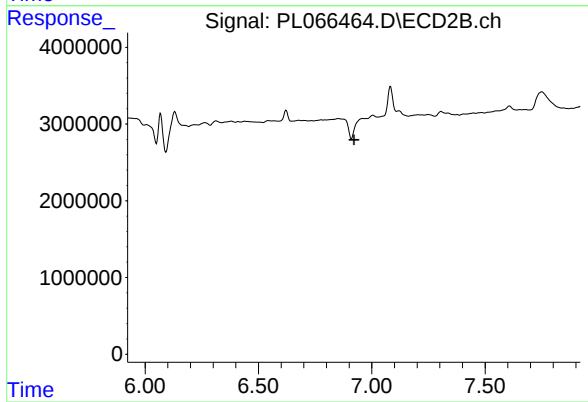


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

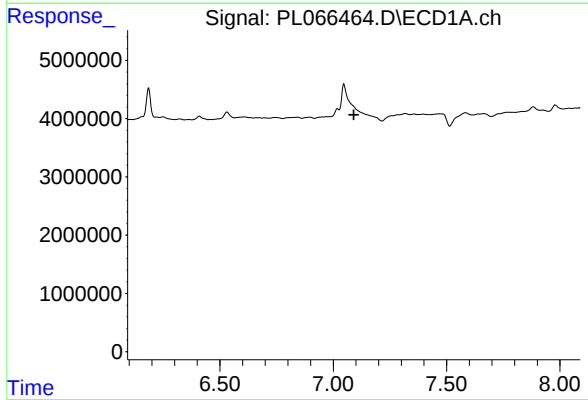


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.090 min
Response: 0
Conc: N.D.

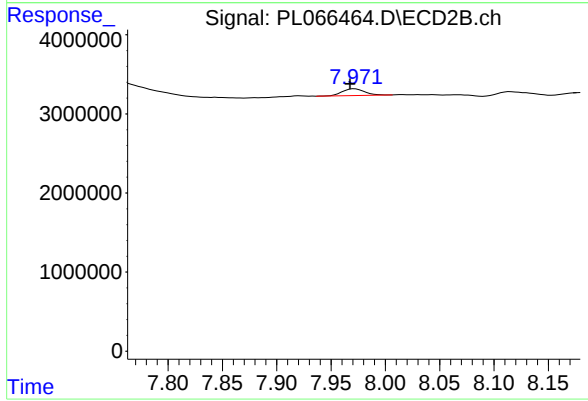


#21 Endrin ketone

R.T.: 7.972 min
Delta R.T.: 0.004 min
Response: 1219943
Conc: 0.34 ng/ml

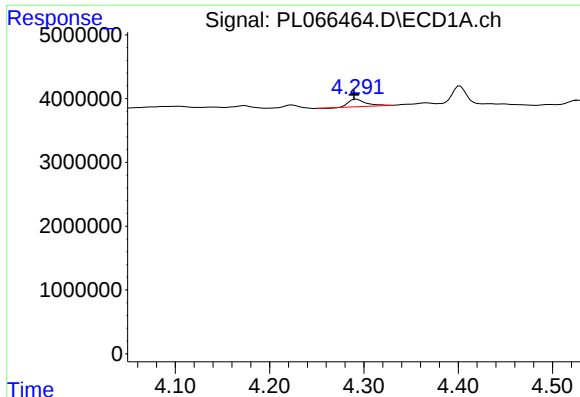


#23 Chlordane-1

R.T.: 4.292 min
Delta R.T.: 0.002 min
Response: 1486018
Conc: 10.48 ng/ml

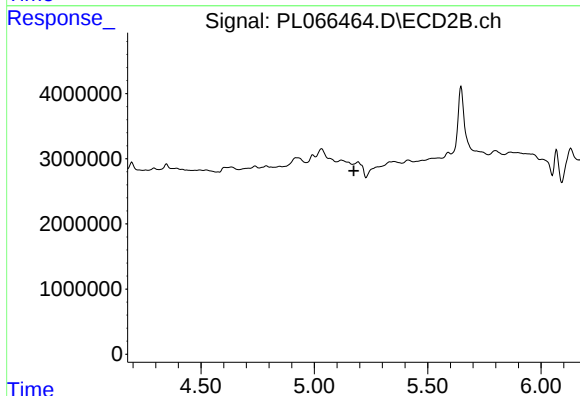


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

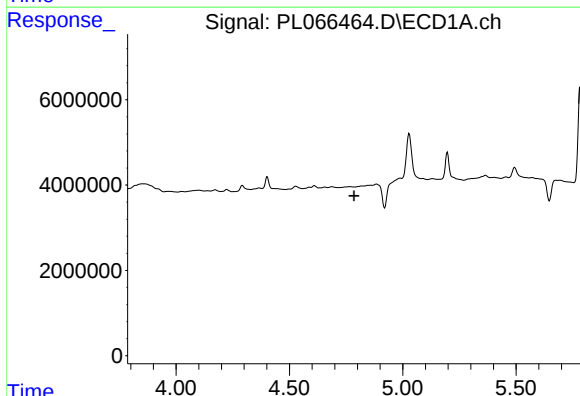


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.786 min
Response: 0
Conc: N.D.

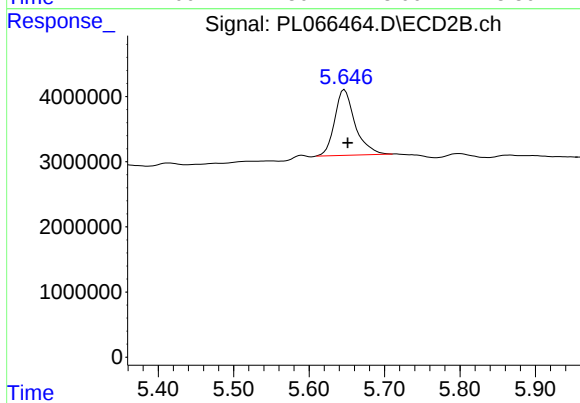


#24 Chlordane-2

R.T.: 5.647 min
Delta R.T.: -0.004 min
Response: 18941965
Conc: 112.80 ng/ml

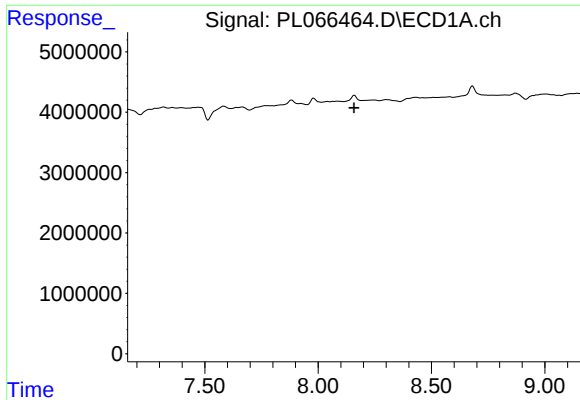

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.159 min
Response: 0
Conc: N.D.

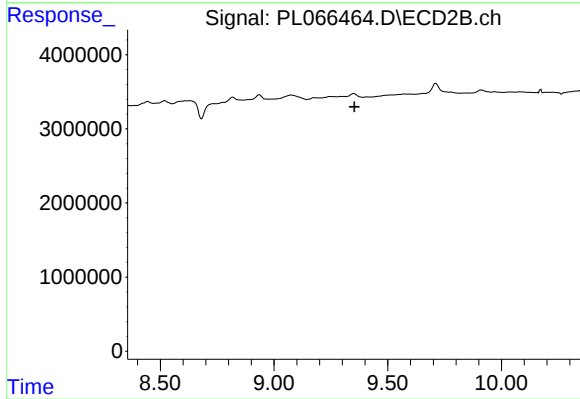

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.353 min
Response: 0
Conc: N.D.