

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
 Data File : PD062371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2021 18:17
 Operator : AR\AJ
 Sample : M2149-09
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-38-9.5-10.0

Manual Integrations
 APPROVED

Ankita
 4/27/2021 10:53:22 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 06:56:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.981	9224514	124.4E6	11.326	11.809
28)	SA Decachlor...	8.257	9.042	20643970	150.3E6	17.019	17.711
Target Compounds							
12)	B 4,4'-DDE	5.643	6.330	995826	11926325	0.820m	0.845

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
Data File : PD062371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2021 18:17
Operator : AR\AJ
Sample : M2149-09
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SB-38-9.5-10.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:53:22 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 06:56:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

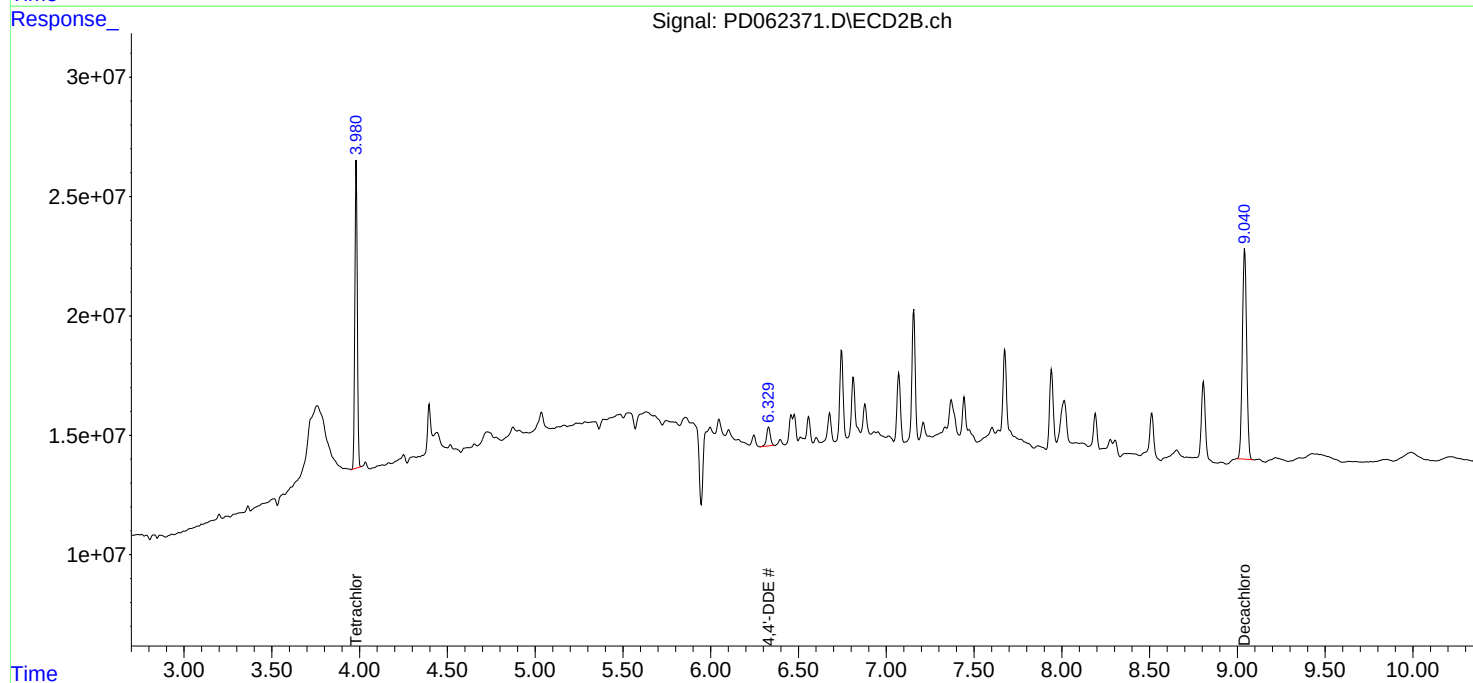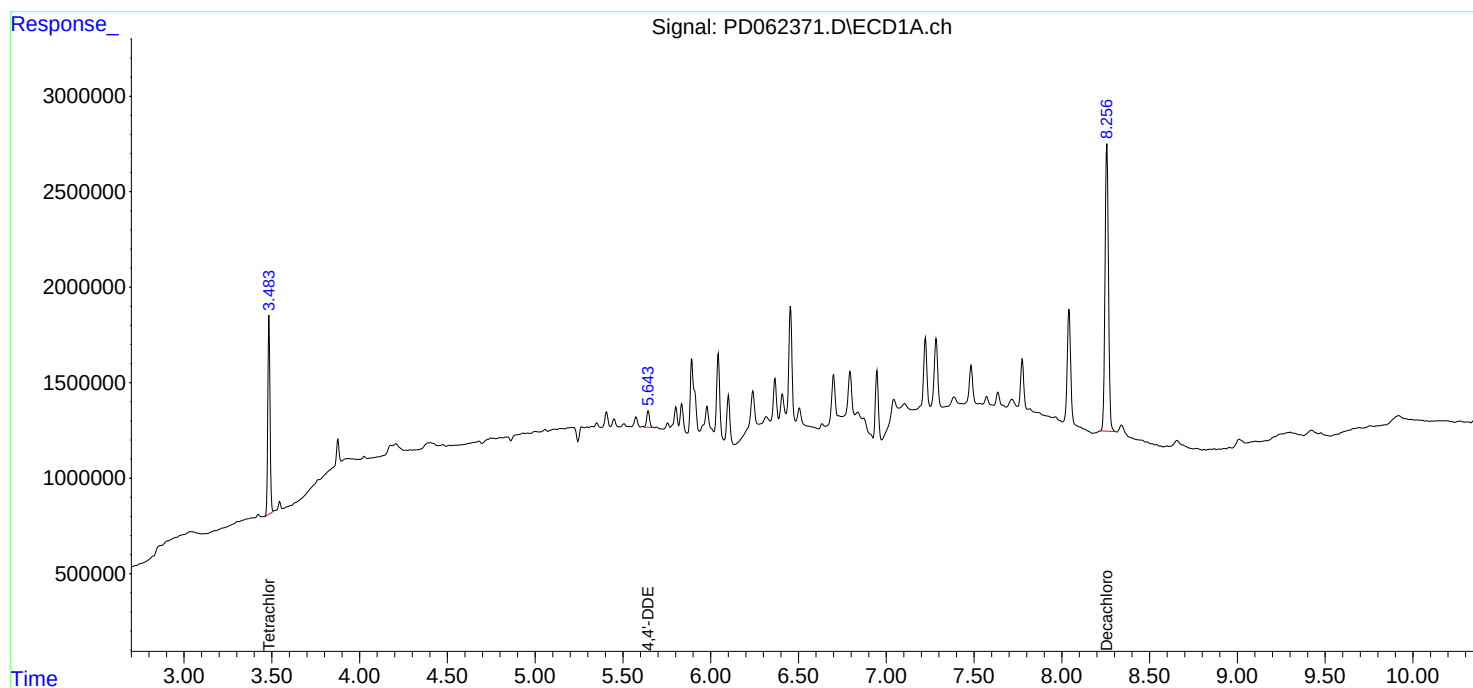

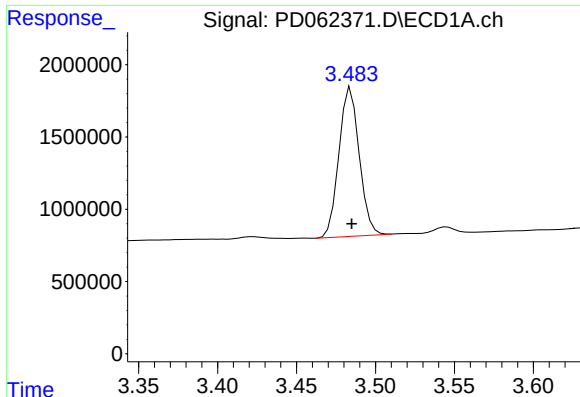


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 9224514
Conc: 11.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-38-9.5-10.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:53:22 AM

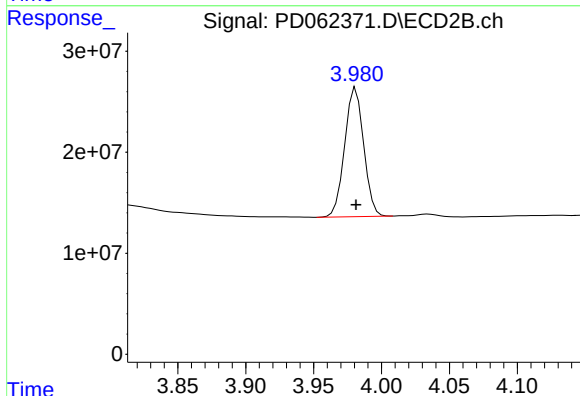


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 124365945
Conc: 11.81 ng/ml

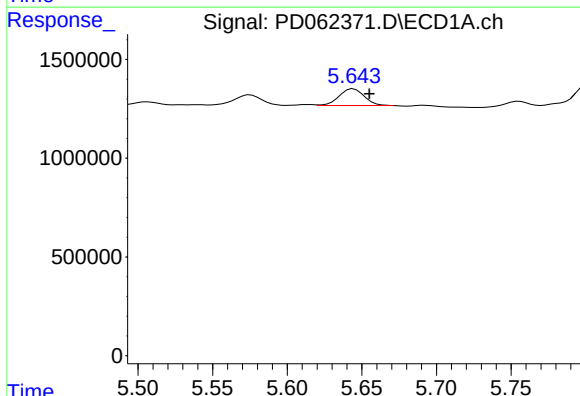


#12 4,4'-DDE

R.T.: 5.643 min
Delta R.T.: -0.012 min
Response: 995826
Conc: 0.82 ng/ml m

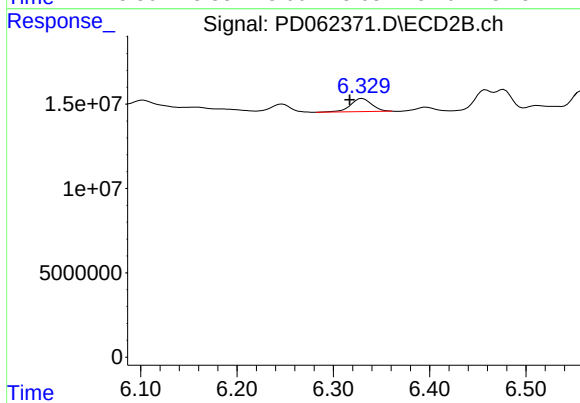

#12 4,4'-DDE

R.T.: 6.330 min
Delta R.T.: 0.013 min
Response: 11926325
Conc: 0.84 ng/ml

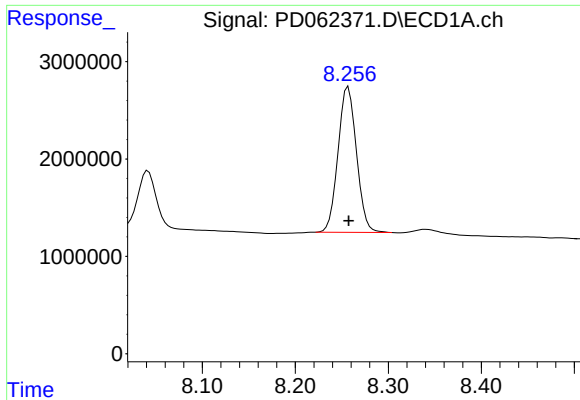


#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 20643970
Conc: 17.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-38-9.5-10.0

Manual Integrations
APPROVED

Ankita
4/27/2021 10:53:22 AM

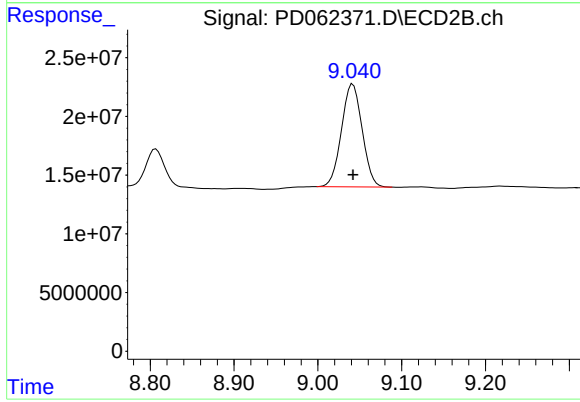

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 150276983
Conc: 17.71 ng/ml