

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
 Data File : PD062379.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2021 20:23
 Operator : AR\AJ
 Sample : M2119-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 12016

Manual Integrations
 APPROVED

Ankita
 4/27/2021 10:53:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 06:58:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.509f	3.994	9246135	73260884	11.352m	6.956m#
28) SA Decachlor...	8.260	9.047	10345145	66496354	8.528	7.837

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
Data File : PD062379.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2021 20:23
Operator : AR\AJ
Sample : M2119-01
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
12016


Manual Integrations
APPROVED

Ankita
4/27/2021 10:53:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 06:58:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

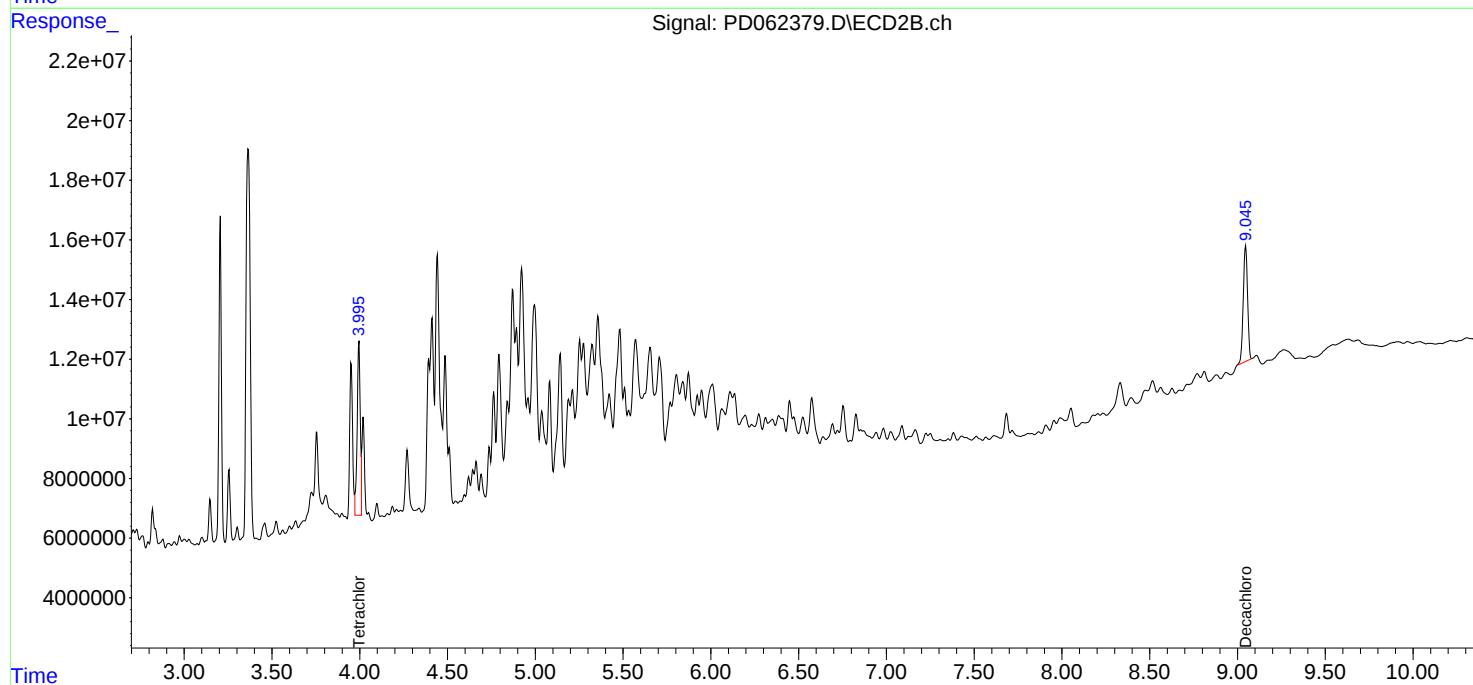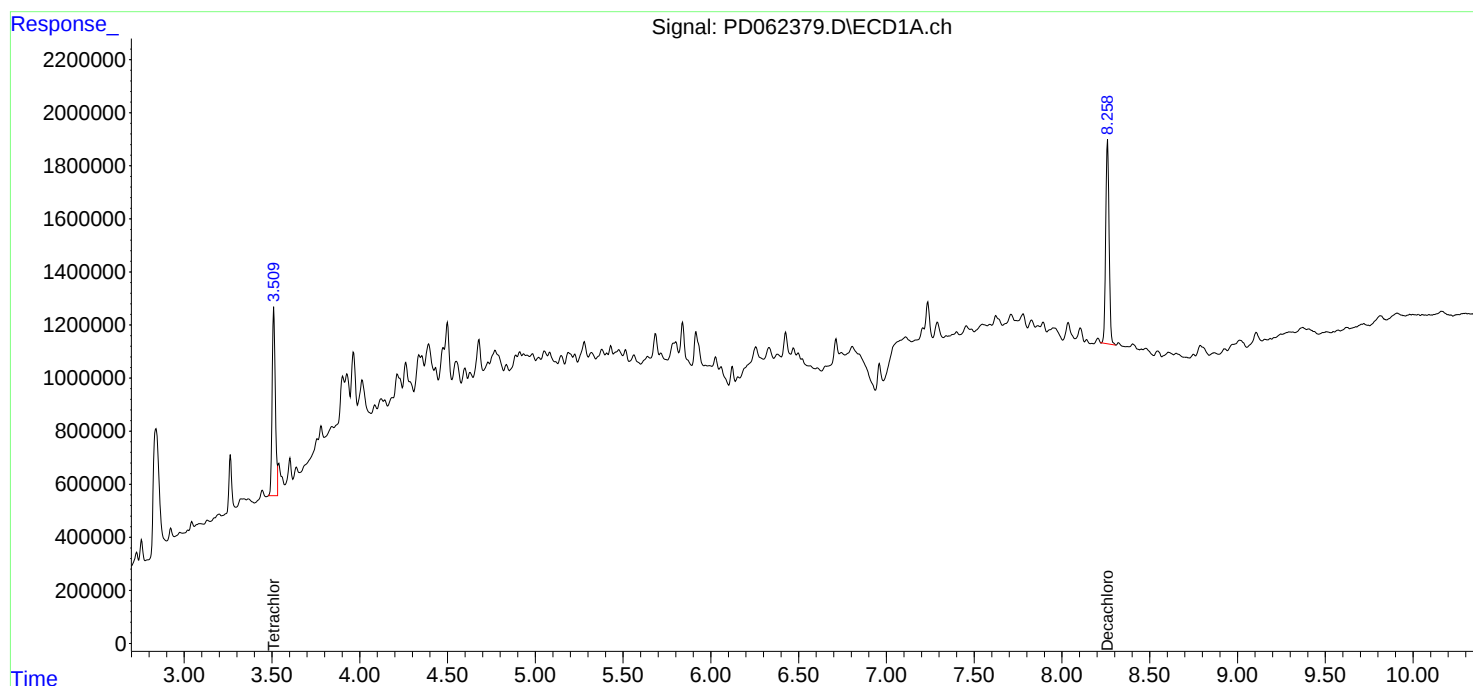

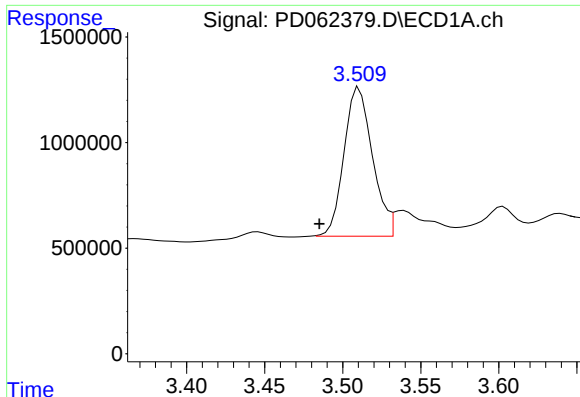


#1 Tetrachloro-m-xylene

R.T.: 3.509 min
Delta R.T.: 0.024 min
Response: 9246135
Conc: 11.35 ng/ml m

Instrument :
ECD_D
ClientSampleId :
12016


Manual Integrations
APPROVED

Ankita
4/27/2021 10:53:29 AM

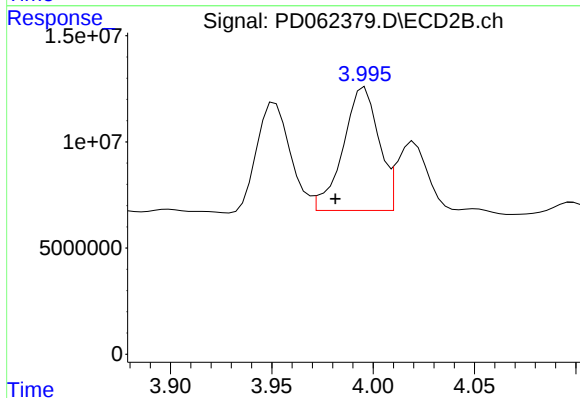


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: 0.013 min
Response: 73260884
Conc: 6.96 ng/ml m

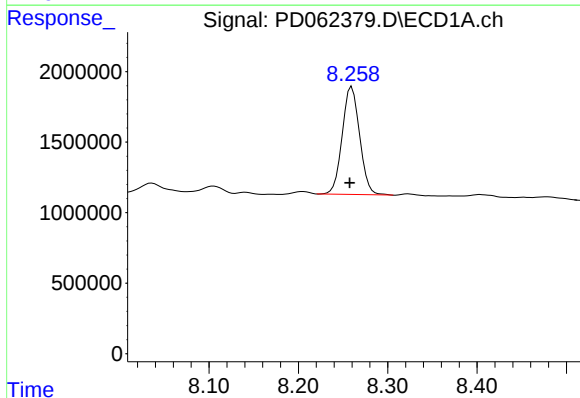

#28 Decachlorobiphenyl

R.T.: 8.260 min
Delta R.T.: 0.002 min
Response: 10345145
Conc: 8.53 ng/ml

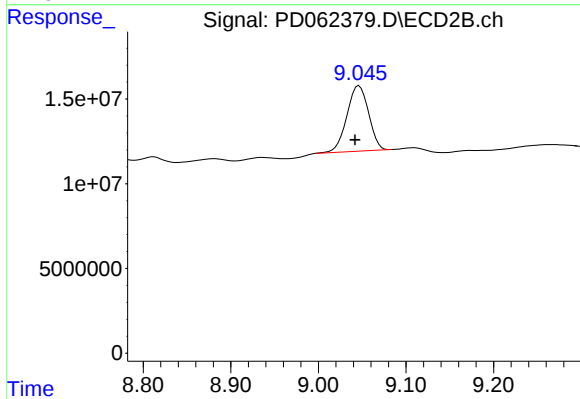

#28 Decachlorobiphenyl

R.T.: 9.047 min
Delta R.T.: 0.005 min
Response: 66496354
Conc: 7.84 ng/ml