

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
 Data File : PD062393.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2021 23:38
 Operator : AR\AJ
 Sample : M2150-07
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EQUIP-BLANK

Manual Integrations
 APPROVED

Ankita
 4/27/2021 10:53:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 07:01:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.484	3.980	16075000	208.9E6	19.736	19.839m
28) SA Decachlor...	8.256	9.042	17597586	130.6E6	14.507	15.388

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
Data File : PD062393.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2021 23:38
Operator : AR\AJ
Sample : M2150-07
Misc :
ALS Vial : 57 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampled :
EQUIP-BLANK


Manual Integrations
APPROVED

Ankita
4/27/2021 10:53:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 07:01:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

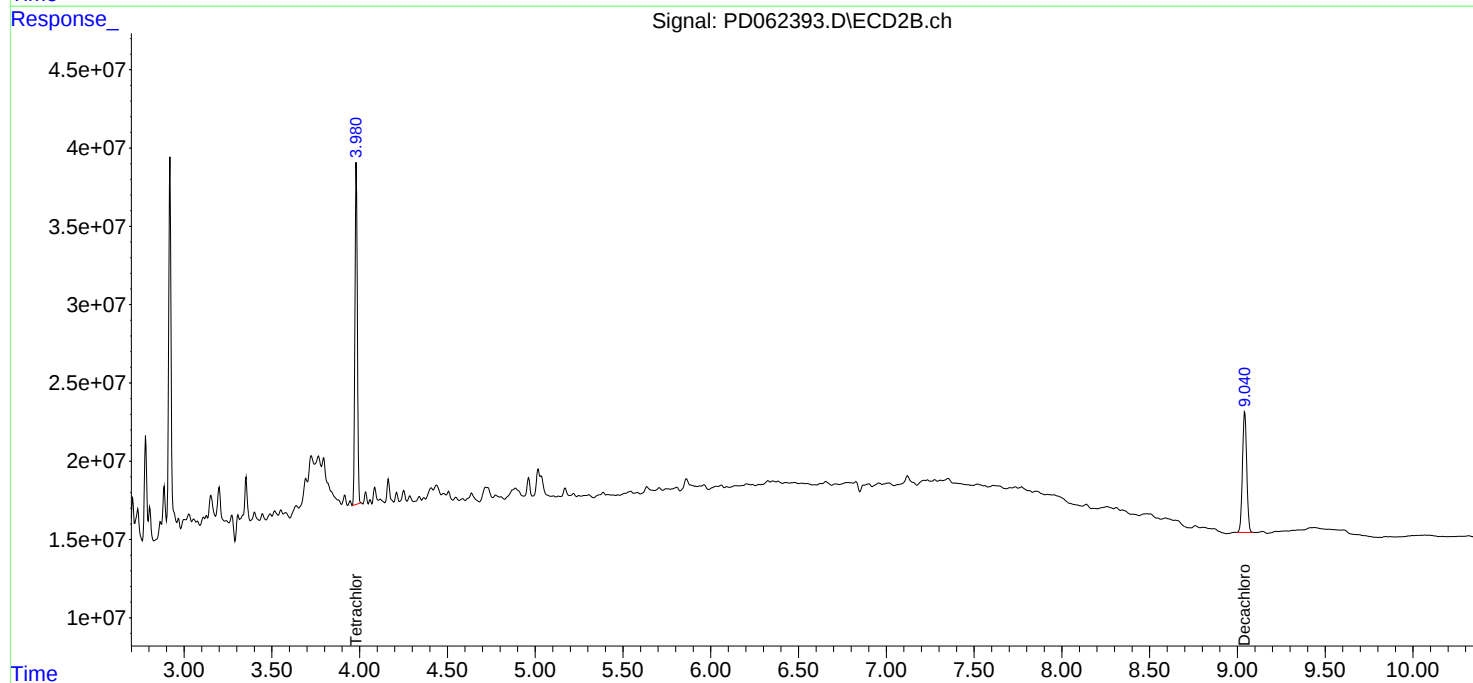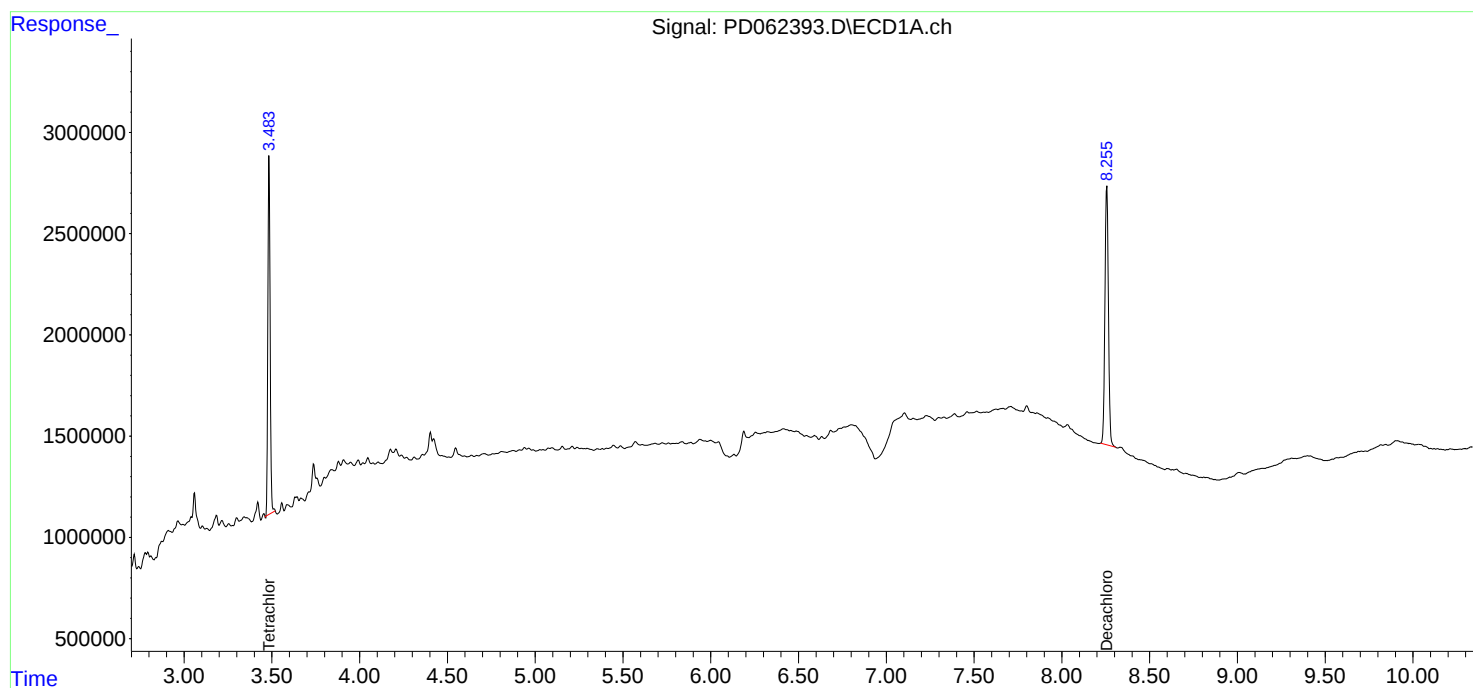

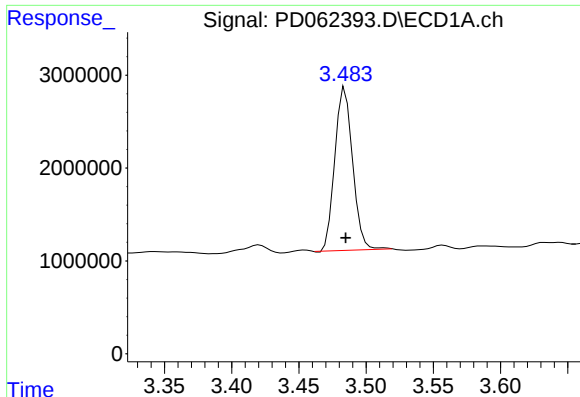


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 16075000
Conc: 19.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
EQUIP-BLANK


Manual Integrations
APPROVED

Ankita
4/27/2021 10:53:36 AM

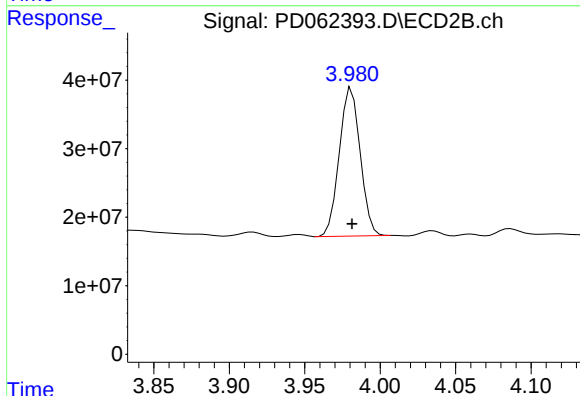


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 208929643
Conc: 19.84 ng/ml m

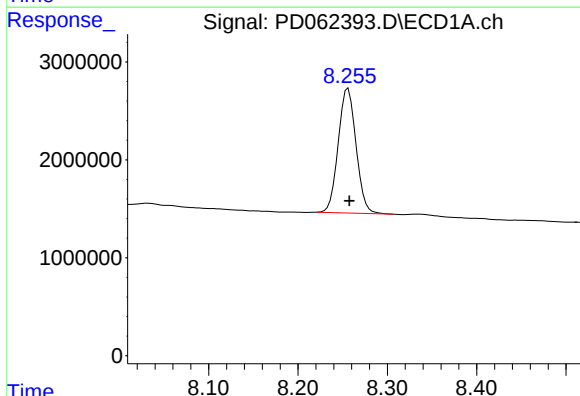

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.001 min
Response: 17597586
Conc: 14.51 ng/ml

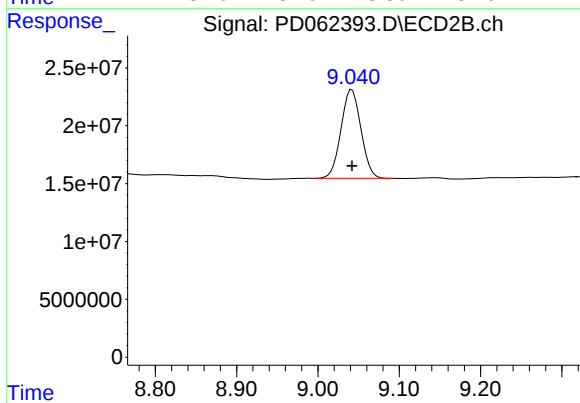

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 130569325
Conc: 15.39 ng/ml