

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
 Data File : PD062396.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2021 00:34
 Operator : AR\AJ
 Sample : M2118-03 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 20071

Manual Integrations
 APPROVED

Ankita
 4/27/2021 10:53:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 07:02:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.484	3.979	1060296	15693305	1.302m	1.490m
28) SA Decachlor...	8.257	9.041	1490801	9307058	1.229m	1.097
Target Compounds						
17) MA 4,4'-DDT	6.413	7.111	3866224	20609089	3.786	2.067 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042421\
Data File : PD062396.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2021 00:34
Operator : AR\AJ
Sample : M2118-03 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
20071


Manual Integrations
APPROVED

Ankita
4/27/2021 10:53:45 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 07:02:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

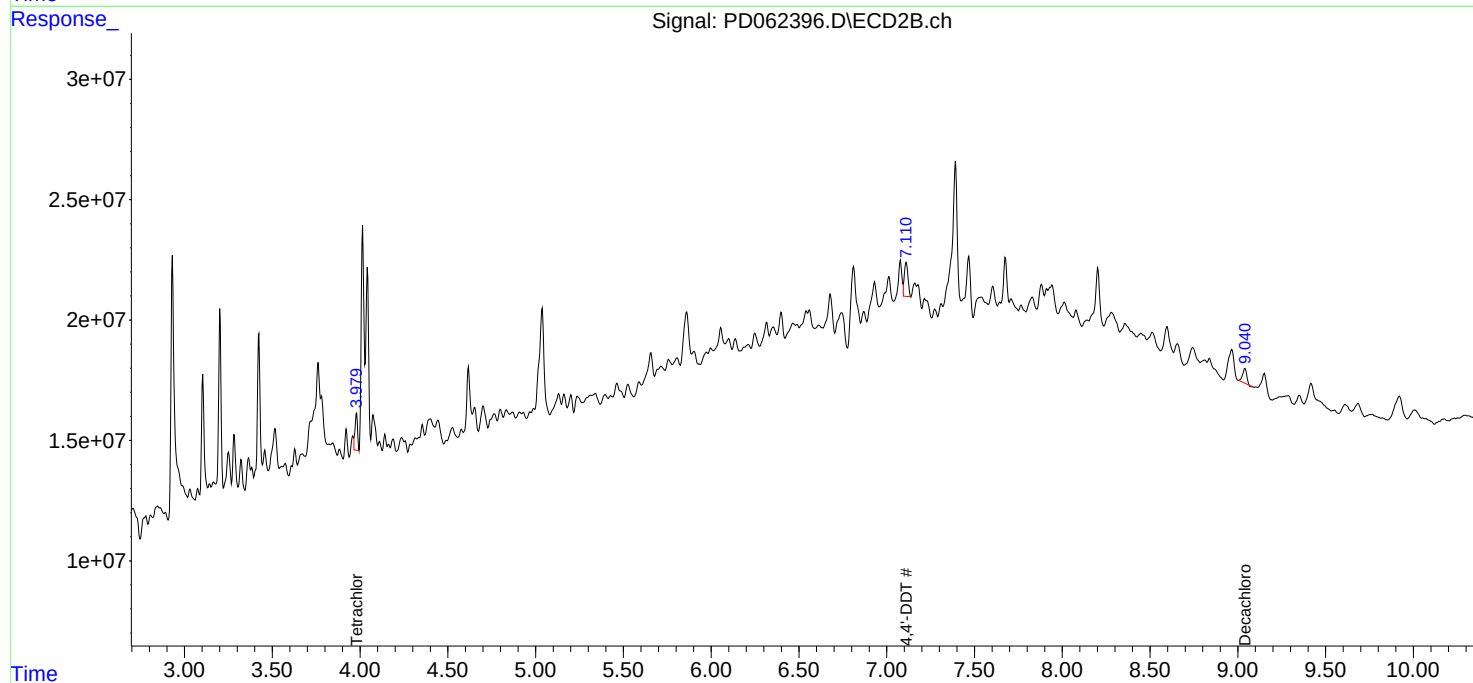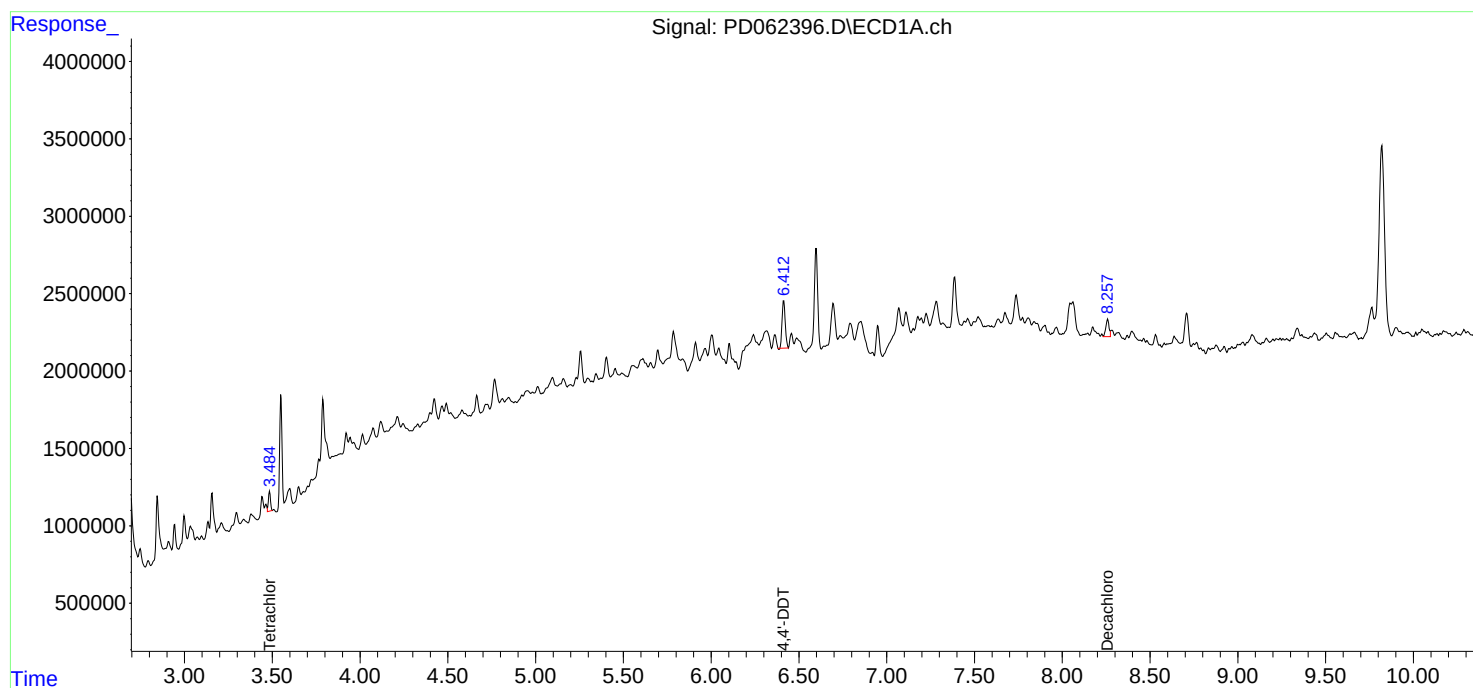

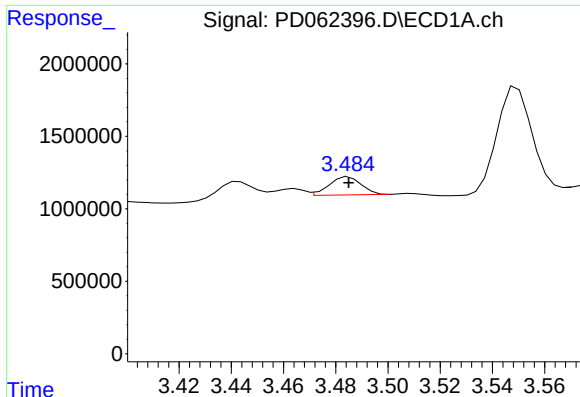


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: -0.001 min
Response: 1060296
Conc: 1.30 ng/ml m

Instrument :
ECD_D
ClientSampleId :
20071


Manual Integrations
APPROVED

Ankita
4/27/2021 10:53:45 AM

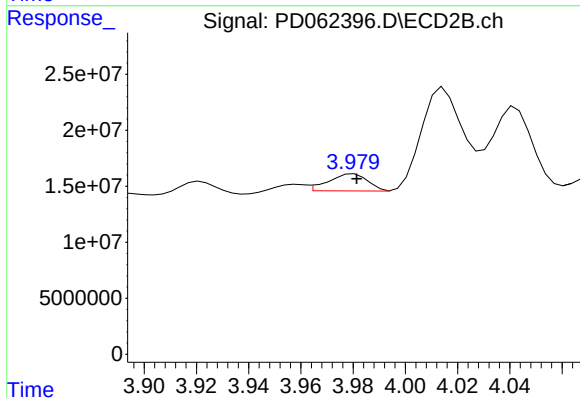


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.002 min
Response: 15693305
Conc: 1.49 ng/ml m

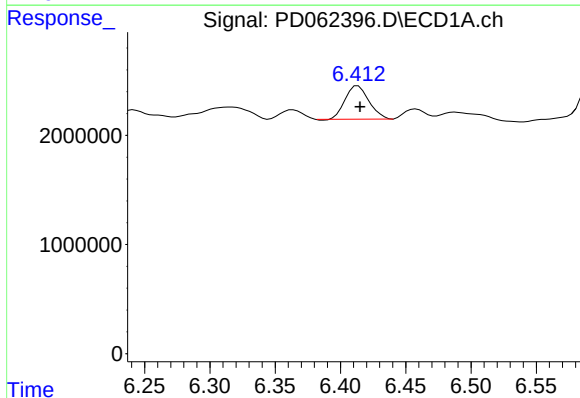


#17 4,4'-DDT

R.T.: 6.413 min
Delta R.T.: -0.002 min
Response: 3866224
Conc: 3.79 ng/ml

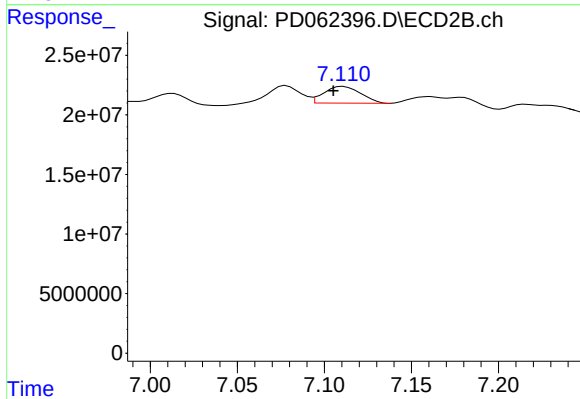

#17 4,4'-DDT

R.T.: 7.111 min
Delta R.T.: 0.006 min
Response: 20609089
Conc: 2.07 ng/ml

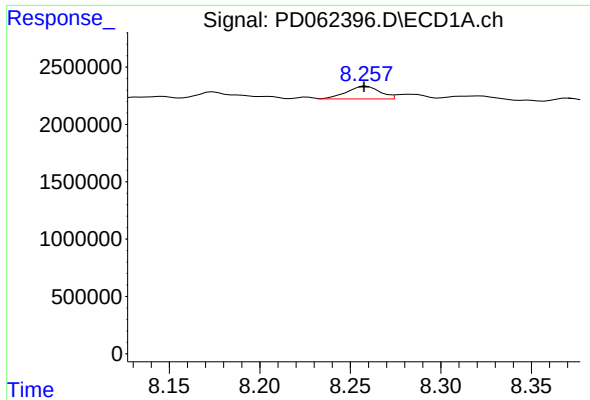


#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 1490801
Conc: 1.23 ng/ml m

Instrument :
ECD_D
ClientSampleId :
20071

Manual Integrations
APPROVED

Ankita
4/27/2021 10:53:45 AM

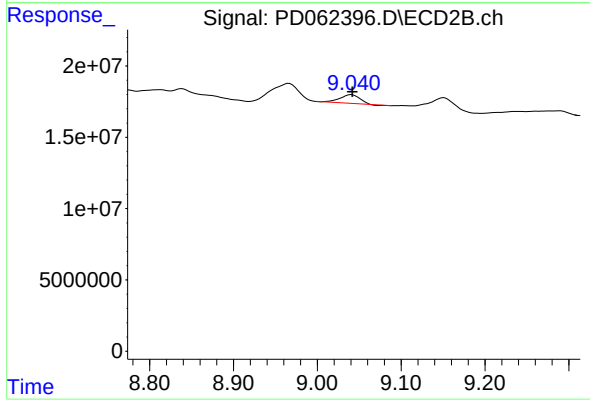

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 9307058
Conc: 1.10 ng/ml