

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042424\
 Data File : PD082581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2024 14:46
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 15:37:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042424CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 24 15:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.776	27914633	69323413	20.000	20.000
27)	SA Decachlor...	9.123	7.909	79737016	149.3E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.023	3.277	46564868	111.4E6	20.000	20.000
3)	MA gamma-BHC...	4.357	3.606	45654389	106.1E6	20.000	20.000
4)	MA Heptachlor	4.950	3.945	45866556	102.0E6	20.000	20.000
9)	A Endosulfan I	6.109	5.095	41192171	86037093	20.000	20.000
13)	MA Dieldrin	6.385	5.359	86138362	192.7E6	40.000	40.000
14)	MA Endrin	6.616	5.634	73571824	166.4E6	40.000	40.000
16)	A 4,4'-DDD	6.748	5.782	61896005	139.5E6	40.000	40.000
17)	MA 4,4'-DDT	7.064	6.033	65902857	147.5E6	40.000	40.000
20)	A Methoxychlor	7.540	6.608	180.1E6	381.2E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042424\
Data File : PD082581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2024 14:46
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 15:37:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042424CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 24 15:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

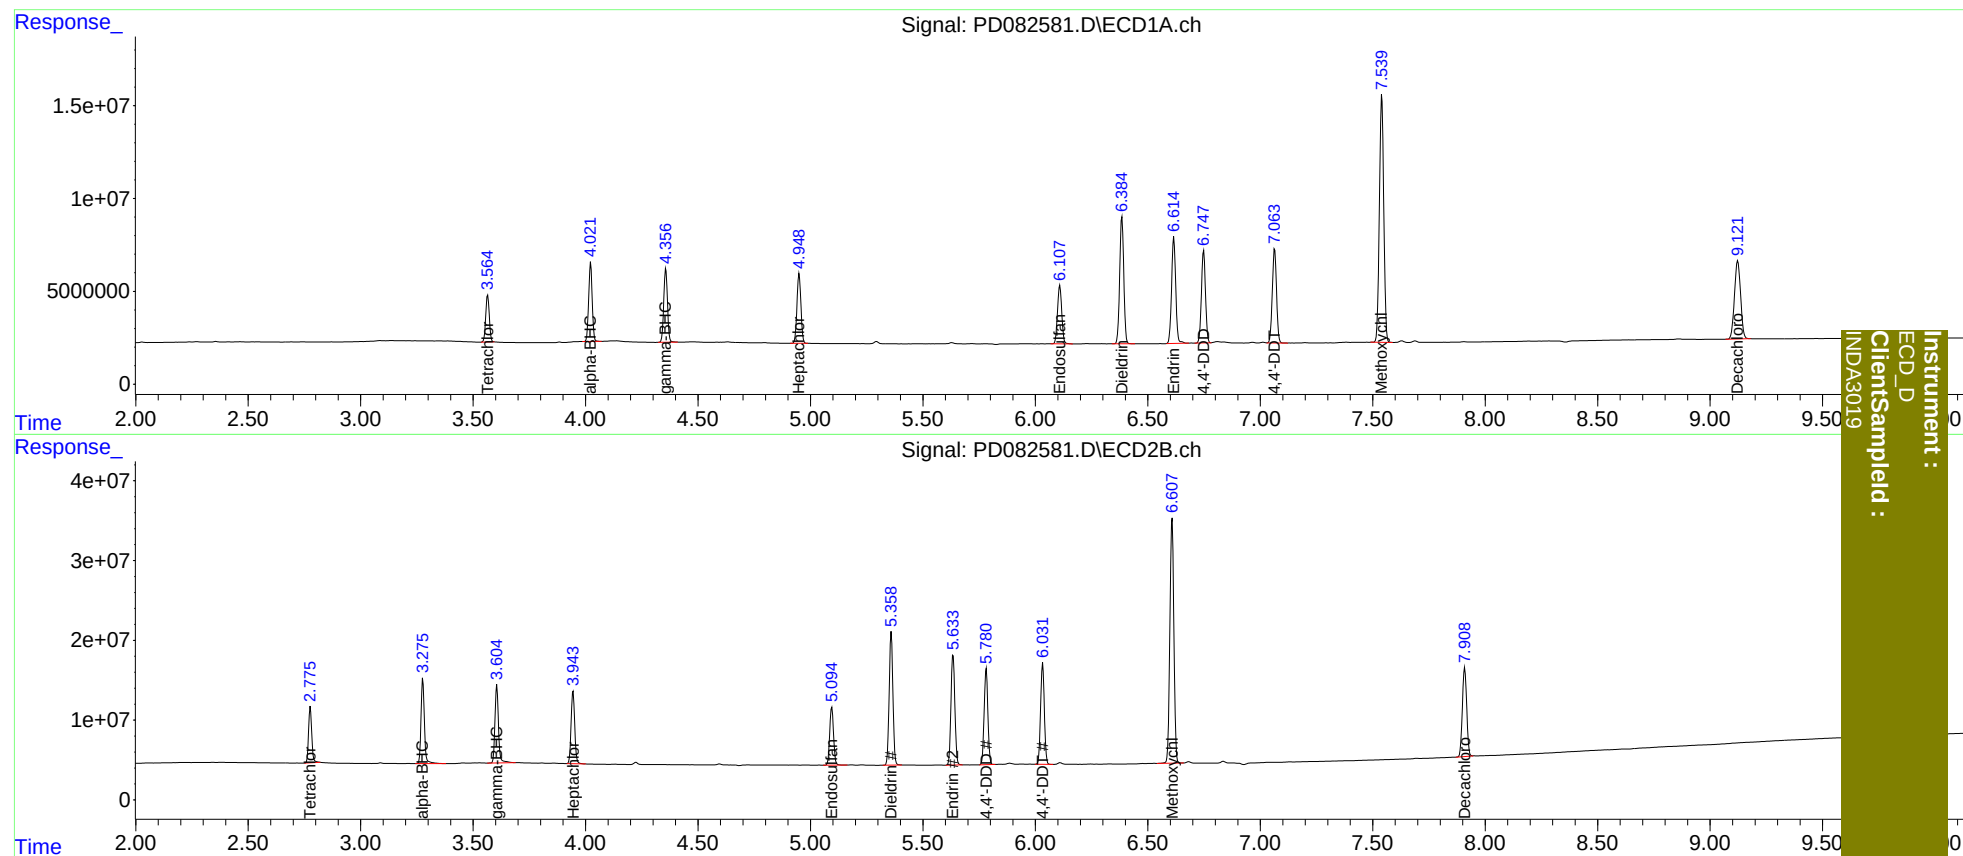


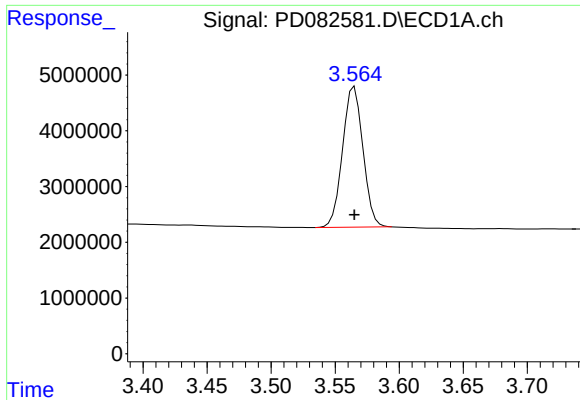

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 27914633
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3019

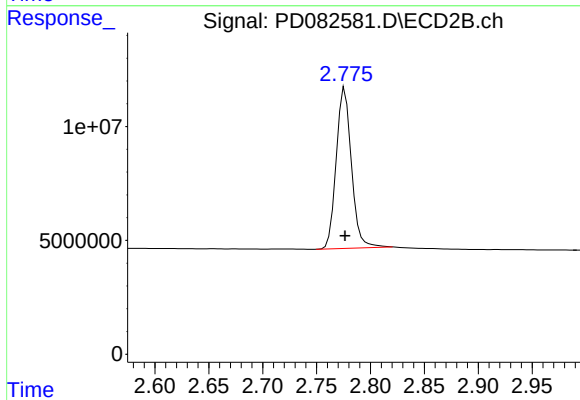


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 69323413
Conc: 20.00 ng/ml

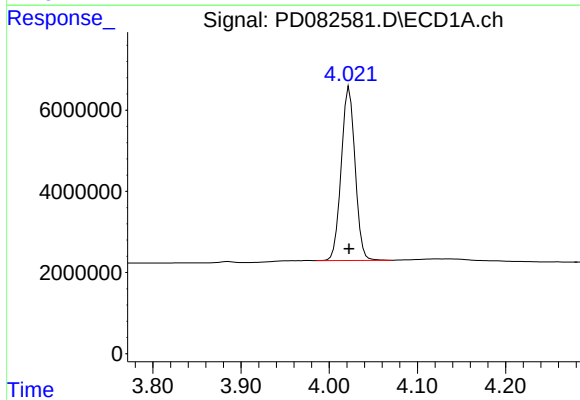


#2 alpha-BHC

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 46564868
Conc: 20.00 ng/ml

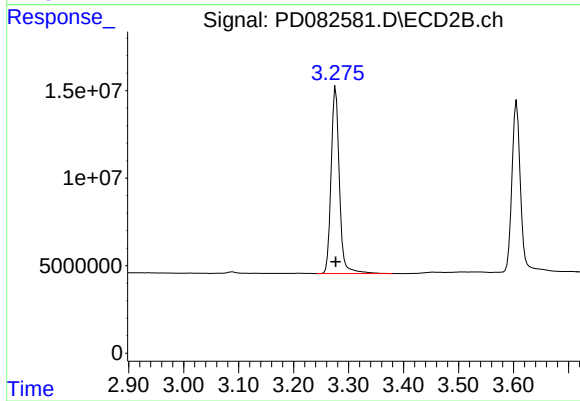

#2 alpha-BHC


R.T.: 3.277 min
Delta R.T.: 0.000 min
Response: 111396195
Conc: 20.00 ng/ml

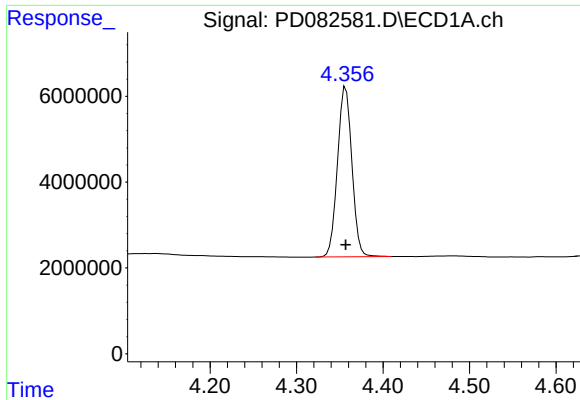

#3 gamma-BHC (Lindane)


R.T.: 4.357 min
Delta R.T.: 0.000 min
Response: 45654389
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3019

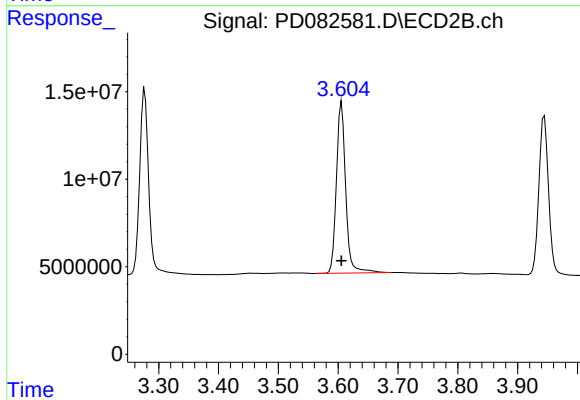


#3 gamma-BHC (Lindane)

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 106134648
Conc: 20.00 ng/ml

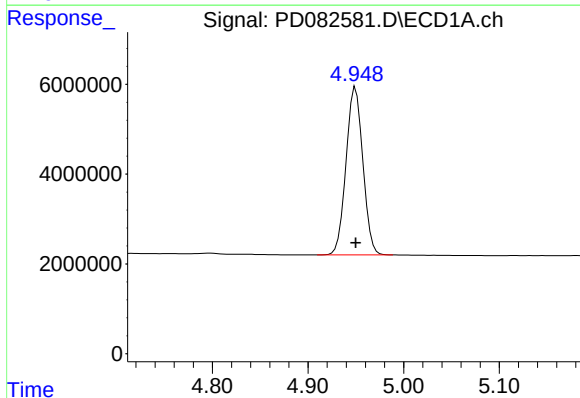


#4 Heptachlor

R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 45866556
Conc: 20.00 ng/ml

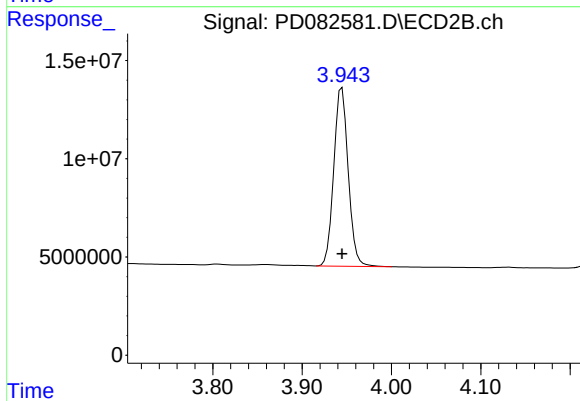

#4 Heptachlor


R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 101972327
Conc: 20.00 ng/ml

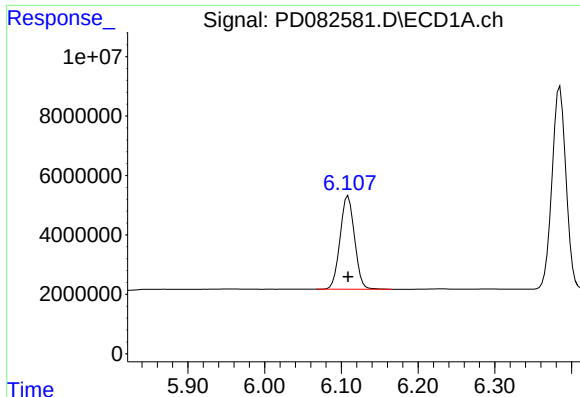

#9 Endosulfan I


R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 41192171
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3019

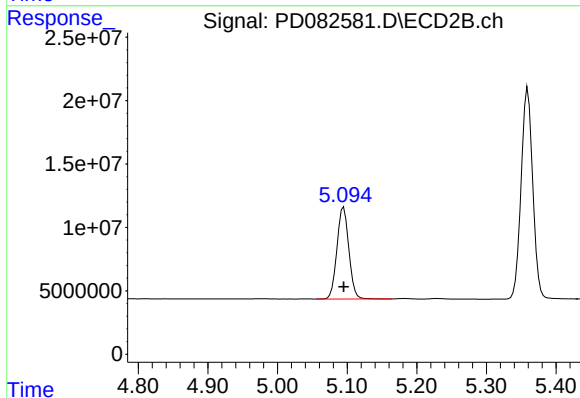


#9 Endosulfan I

R.T.: 5.095 min
Delta R.T.: 0.000 min
Response: 86037093
Conc: 20.00 ng/ml

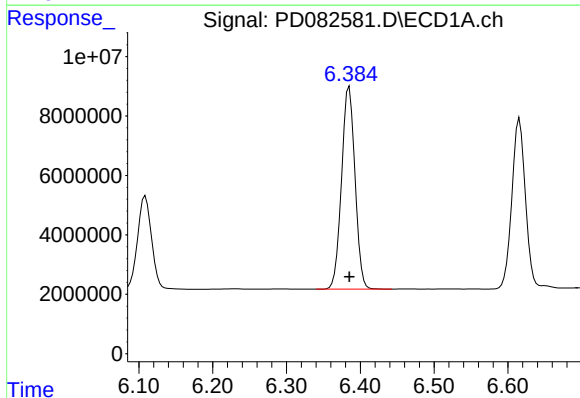


#13 Dieldrin

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 86138362
Conc: 40.00 ng/ml

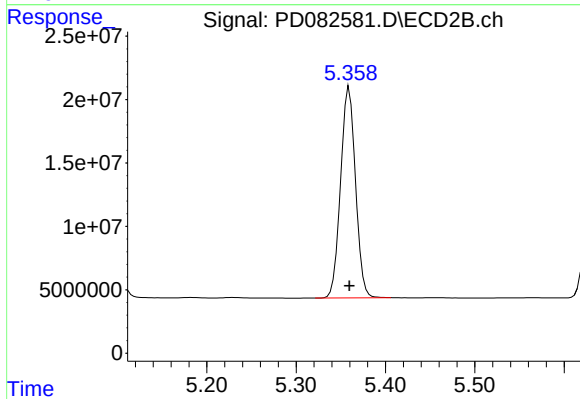

#13 Dieldrin


R.T.: 5.359 min
Delta R.T.: 0.000 min
Response: 192691477
Conc: 40.00 ng/ml

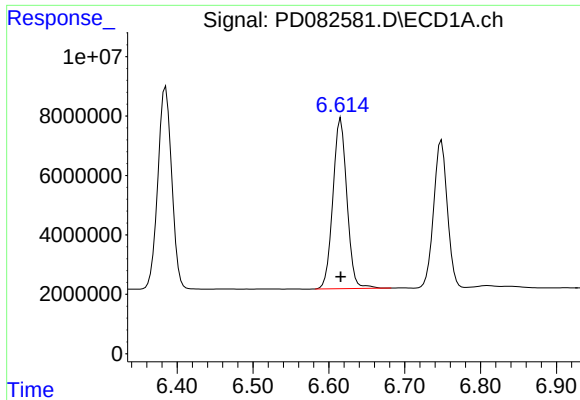

#14 Endrin


R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 73571824
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3019

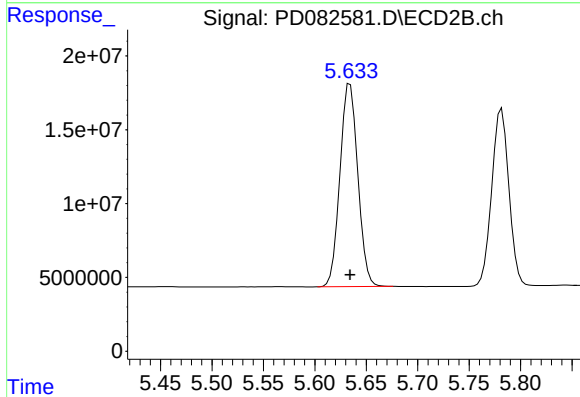


#14 Endrin

R.T.: 5.634 min
Delta R.T.: 0.000 min
Response: 166378808
Conc: 40.00 ng/ml

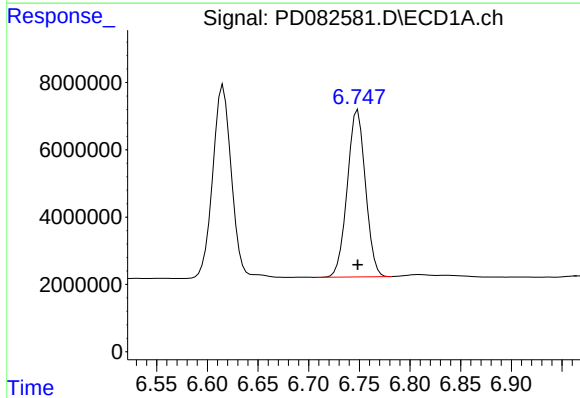


#16 4,4'-DDD

R.T.: 6.748 min
Delta R.T.: 0.000 min
Response: 61896005
Conc: 40.00 ng/ml

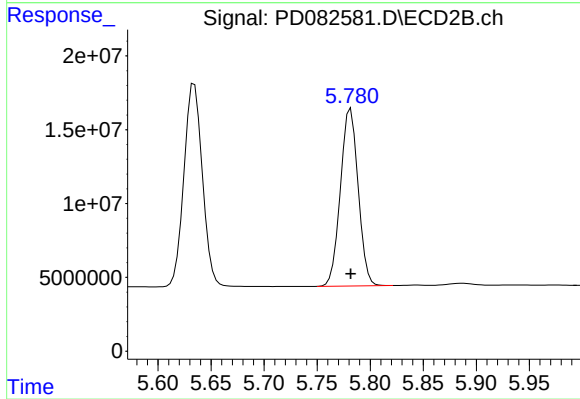

#16 4,4'-DDD


R.T.: 5.782 min
Delta R.T.: 0.000 min
Response: 139545002
Conc: 40.00 ng/ml

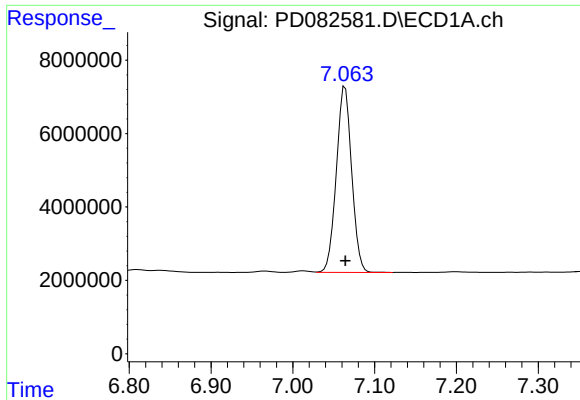

#17 4,4'-DDT


R.T.: 7.064 min
Delta R.T.: 0.000 min
Response: 65902857
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3019

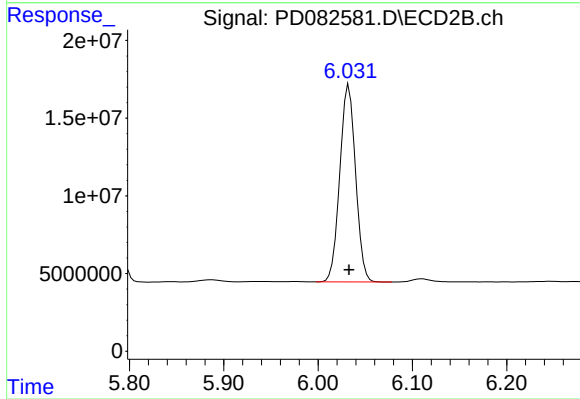


#17 4,4'-DDT

R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 147508023
Conc: 40.00 ng/ml

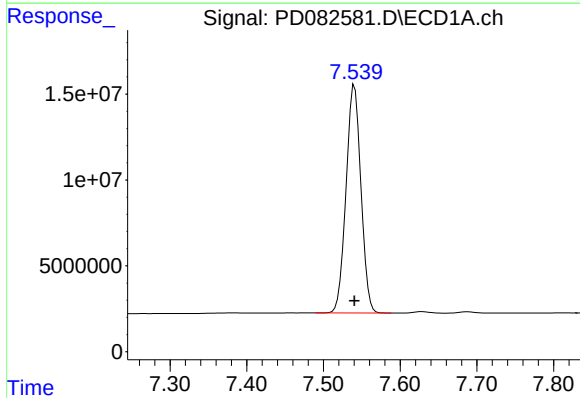


#20 Methoxychlor

R.T.: 7.540 min
Delta R.T.: 0.000 min
Response: 180115841
Conc: 200.00 ng/ml

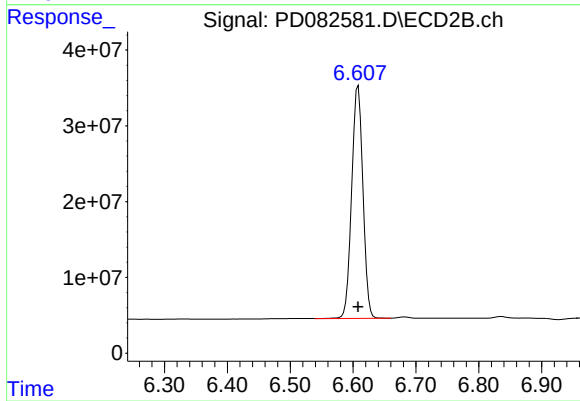

#20 Methoxychlor

R.T.: 6.608 min
Delta R.T.: 0.000 min
Response: 381210819
Conc: 200.00 ng/ml

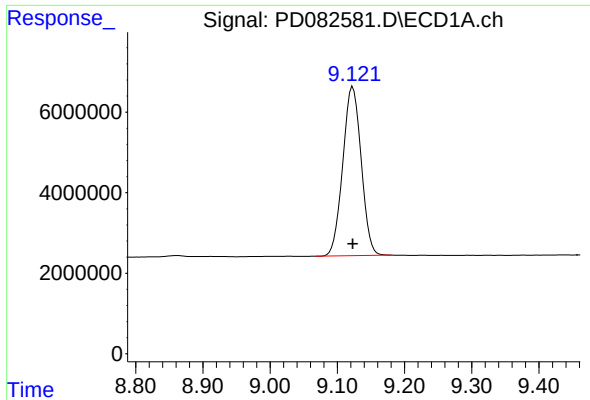

#27 Decachlorobiphenyl


R.T.: 9.123 min

Delta R.T.: 0.000 min

Response: 79737016

Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3019

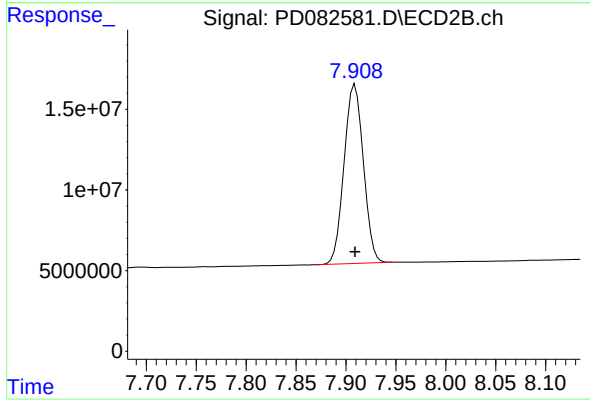

#27 Decachlorobiphenyl

R.T.: 7.909 min

Delta R.T.: 0.000 min

Response: 149316766

Conc: 40.00 ng/ml