

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD042523\  
 Data File : PD074901.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 Apr 2023 19:21  
 Operator : AR\AJ  
 Sample : 02418-03  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 EW8Y9

Manual Integrations  
 APPROVED

Reviewed By : Abdul Mirza 04/26/2023  
 Supervised By : Ankita Jodhani 04/26/2023

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 25 22:18:08 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD041423CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Apr 14 02:10:15 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml    | ng/ml    |
|-----------------------------|-----------------|-------|-------|----------|----------|----------|----------|
| -----                       |                 |       |       |          |          |          |          |
| System Monitoring Compounds |                 |       |       |          |          |          |          |
| 1)                          | SA Tetrachlo... | 3.549 | 2.770 | 28731770 | 15275363 | 11.254   | 10.858   |
| 27)                         | SA Decachlor... | 9.092 | 7.918 | 65974060 | 16793683 | 21.523   | 12.443 # |
| Target Compounds            |                 |       |       |          |          |          |          |
| 4)                          | MA Heptachlor   | 4.930 | 3.944 | 215.0E6  | 96136699 | 52.658   | 50.606   |
| 5)                          | MB Aldrin       | 5.273 | 4.224 | 701.7E6  | 325.7E6  | 178.268  | 172.136  |
| 8)                          | B Heptachlo...  | 5.699 | 4.727 | 296.2E6  | 137.3E6  | 80.951m  | 78.916   |
| 10)                         | B trans-Chl...  | 5.957 | 4.977 | 319.5E6  | 155.2E6  | 90.597   | 90.897   |
| 11)                         | B cis-Chlor...  | 6.040 | 5.042 | 218.2E6  | 51523962 | 59.388   | 29.809 # |
| 12)                         | B 4,4'-DDE      | 6.208 | 5.232 | 143.7E6  | 69123063 | 41.609   | 42.335   |
| 13)                         | MA Dieldrin     | 6.364 | 5.363 | 5067.6E6 | 1871.2E6 | 1355.723 | 1053.421 |
| 16)                         | A 4,4'-DDD      | 6.726 | 5.786 | 16147198 | 14983033 | 5.669m   | 10.833 # |
| 17)                         | MA 4,4'-DDT     | 7.042 | 6.038 | 440.7E6  | 208.8E6  | 144.830  | 145.207  |
| -----                       |                 |       |       |          |          |          |          |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD042523\  
Data File : PD074901.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Apr 2023 19:21  
Operator : AR\AJ  
Sample : 02418-03  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 25 22:18:08 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD041423CLP.M  
Quant Title : GC Extractables  
QLast Update : Fri Apr 14 02:10:15 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

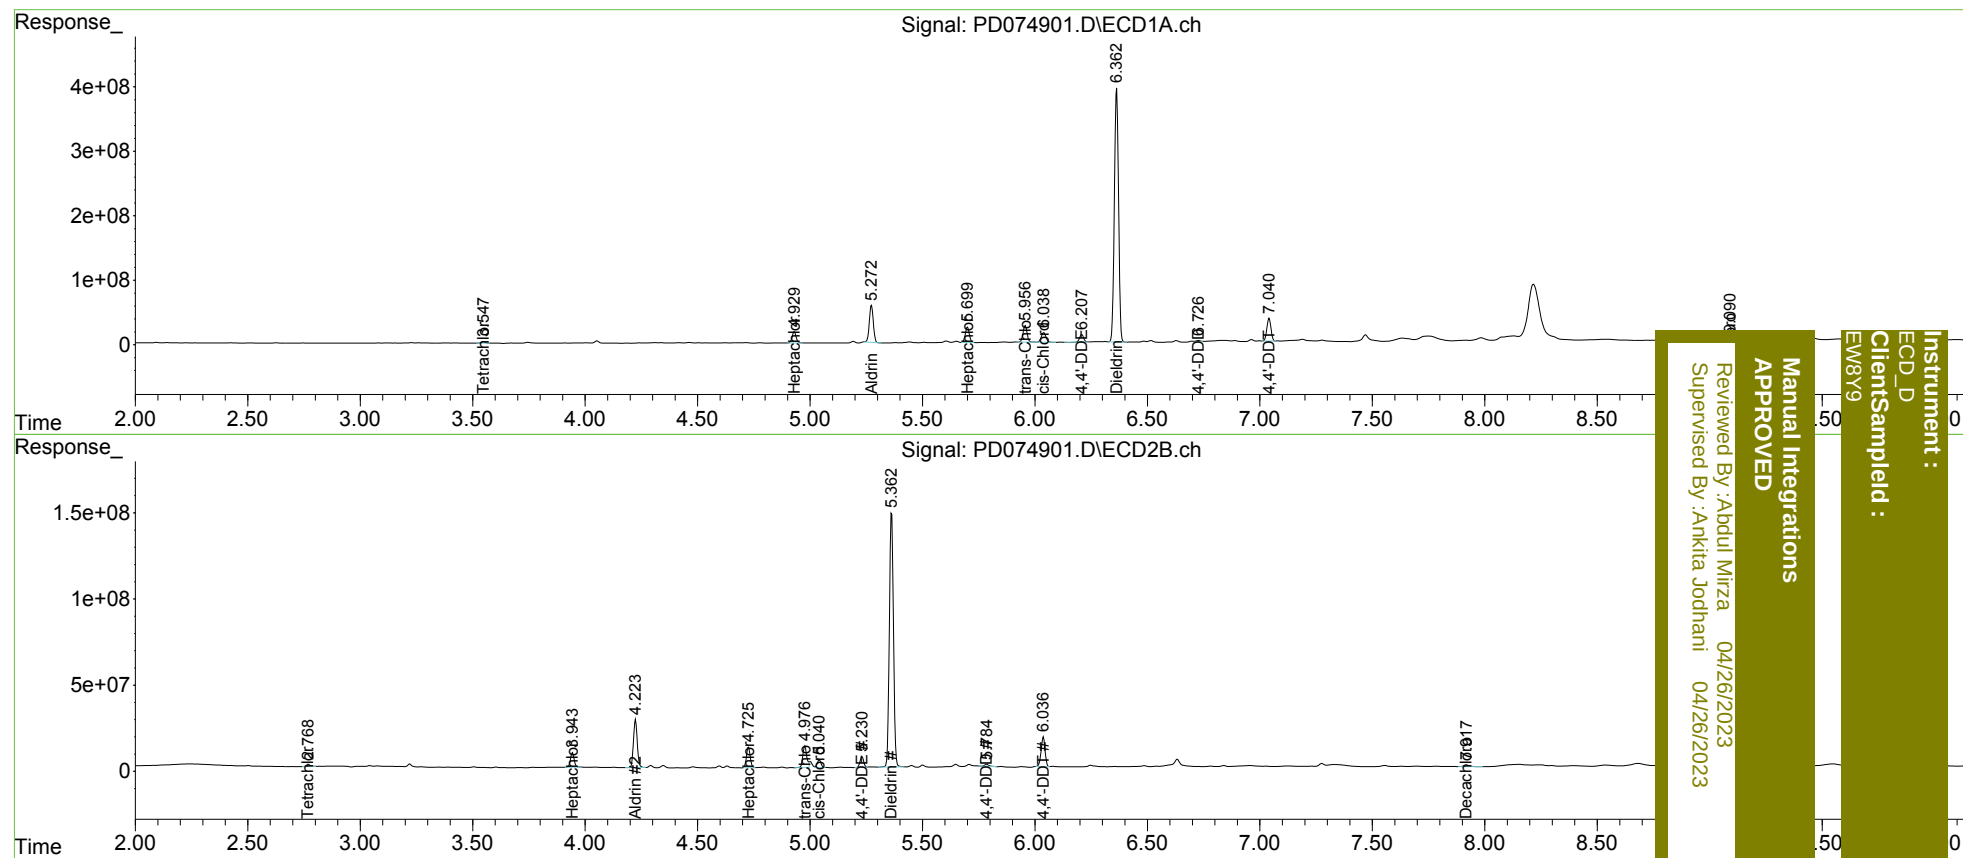

Instrument :  
ECD\_D  
ClientSampled :  
EW8Y9

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 04/26/2023  
Supervised By :Ankita Jodhani 04/26/2023