

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042525\
 Data File : PD088267.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2025 10:25
 Operator : AR\AJ
 Sample : PIBLK164
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK515

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 11:29:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041025CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 14 12:47:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.558	2.882	50138542	355.8E6	25.423	23.144
27)	SA Decachlor...	9.080	8.077	118.7E6	629.9E6	35.419	35.478
Target Compounds							
3)	MA gamma-BHC...	4.303f	0.000	1059735	0	0.266	N.D. #
6)	B beta-BHC	0.000	3.994f	0	25338991	N.D.	2.581
7)	B delta-BHC	4.786	0.000	3317802	0	0.838	N.D. #
8)	B Heptachlo...	5.654f	0.000	251352	0	<MDL	N.D. #
10)	B trans-Chl...	6.003f	0.000	1566404	0	0.459	N.D. #
11)	B cis-Chlor...	6.003	0.000	1566404	0	0.458	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042525\
Data File : PD088267.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2025 10:25
Operator : AR\AJ
Sample : PIBLK164
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 11:29:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041025CLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 14 12:47:00 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

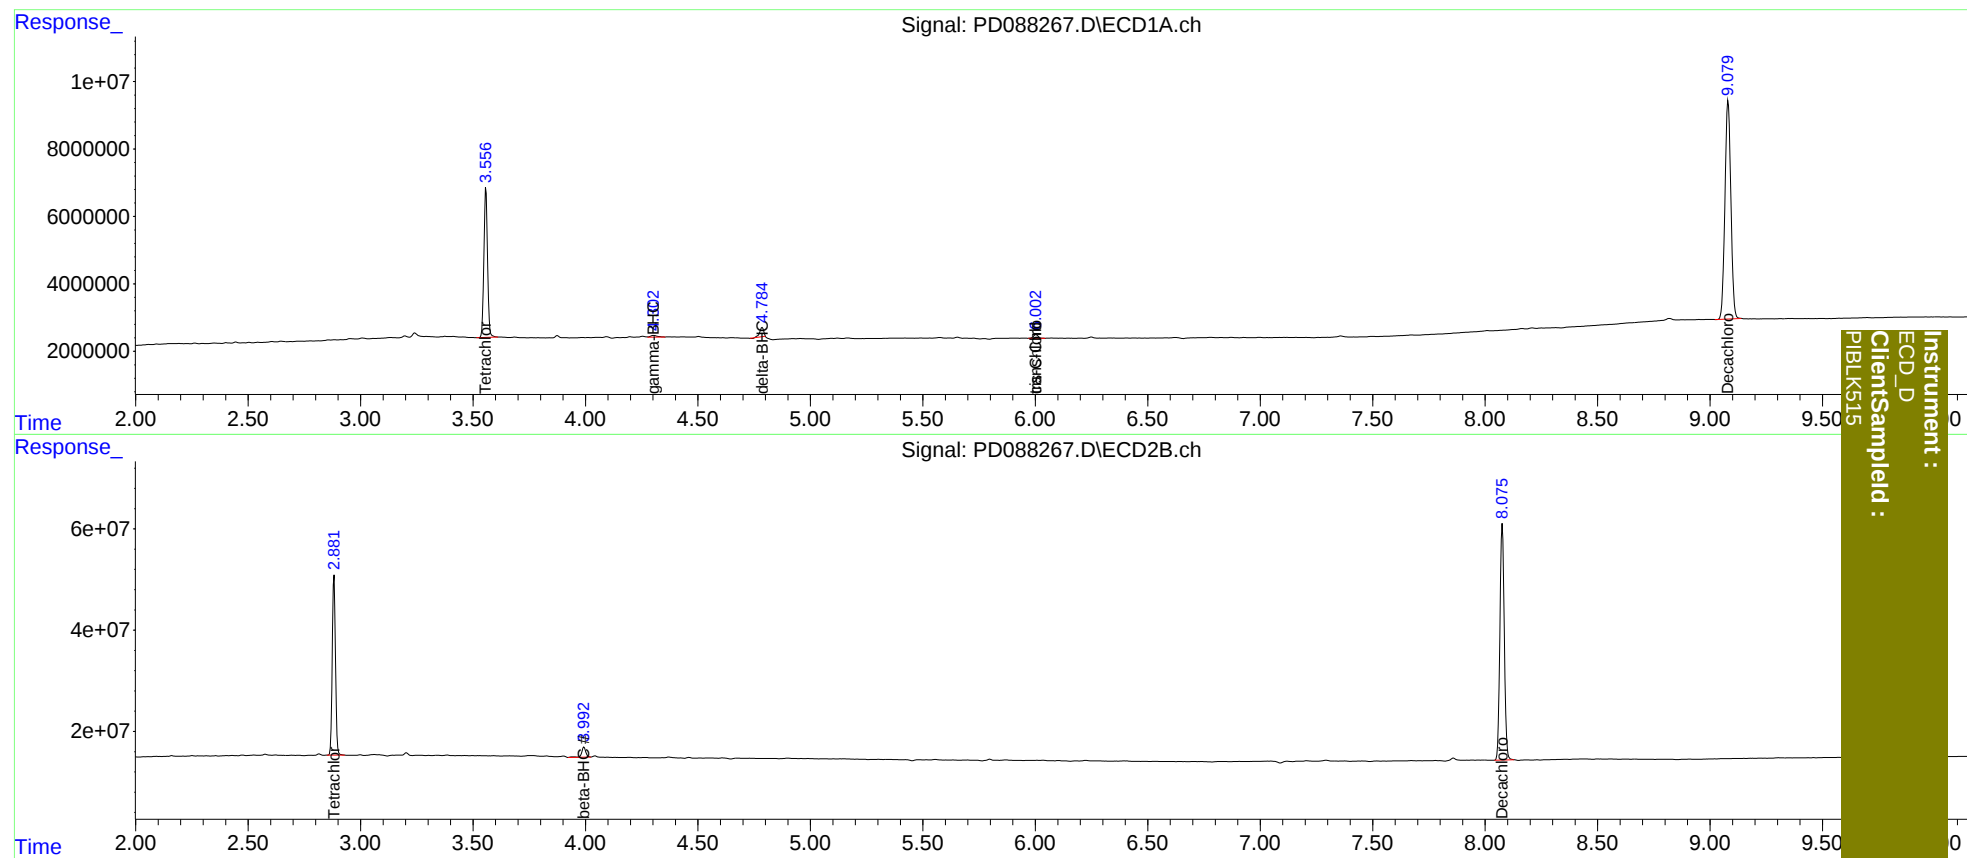


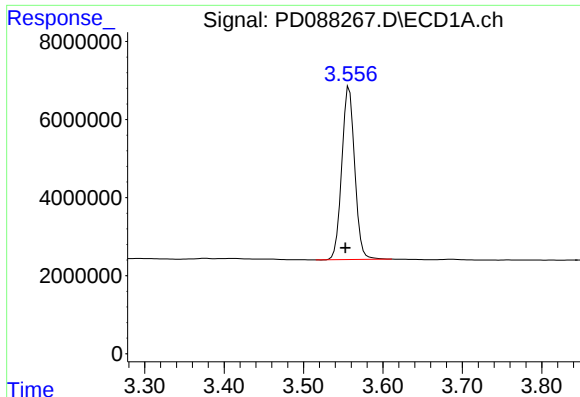

#1 Tetrachloro-m-xylene


R.T.: 3.558 min
Delta R.T.: 0.005 min
Response: 50138542
Conc: 25.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK515

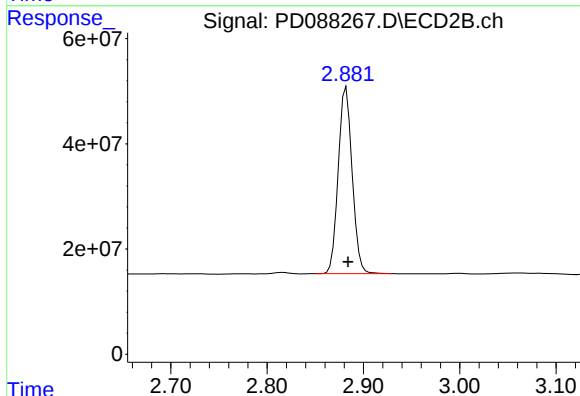


#1 Tetrachloro-m-xylene

R.T.: 2.882 min
Delta R.T.: -0.002 min
Response: 355755349
Conc: 23.14 ng/ml

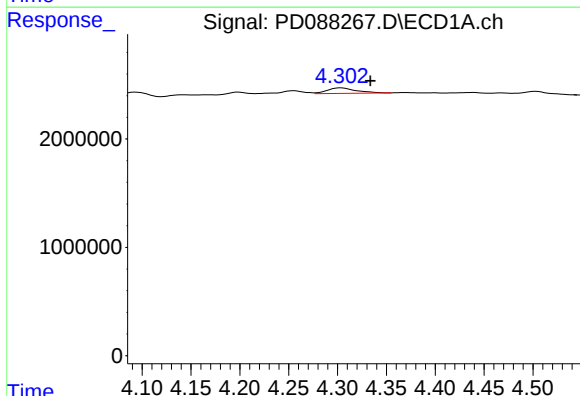


#3 gamma-BHC (Lindane)

R.T.: 4.303 min
Delta R.T.: -0.030 min
Response: 1059735
Conc: 0.27 ng/ml

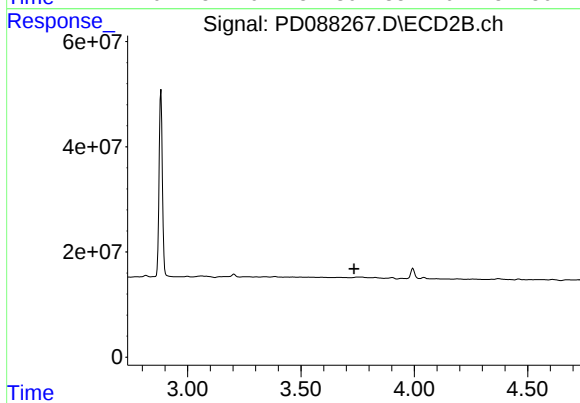

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.734 min
Response: 0
Conc: N.D.

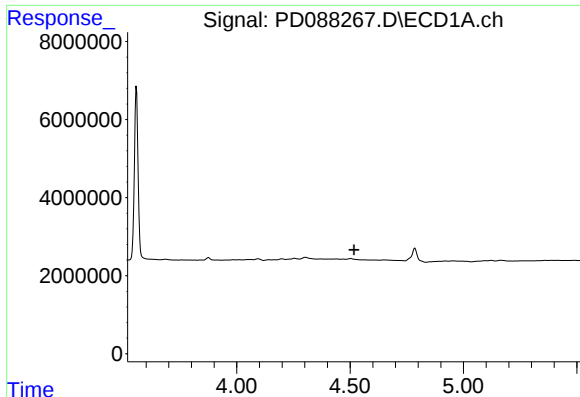

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK515

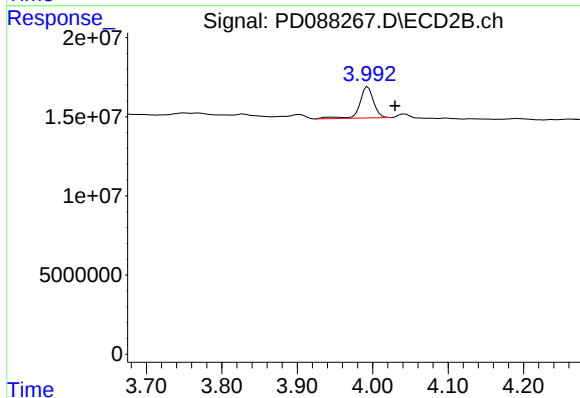


#6 beta-BHC

R.T.: 3.994 min
Delta R.T.: -0.036 min
Response: 25338991
Conc: 2.58 ng/ml

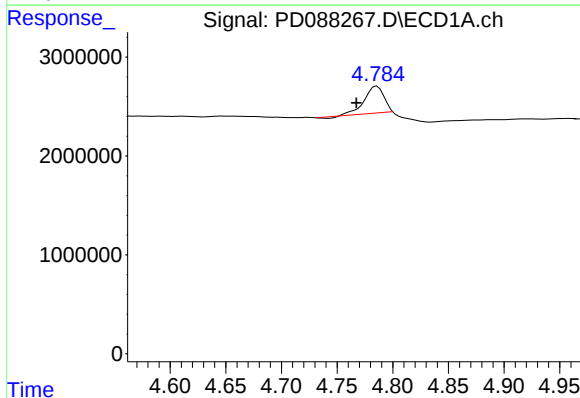


#7 delta-BHC

R.T.: 4.786 min
Delta R.T.: 0.019 min
Response: 3317802
Conc: 0.84 ng/ml

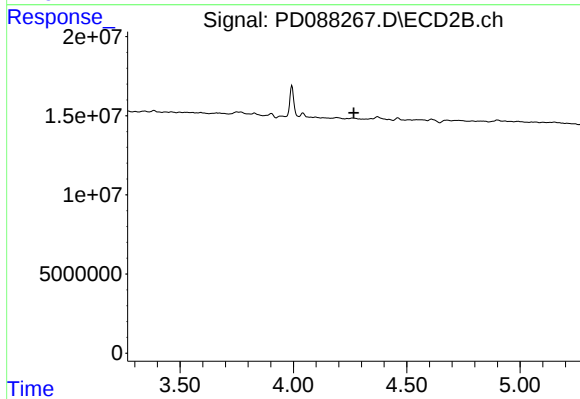

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.267 min
Response: 0
Conc: N.D.

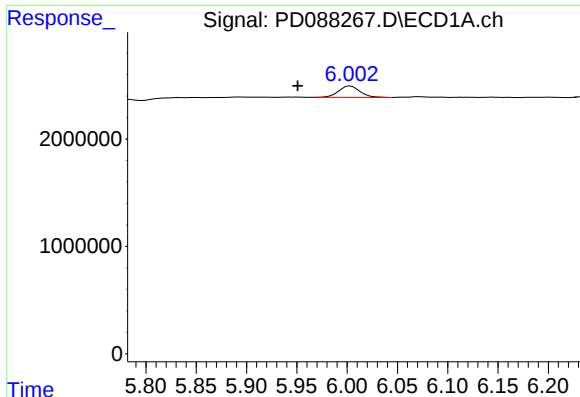

#10 trans-Chlordane


R.T.: 6.003 min
Delta R.T.: 0.052 min
Response: 1566404
Conc: 0.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK515

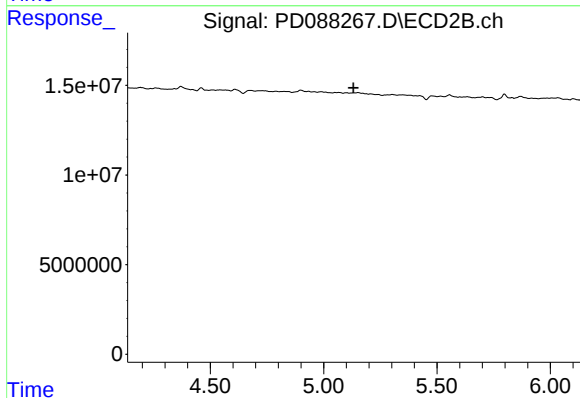


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.132 min
Response: 0
Conc: N.D.

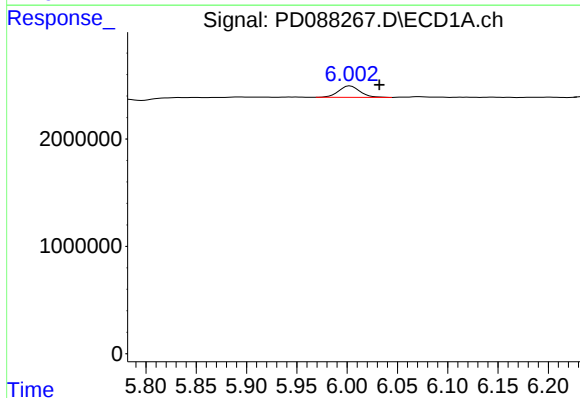


#11 cis-Chlordane

R.T.: 6.003 min
Delta R.T.: -0.029 min
Response: 1566404
Conc: 0.46 ng/ml

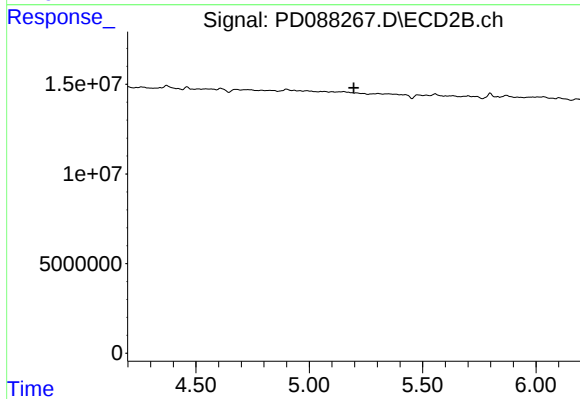

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.196 min
Response: 0
Conc: N.D.

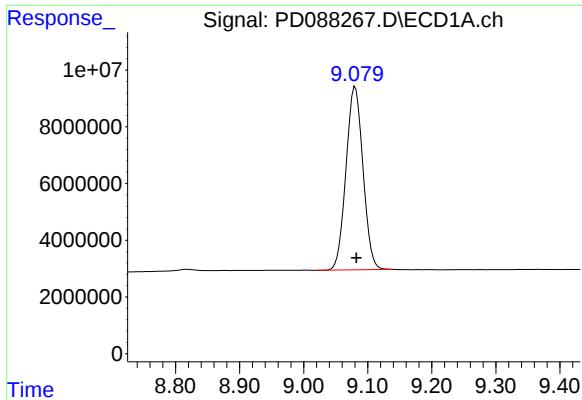

#27 Decachlorobiphenyl

R.T.: 9.080 min
Delta R.T.: -0.002 min
Response: 118703936
Conc: 35.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK515

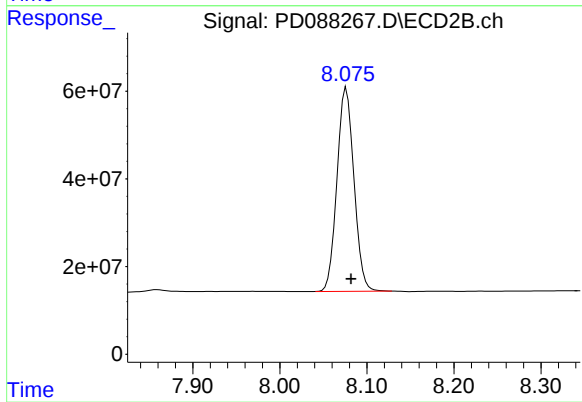

#27 Decachlorobiphenyl

R.T.: 8.077 min
Delta R.T.: -0.005 min
Response: 629932424
Conc: 35.48 ng/ml