

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
 Data File : PD062412.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2021 13:48
 Operator : AR\AJ
 Sample : M2132-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-2-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 16:06:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	11256741	152.7E6	13.821	14.501
28)	SA Decachlor...	8.257	9.041	14332266	98551962	11.815	11.615
Target Compounds							
8)	B Heptachlo...	0.000	5.859	0	9700110	N.D.	0.706 #
9)	A Endosulfan I	0.000	6.197	0	680160	N.D.	0.052 #
11)	B alpha-Chl...	0.000	6.164	0	1220683	N.D.	0.089 #
12)	B 4,4'-DDE	0.000	6.316	0	3073708	N.D.	0.218 #
13)	MA Dieldrin	0.000	6.461	0	1196067	N.D.	0.085 #
15)	B Endosulfa...	0.000	6.901	0	517548	N.D.	0.045 #
16)	A 4,4'-DDD	0.000	6.810	0	2454185	N.D.	0.220 #
17)	MA 4,4'-DDT	0.000	7.115	0	1062898	N.D.	0.107 #
21)	B Endrin ke...	0.000	7.739f	0	1292420	N.D.	0.129 #
22)	Mirex	0.000	8.181	0	2531249	N.D.	0.405 #
26)	Chlordane-4	0.000	6.164	0	1220683	N.D.	0.536 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
Data File : PD062412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2021 13:48
Operator : AR\AJ
Sample : M2132-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-2-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 16:06:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

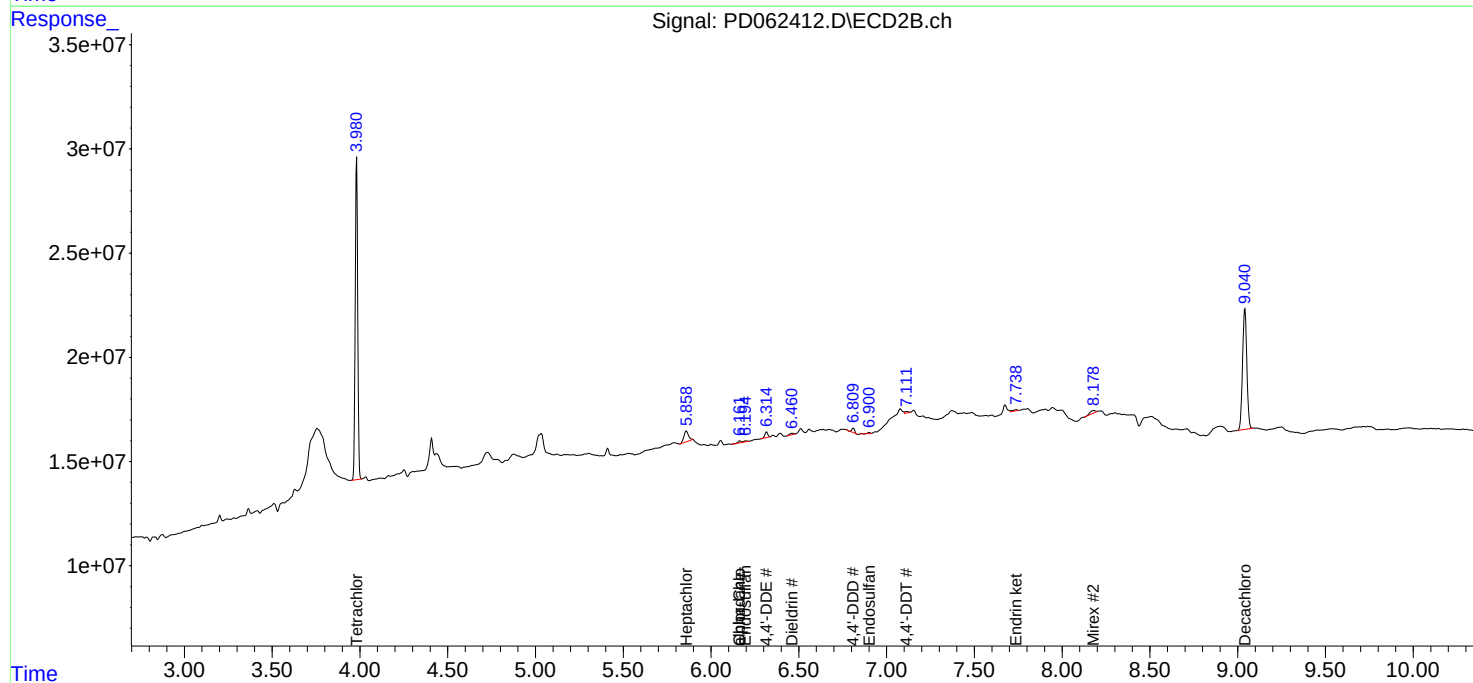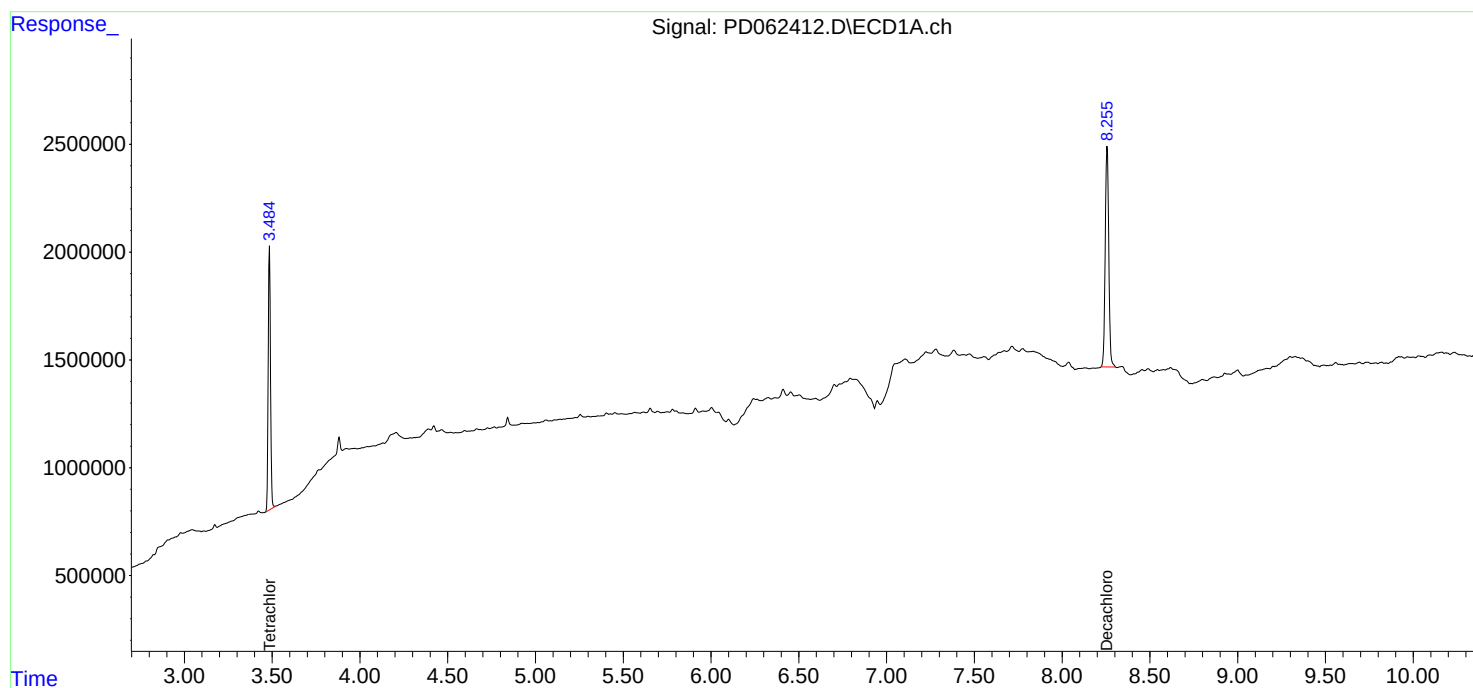


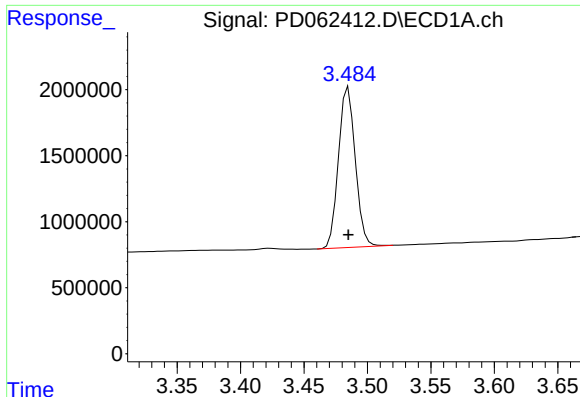

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 11256741
Conc: 13.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-2-COMP

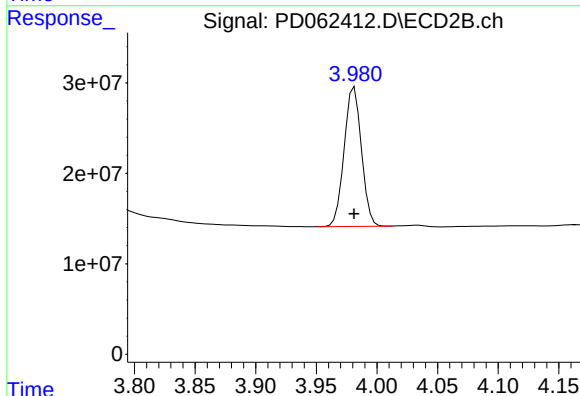


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 152719293
Conc: 14.50 ng/ml

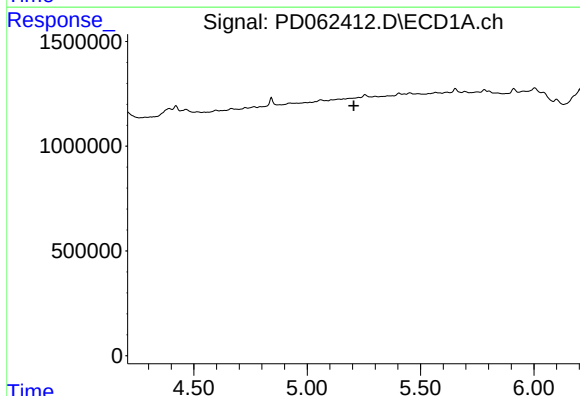


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.206 min
Response: 0
Conc: N.D.

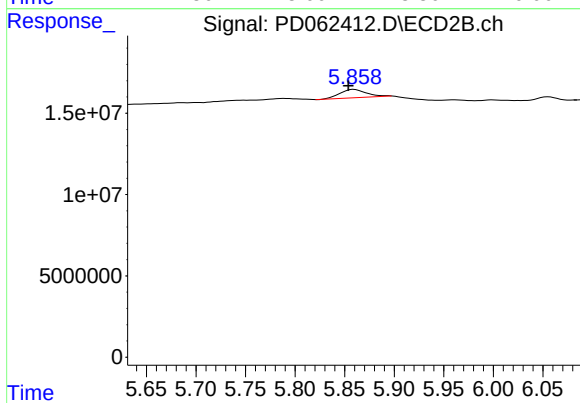

#8 Heptachlor epoxide


R.T.: 5.859 min
Delta R.T.: 0.006 min
Response: 9700110
Conc: 0.71 ng/ml

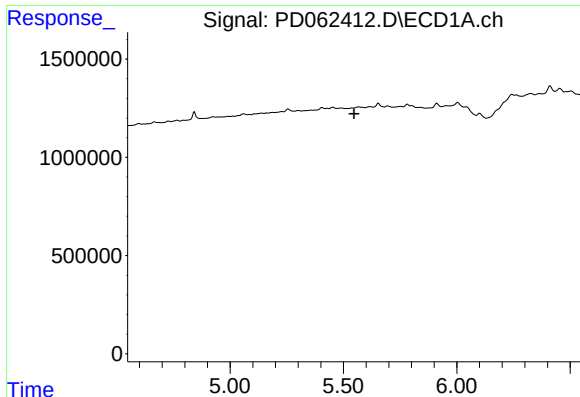

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.547 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-2-COMP

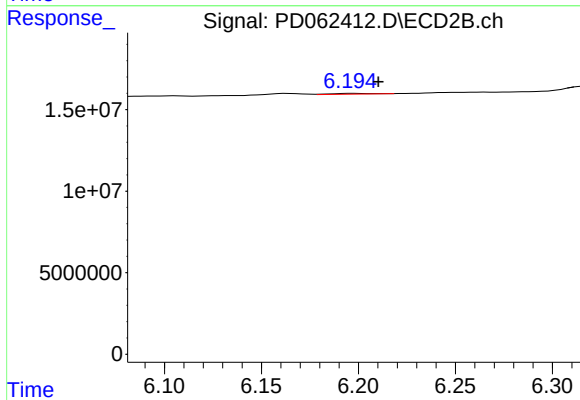


#9 Endosulfan I

R.T.: 6.197 min
Delta R.T.: -0.013 min
Response: 680160
Conc: 0.05 ng/ml

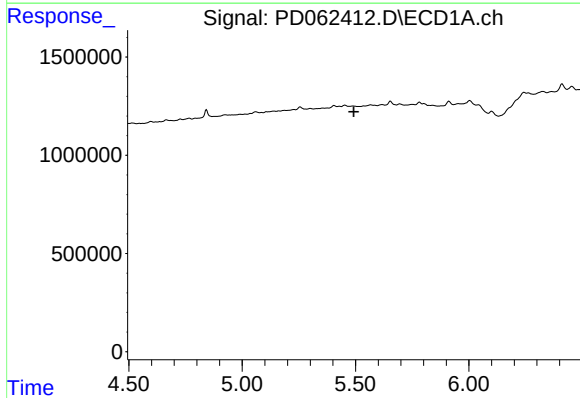


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.492 min
Response: 0
Conc: N.D.

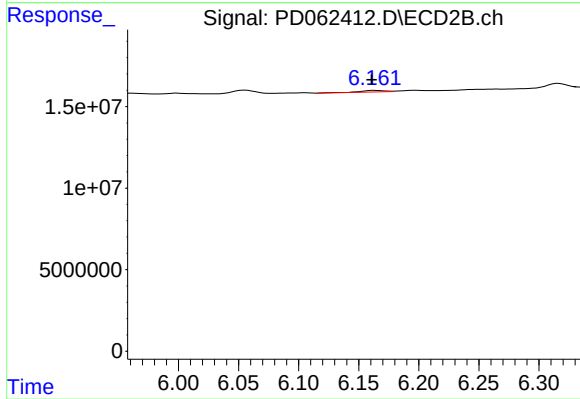

#11 alpha-Chlordane


R.T.: 6.164 min
Delta R.T.: 0.003 min
Response: 1220683
Conc: 0.09 ng/ml

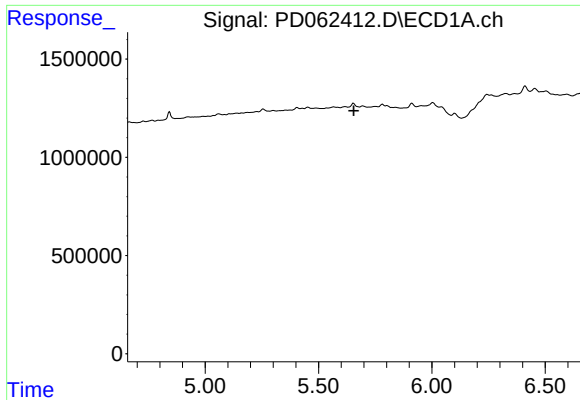

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.655 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-2-COMP

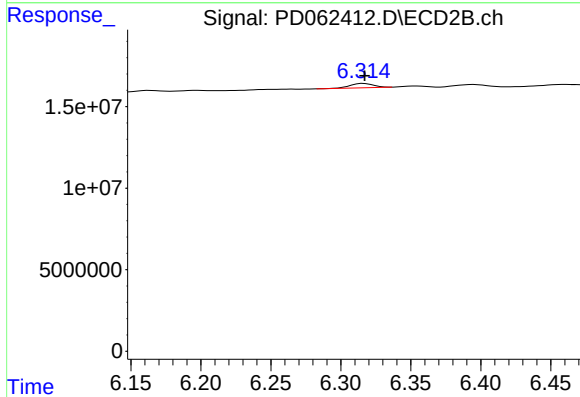


#12 4,4'-DDE

R.T.: 6.316 min
Delta R.T.: 0.000 min
Response: 3073708
Conc: 0.22 ng/ml

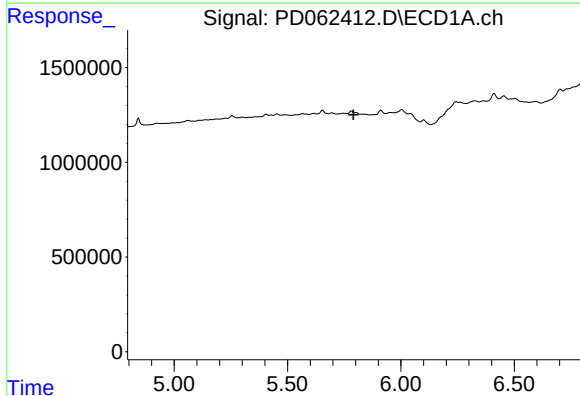


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.791 min
Response: 0
Conc: N.D.

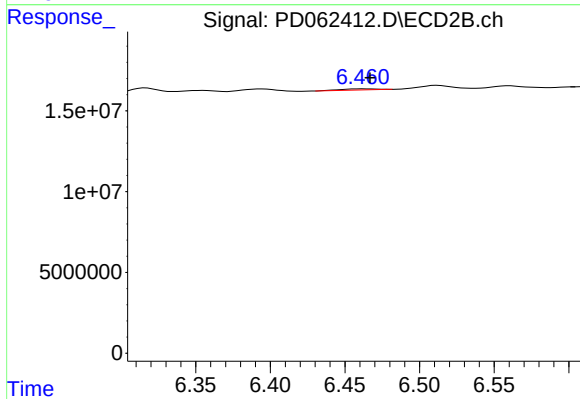

#13 Dieldrin


R.T.: 6.461 min
Delta R.T.: -0.006 min
Response: 1196067
Conc: 0.09 ng/ml

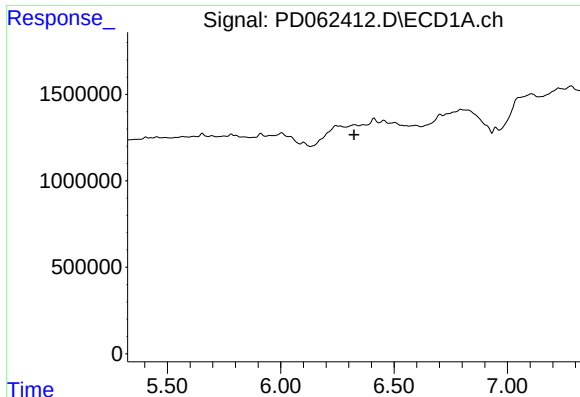

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-2-COMP

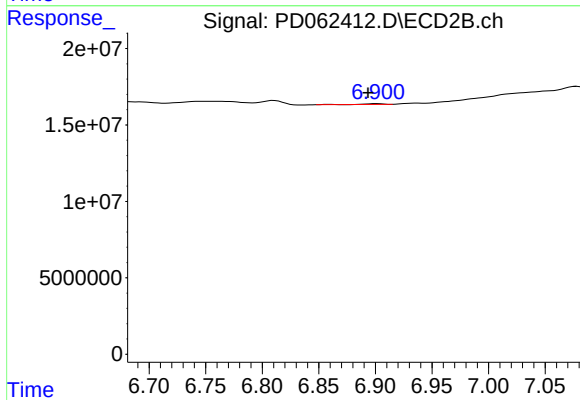


#15 Endosulfan II

R.T.: 6.901 min
Delta R.T.: 0.008 min
Response: 517548
Conc: 0.04 ng/ml

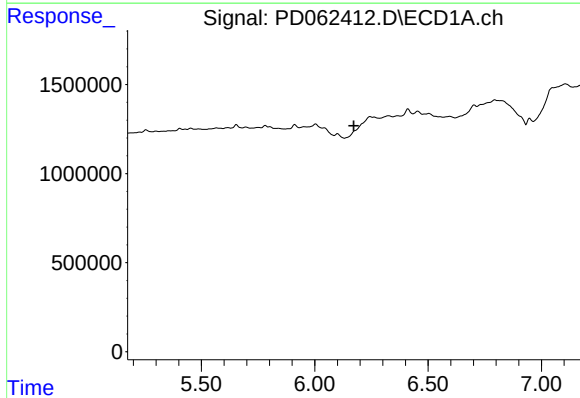


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.173 min
Response: 0
Conc: N.D.

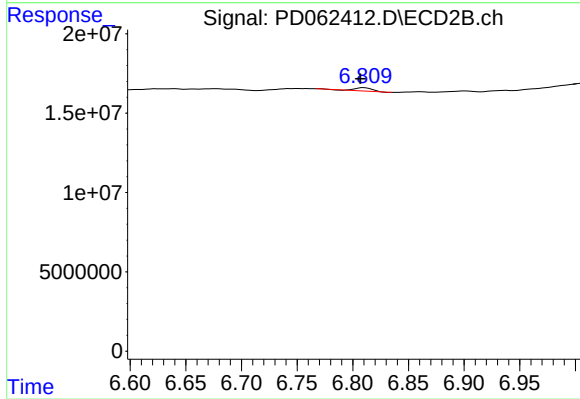

#16 4,4'-DDD


R.T.: 6.810 min
Delta R.T.: 0.004 min
Response: 2454185
Conc: 0.22 ng/ml

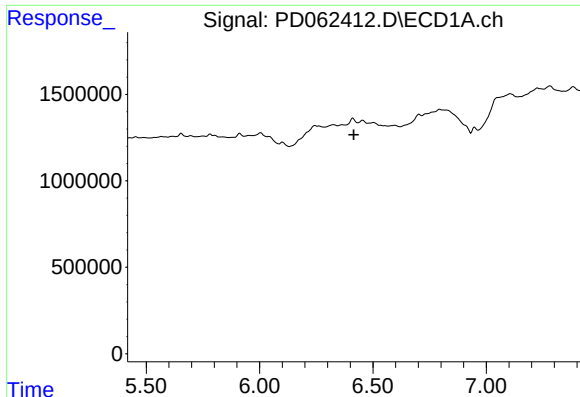

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.415 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-2-COMP

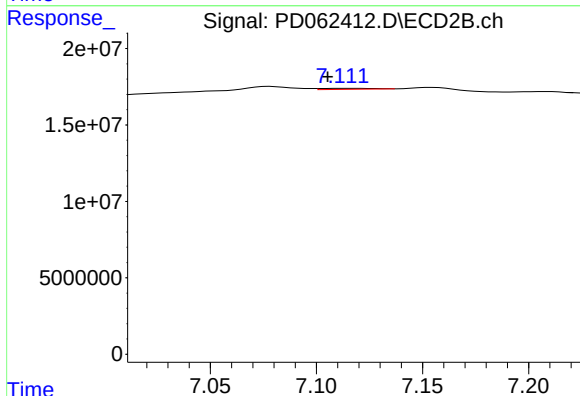


#17 4,4'-DDT

R.T.: 7.115 min
Delta R.T.: 0.010 min
Response: 1062898
Conc: 0.11 ng/ml

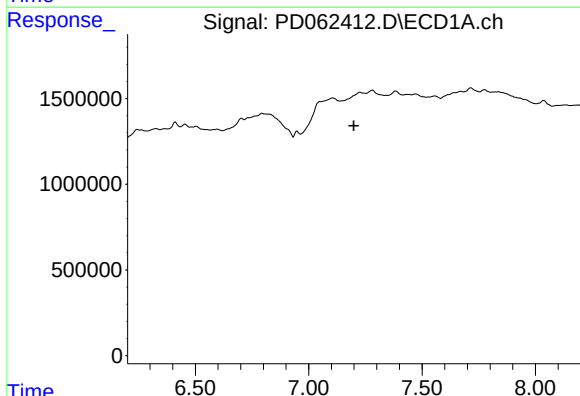


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

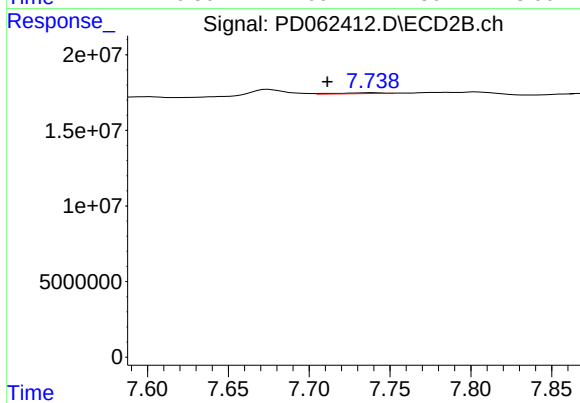

#21 Endrin ketone


R.T.: 7.739 min
Delta R.T.: 0.028 min
Response: 1292420
Conc: 0.13 ng/ml

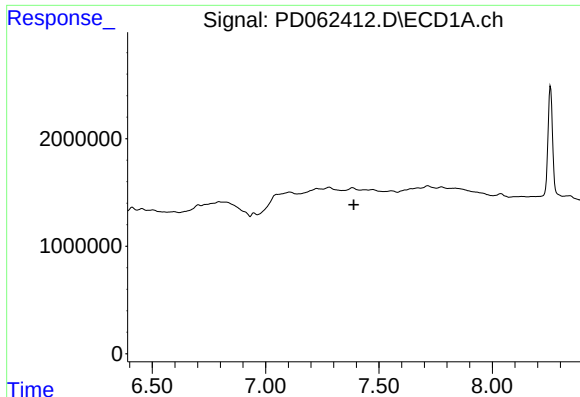

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.390 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-2-COMP

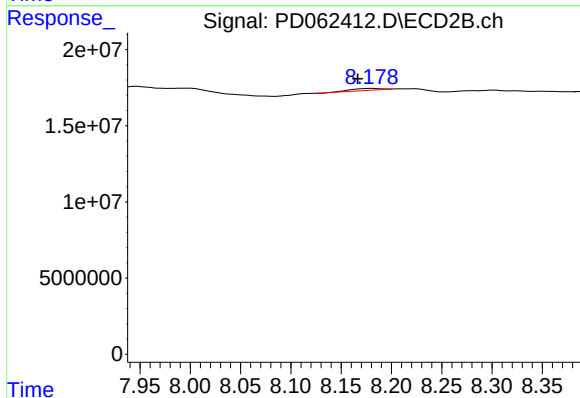


#22 Mirex

R.T.: 8.181 min
Delta R.T.: 0.014 min
Response: 2531249
Conc: 0.40 ng/ml

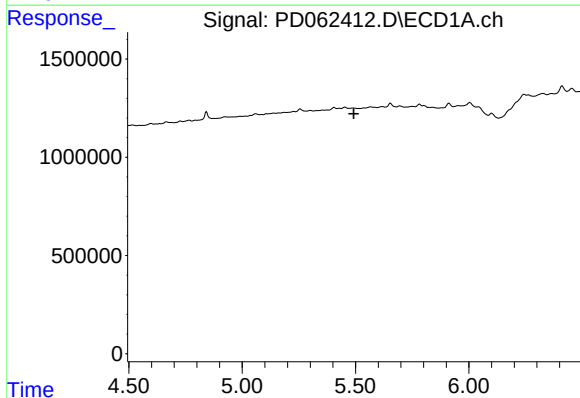


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.493 min
Response: 0
Conc: N.D.

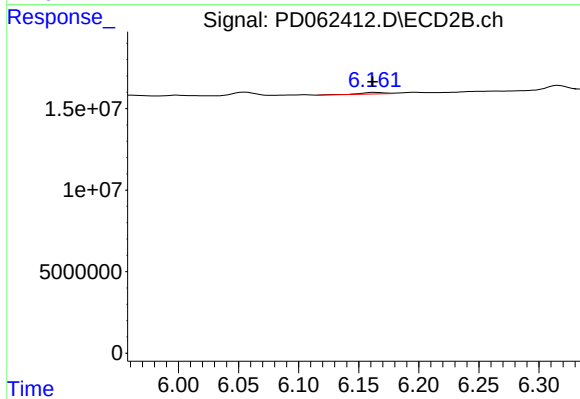

#26 Chlordane-4


R.T.: 6.164 min
Delta R.T.: 0.002 min
Response: 1220683
Conc: 0.54 ng/ml

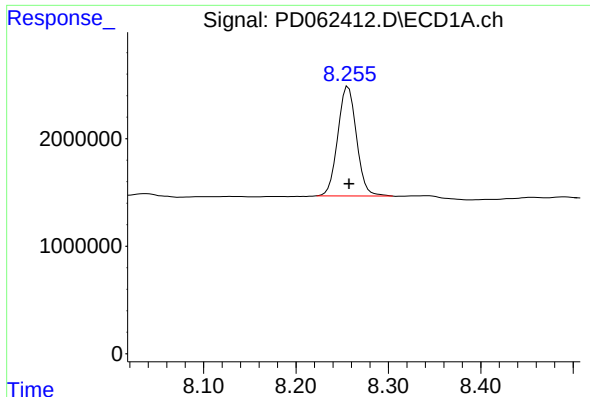

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 14332266
Conc: 11.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-2-COMP

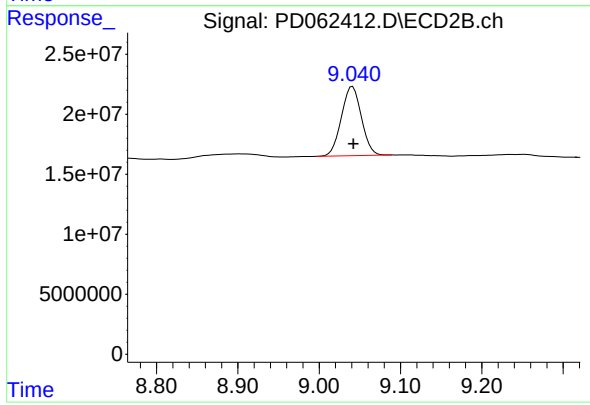

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 98551962
Conc: 11.61 ng/ml