

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
 Data File : PD062416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2021 14:44
 Operator : AR\AJ
 Sample : M2149-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-39-9.5-10.0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 16:07:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	17082869	226.2E6	20.974	21.483
28)	SA Decachlor...	8.257	9.042	17772669	135.1E6	14.651	15.926
Target Compounds							
8)	B Heptachlo...	0.000	5.861	0	7763498	N.D.	0.565 #
9)	A Endosulfan I	0.000	6.201	0	1477677	N.D.	0.113 #
14)	MA Endrin	0.000	6.696	0	613284	N.D.	0.050 #
15)	B Endosulfa...	0.000	6.903	0	1772080	N.D.	0.154 #
18)	B Endrin al...	0.000	7.019	0	1421703	N.D.	0.151 #
19)	B Endosulfa...	0.000	7.237	0	3976172	N.D.	0.367 #
20)	A Methoxychlor	0.000	7.591f	0	488449	N.D.	0.100 #
22)	Mirex	0.000	8.164	0	4292911	N.D.	0.687 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
Data File : PD062416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2021 14:44
Operator : AR\AJ
Sample : M2149-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SB-39-9.5-10.0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 16:07:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

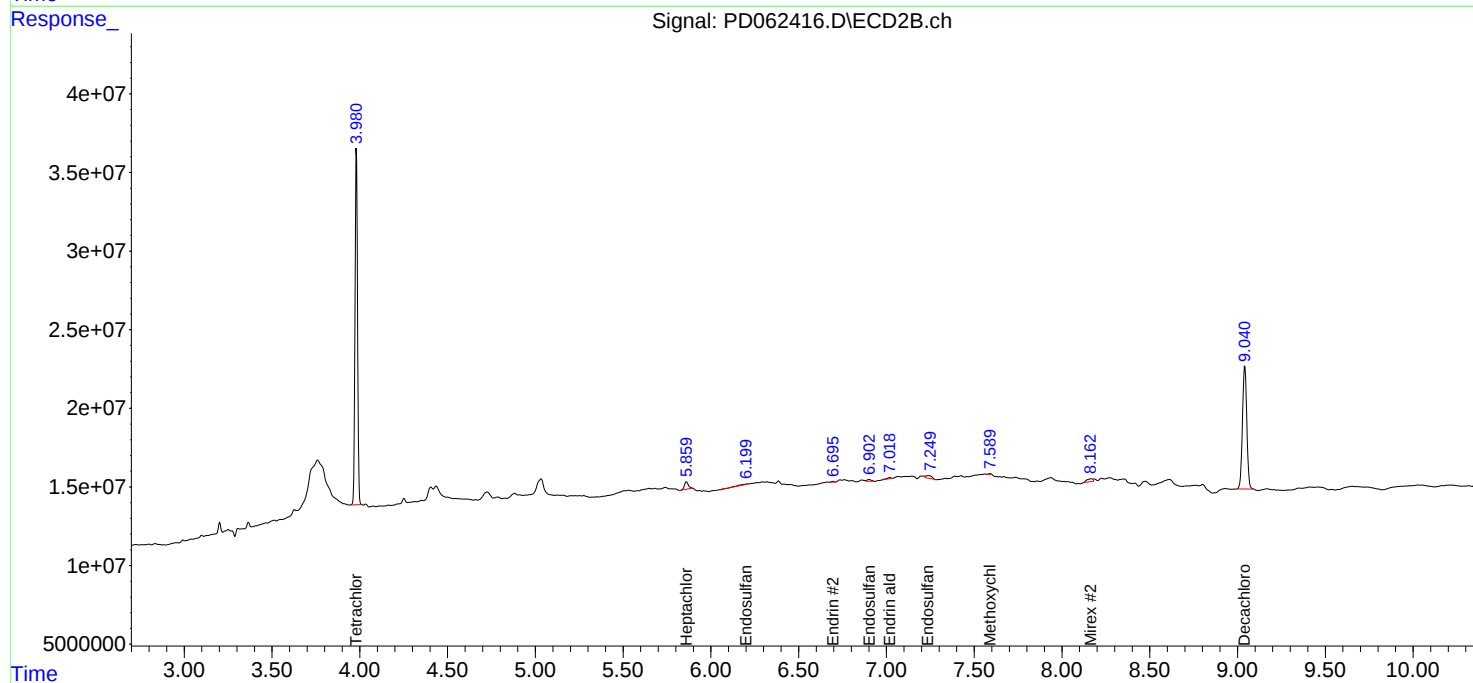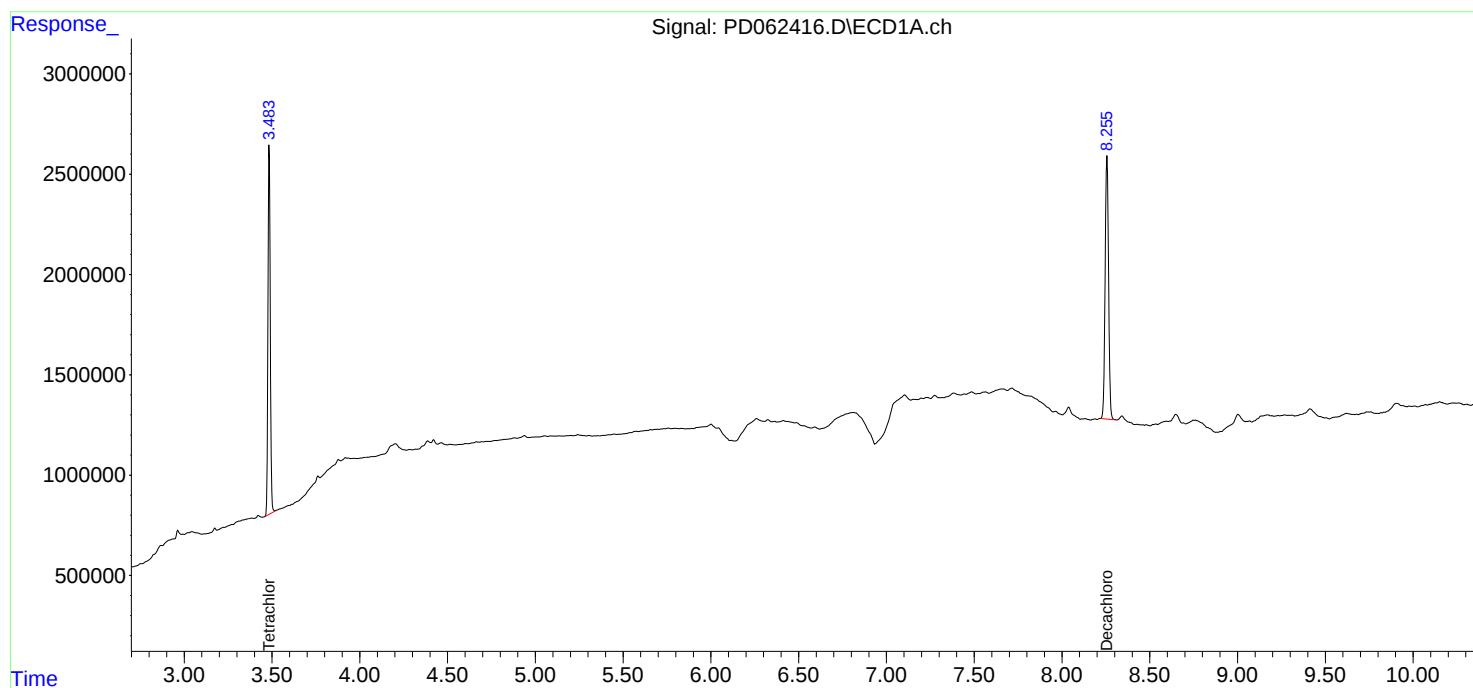


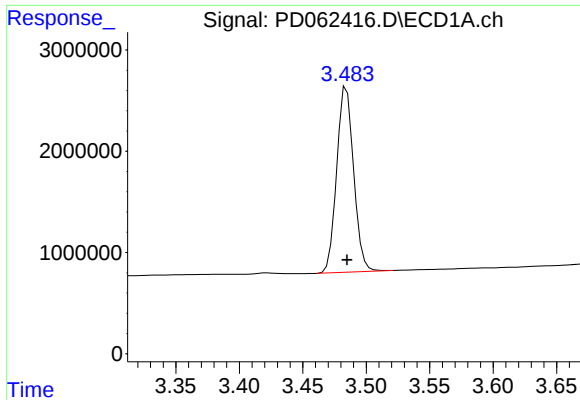

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 17082869
Conc: 20.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-39-9.5-10.0

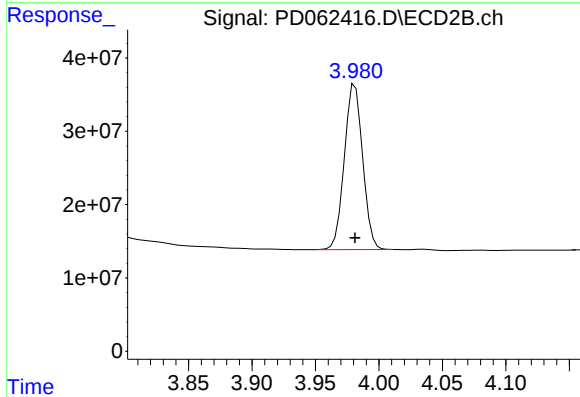


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 226243544
Conc: 21.48 ng/ml

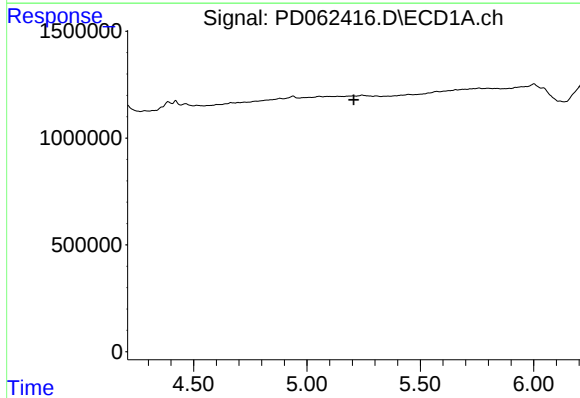


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.206 min
Response: 0
Conc: N.D.

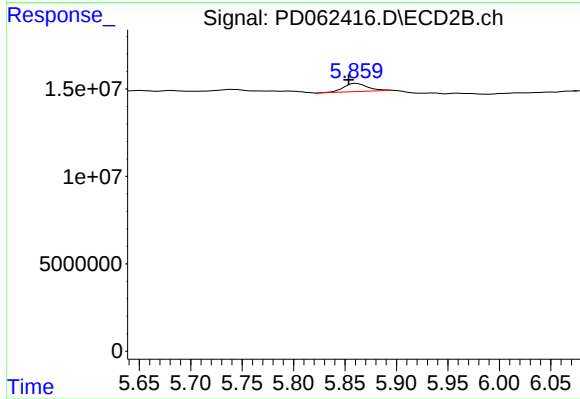

#8 Heptachlor epoxide


R.T.: 5.861 min
Delta R.T.: 0.007 min
Response: 7763498
Conc: 0.57 ng/ml

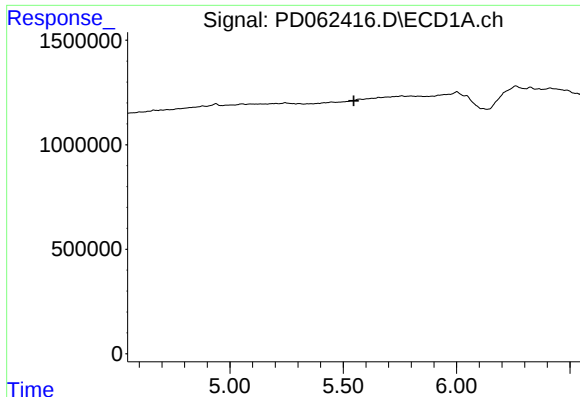

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.547 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SB-39-9.5-10.0

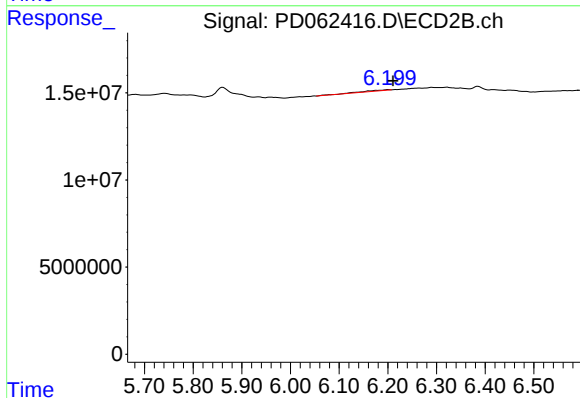


#9 Endosulfan I

R.T.: 6.201 min
Delta R.T.: -0.009 min
Response: 1477677
Conc: 0.11 ng/ml

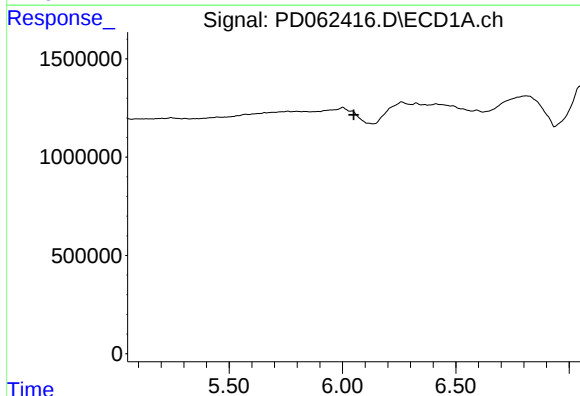


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.050 min
Response: 0
Conc: N.D.

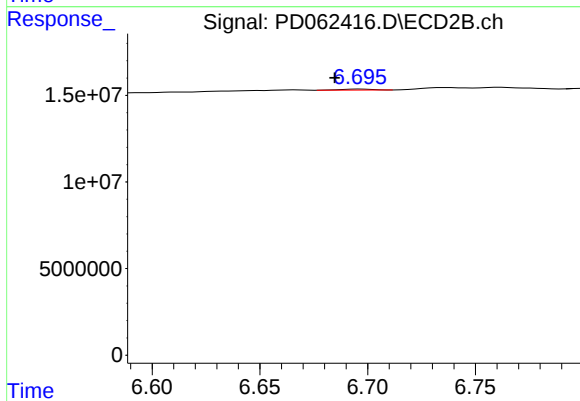

#14 Endrin


R.T.: 6.696 min
Delta R.T.: 0.012 min
Response: 613284
Conc: 0.05 ng/ml

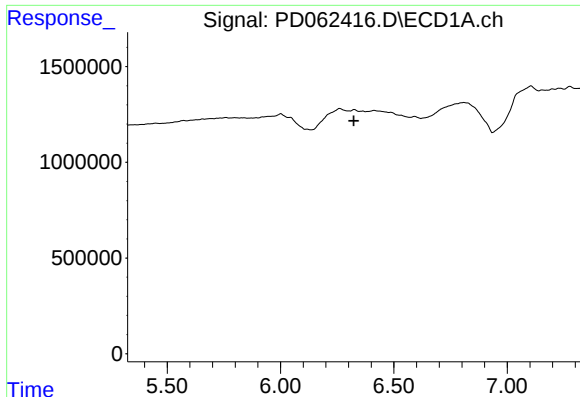

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SB-39-9.5-10.0

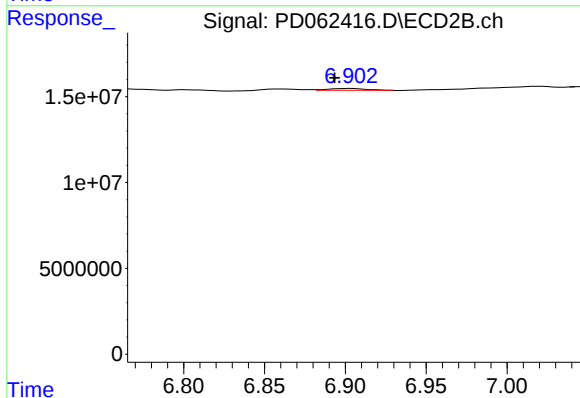


#15 Endosulfan II

R.T.: 6.903 min
Delta R.T.: 0.010 min
Response: 1772080
Conc: 0.15 ng/ml

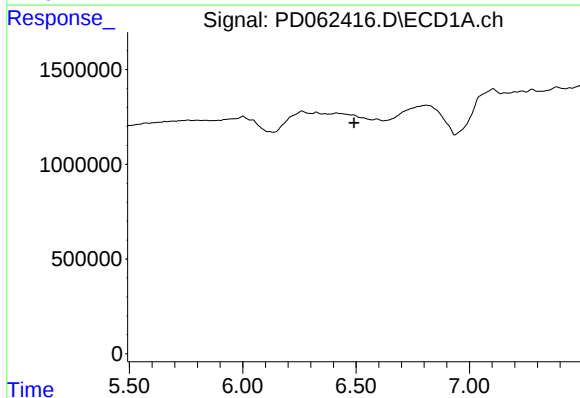


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

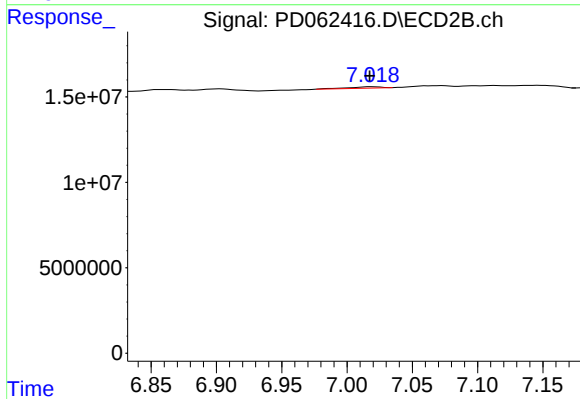

#18 Endrin aldehyde


R.T.: 7.019 min
Delta R.T.: 0.002 min
Response: 1421703
Conc: 0.15 ng/ml

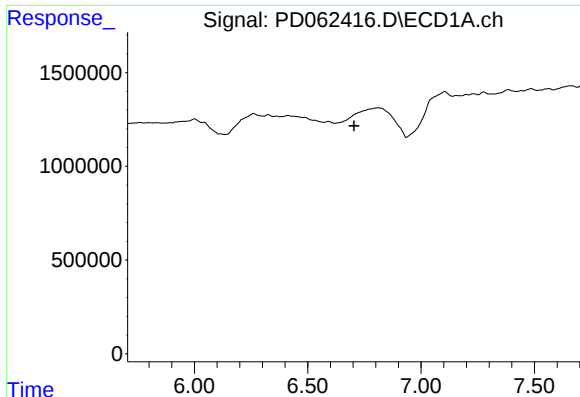

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SB-39-9.5-10.0

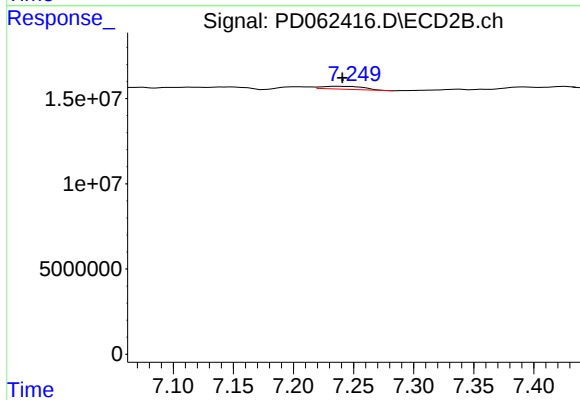


#19 Endosulfan Sulfate

R.T.: 7.237 min
Delta R.T.: -0.003 min
Response: 3976172
Conc: 0.37 ng/ml

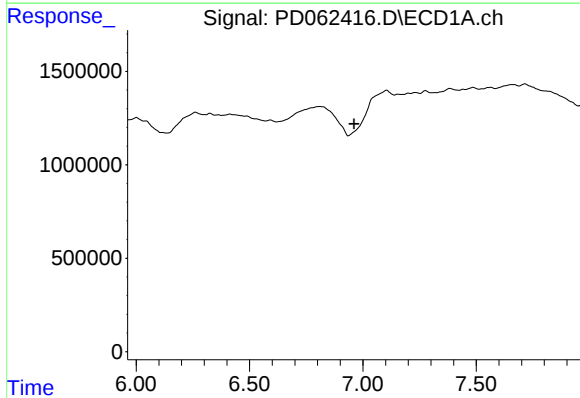


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.962 min
Response: 0
Conc: N.D.

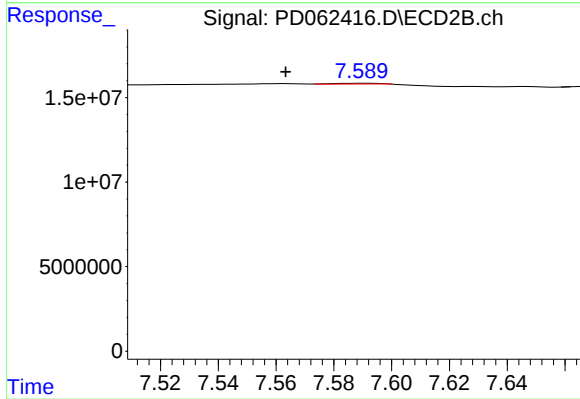

#20 Methoxychlor


R.T.: 7.591 min
Delta R.T.: 0.028 min
Response: 488449
Conc: 0.10 ng/ml

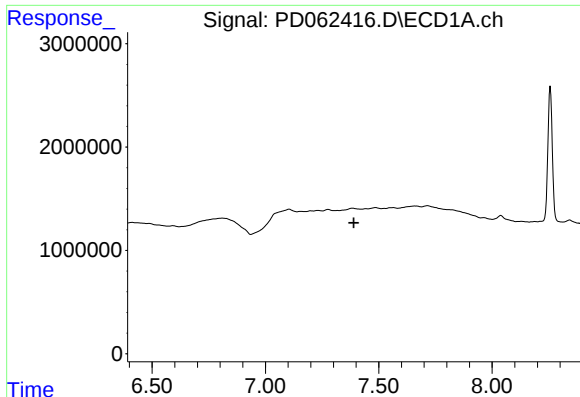

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.390 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SB-39-9.5-10.0

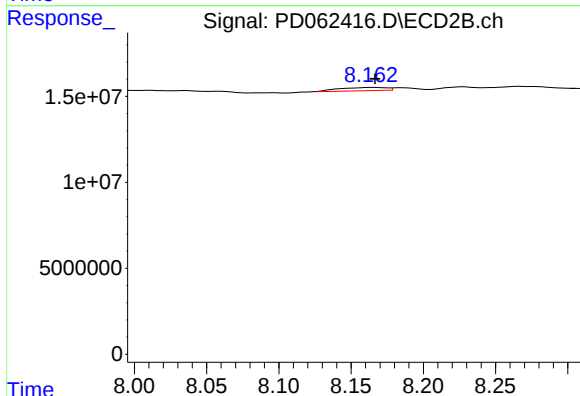


#22 Mirex

R.T.: 8.164 min
Delta R.T.: -0.003 min
Response: 4292911
Conc: 0.69 ng/ml

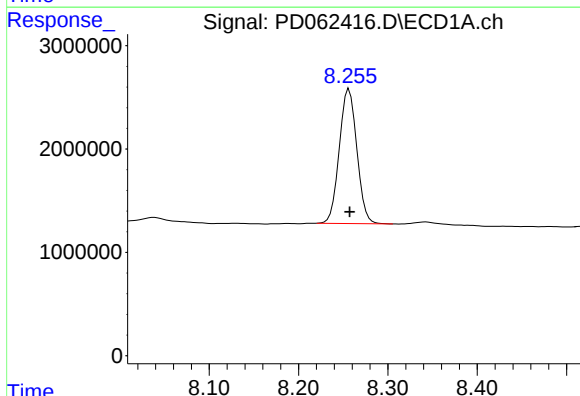

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 17772669
Conc: 14.65 ng/ml

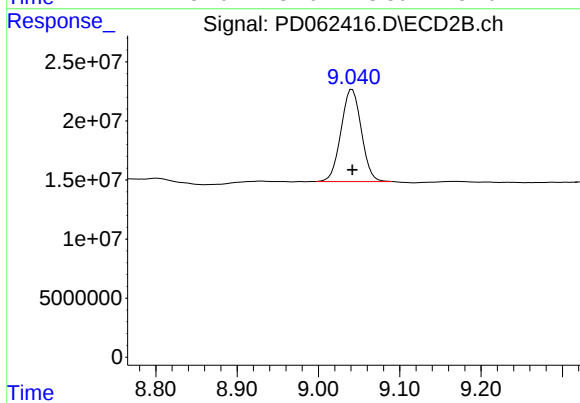

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 135129418
Conc: 15.93 ng/ml