

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
 Data File : PD062422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2021 16:25
 Operator : AR\AJ
 Sample : PB135936BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB135936BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 18:38:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.981	15514699	214.0E6	19.048	20.319
28)	SA Decachlor...	8.256	9.041	22397025	168.7E6	18.464	19.885
Target Compounds							
3)	MA gamma-BHC...	0.000	4.655	0	227702	N.D.	0.014 #
8)	B Heptachlo...	0.000	5.862	0	11014111	N.D.	0.802 #
9)	A Endosulfan I	0.000	6.196	0	987283	N.D.	0.075 #
15)	B Endosulfa...	0.000	6.900	0	4527758	N.D.	0.393 #
18)	B Endrin al...	0.000	7.021	0	491880	N.D.	0.052 #
22)	Mirex	0.000	8.171	0	4449131	N.D.	0.712 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
Data File : PD062422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2021 16:25
Operator : AR\AJ
Sample : PB135936BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB135936BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 18:38:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

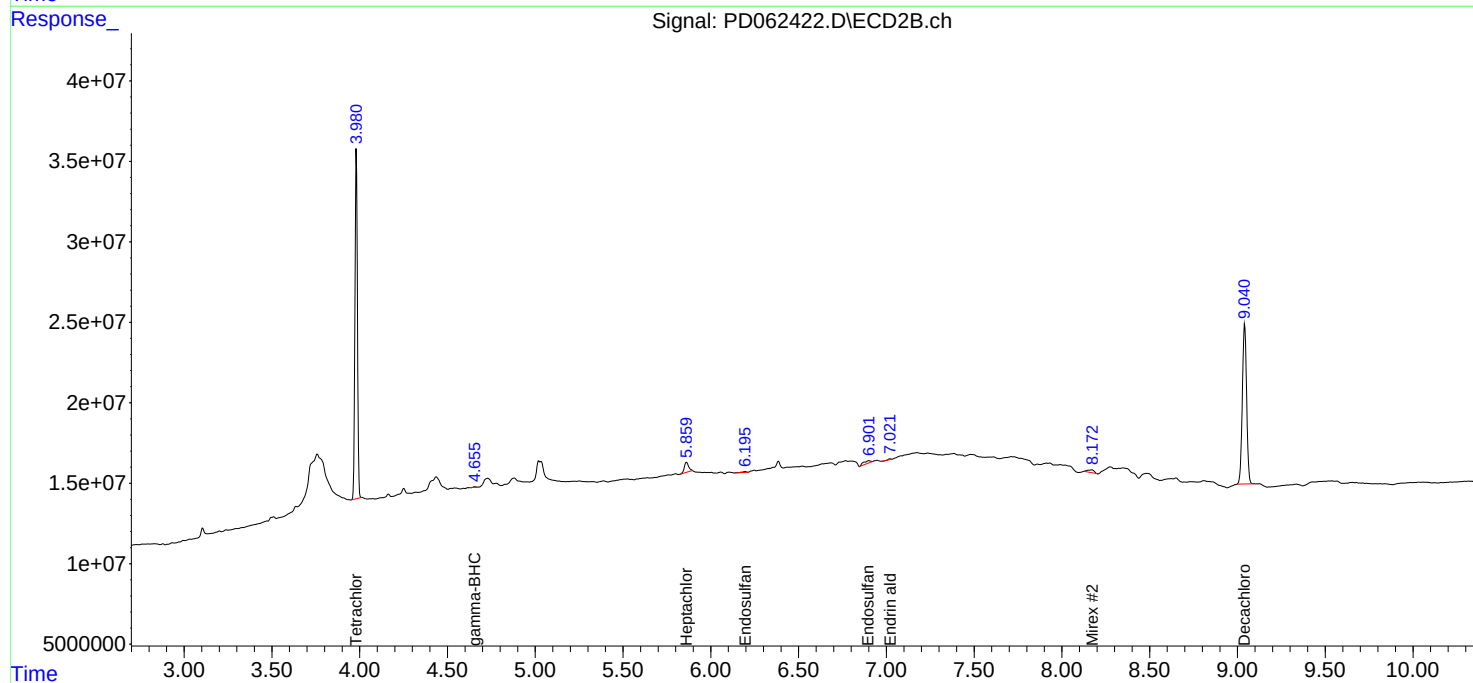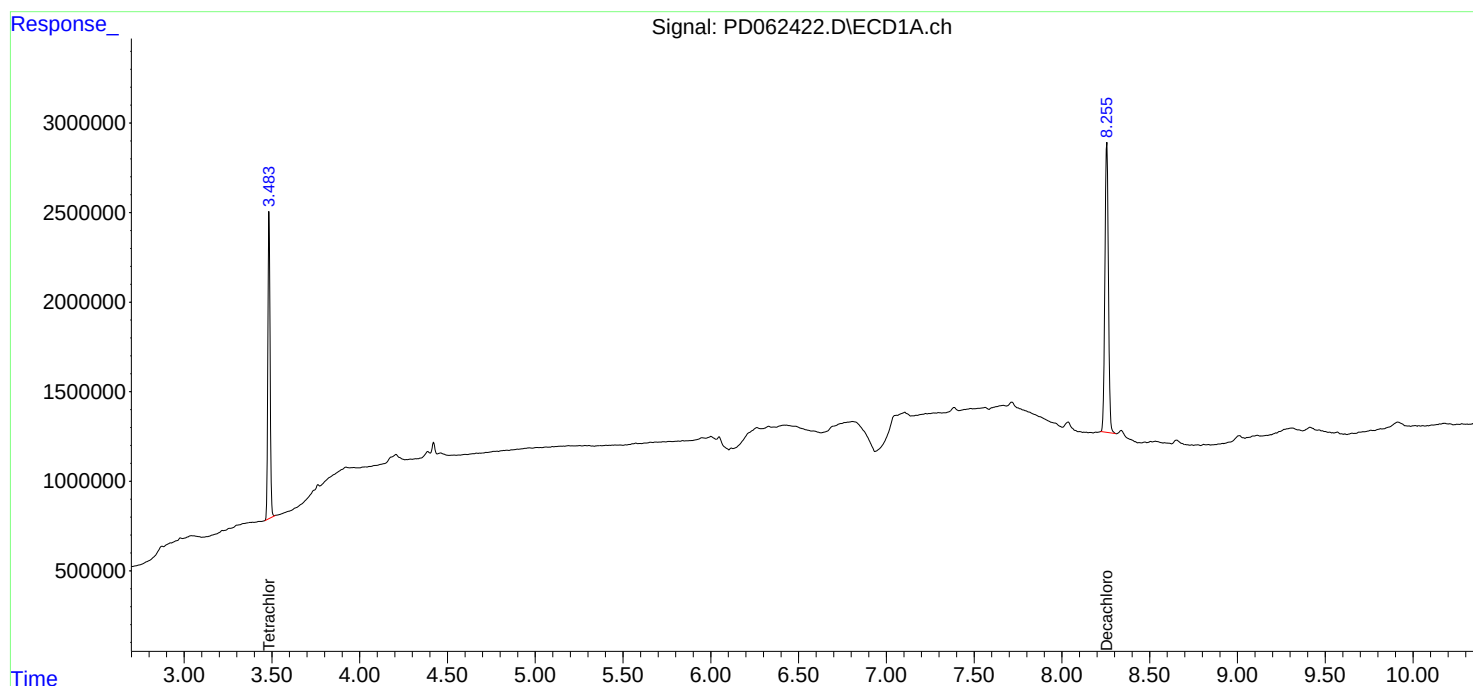


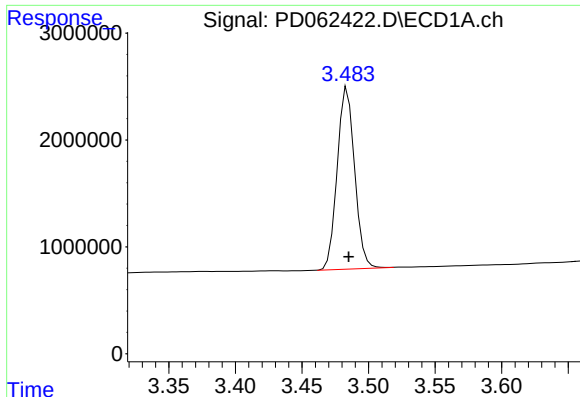

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 15514699
Conc: 19.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB135936BL

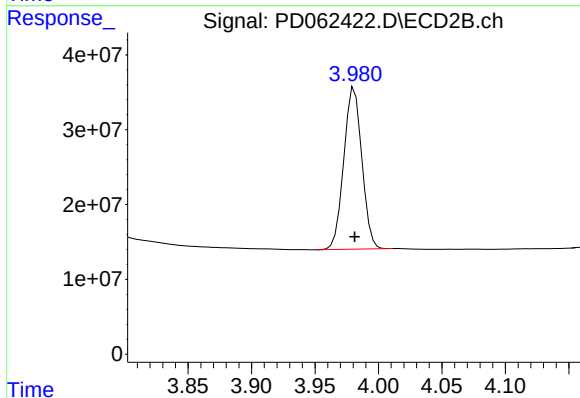


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 213988520
Conc: 20.32 ng/ml

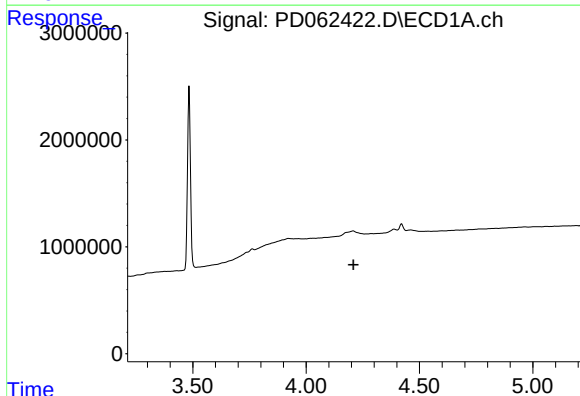


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.209 min
Response: 0
Conc: N.D.

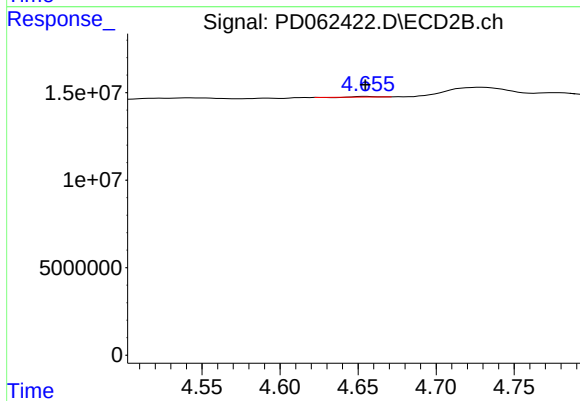

#3 gamma-BHC (Lindane)


R.T.: 4.655 min
Delta R.T.: 0.000 min
Response: 227702
Conc: 0.01 ng/ml

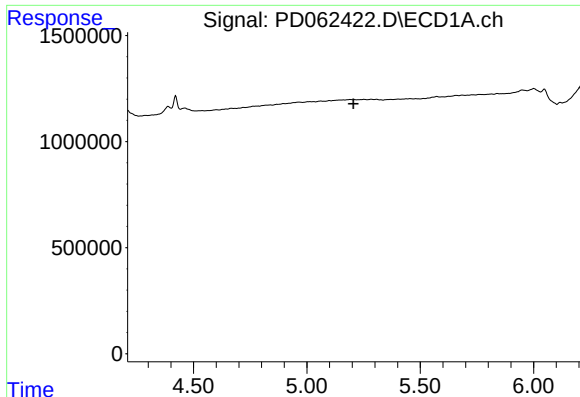

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.206 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB135936BL

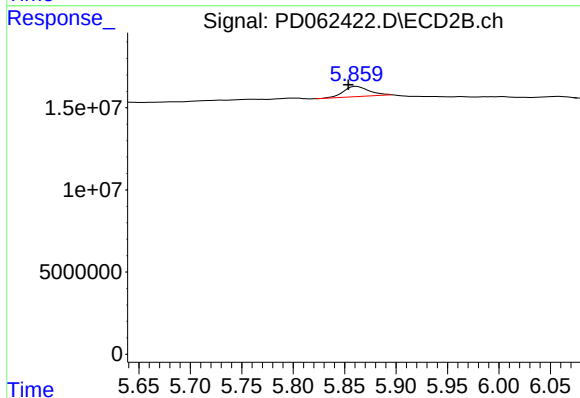


#8 Heptachlor epoxide

R.T.: 5.862 min
Delta R.T.: 0.008 min
Response: 11014111
Conc: 0.80 ng/ml

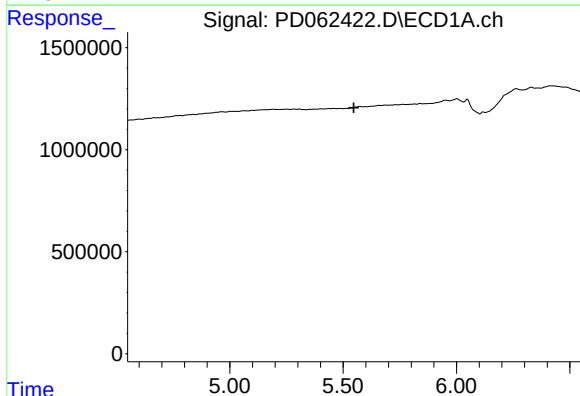


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.547 min
Response: 0
Conc: N.D.

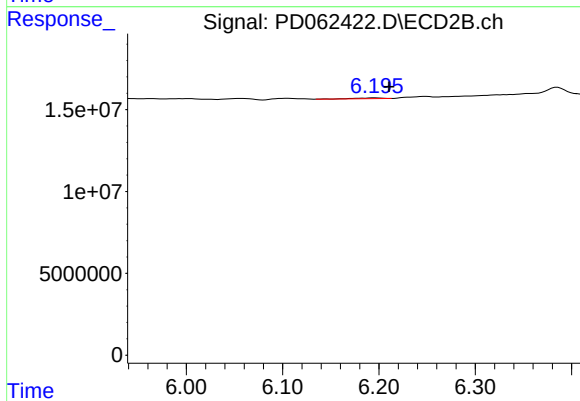

#9 Endosulfan I


R.T.: 6.196 min
Delta R.T.: -0.015 min
Response: 987283
Conc: 0.08 ng/ml

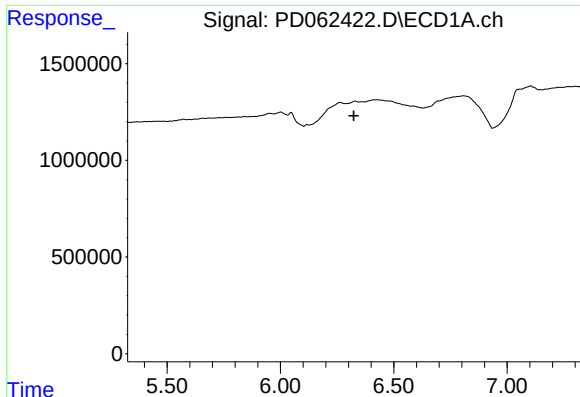

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB135936BL

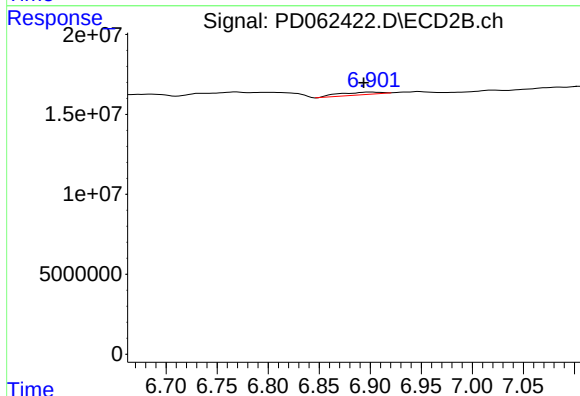


#15 Endosulfan II

R.T.: 6.900 min
Delta R.T.: 0.007 min
Response: 4527758
Conc: 0.39 ng/ml

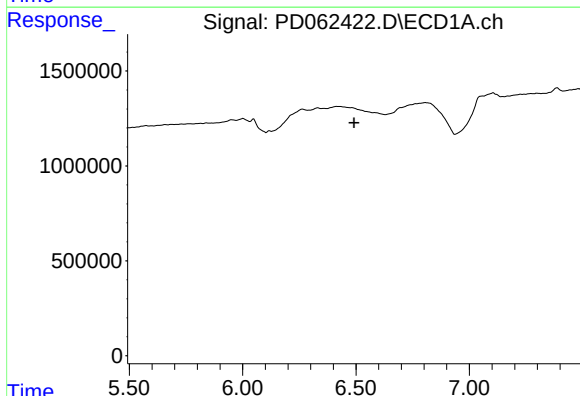


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

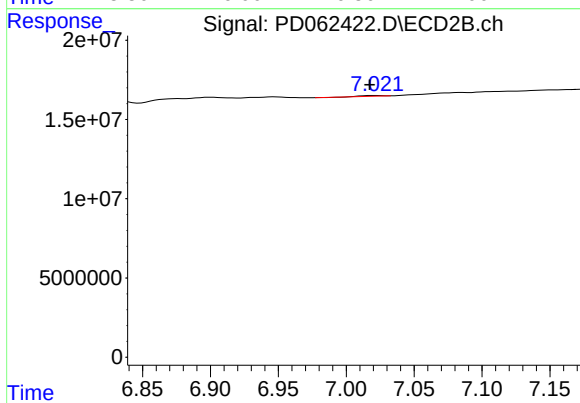

#18 Endrin aldehyde


R.T.: 7.021 min
Delta R.T.: 0.004 min
Response: 491880
Conc: 0.05 ng/ml

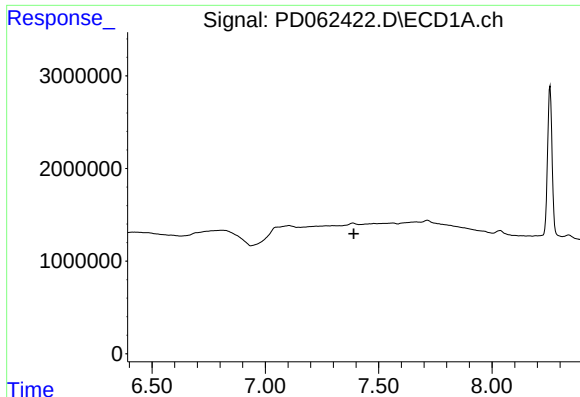

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.390 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB135936BL

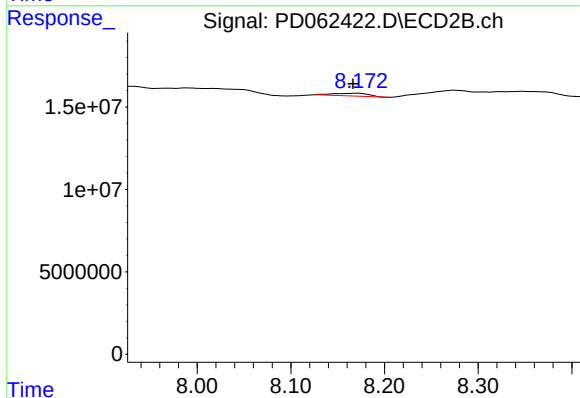


#22 Mirex

R.T.: 8.171 min
Delta R.T.: 0.004 min
Response: 4449131
Conc: 0.71 ng/ml

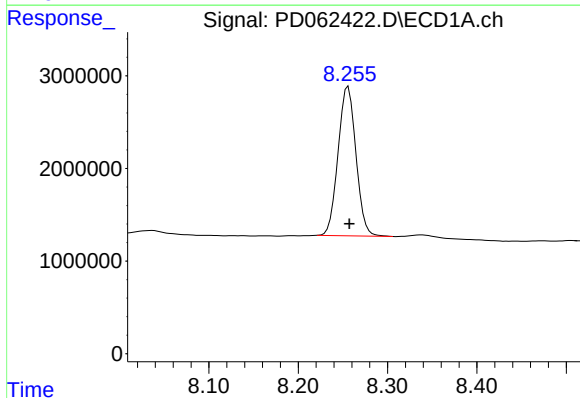

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.002 min
Response: 22397025
Conc: 18.46 ng/ml

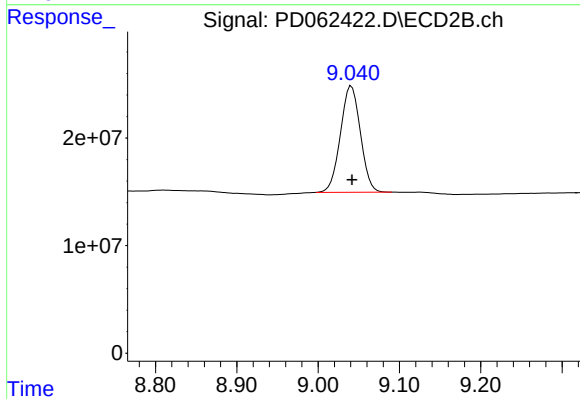

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 168720688
Conc: 19.88 ng/ml