

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
 Data File : PD062403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2021 11:24
 Operator : AR\AJ
 Sample : M2118-03 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 20071

Manual Integrations
 APPROVED

Ankita
 4/27/2021 2:04:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 15:48:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.491	3.978	970802	12607060	1.192	1.197m
28) SA Decachlor...	8.265	9.046	1688962	12214916	1.392	1.440
Target Compounds						
17) MA 4,4'-DDT	6.421	7.112	4773765	24338785	4.675m	2.441 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
Data File : PD062403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2021 11:24
Operator : AR\AJ
Sample : M2118-03 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampled :
20071


Manual Integrations
APPROVED

Ankita
4/27/2021 2:04:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 15:48:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

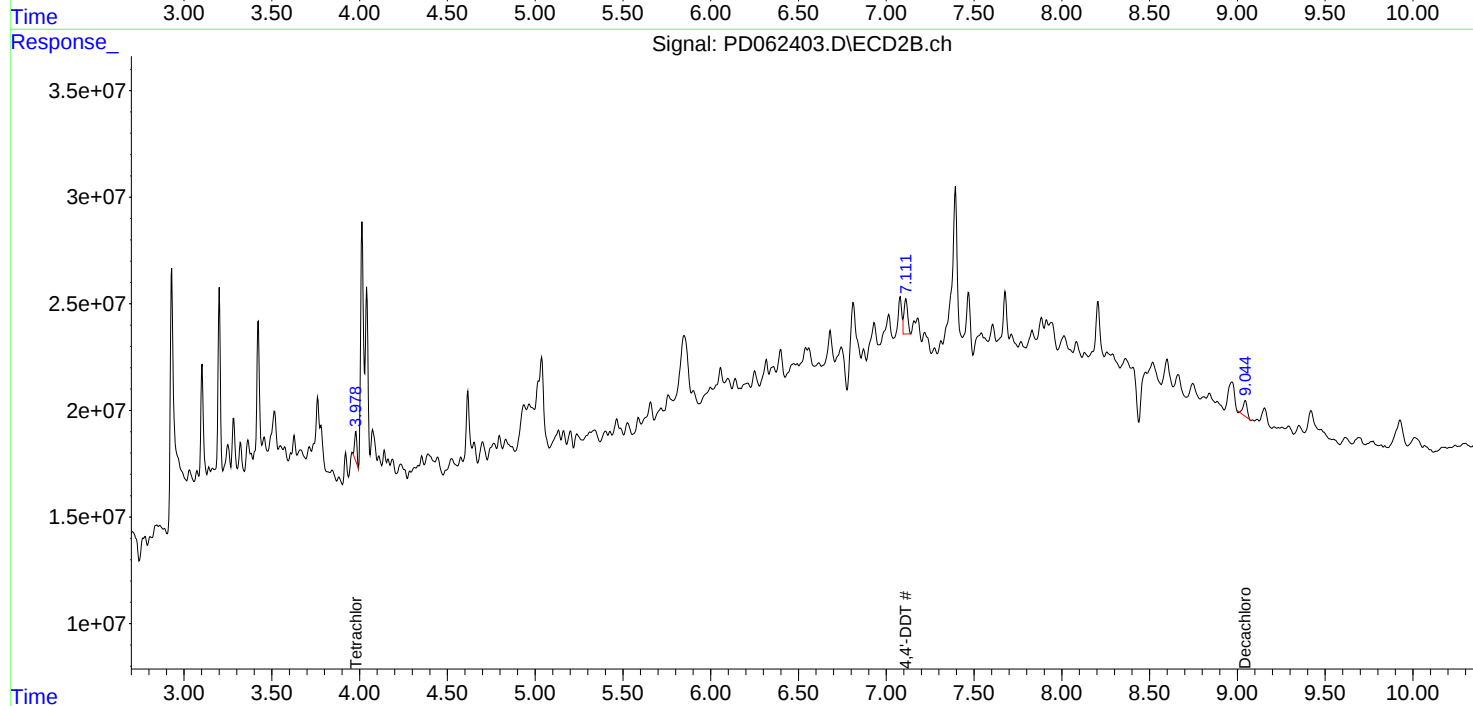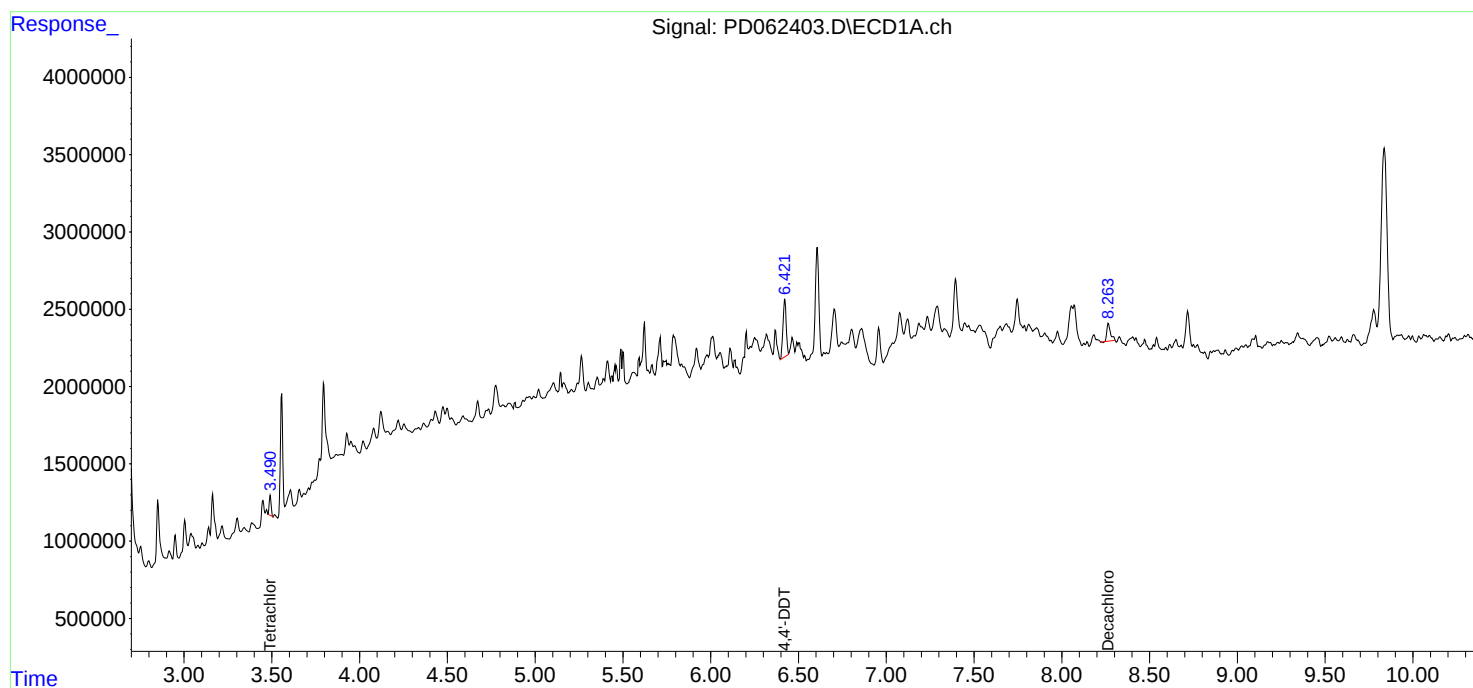

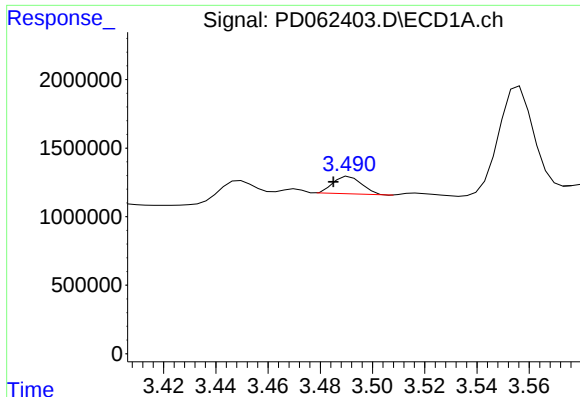


#1 Tetrachloro-m-xylene

R.T.: 3.491 min
Delta R.T.: 0.006 min
Response: 970802
Conc: 1.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
20071


Manual Integrations
APPROVED

Ankita
4/27/2021 2:04:24 PM

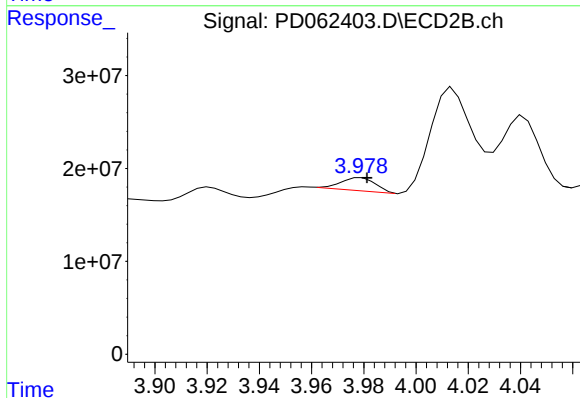


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.003 min
Response: 12607060
Conc: 1.20 ng/ml m

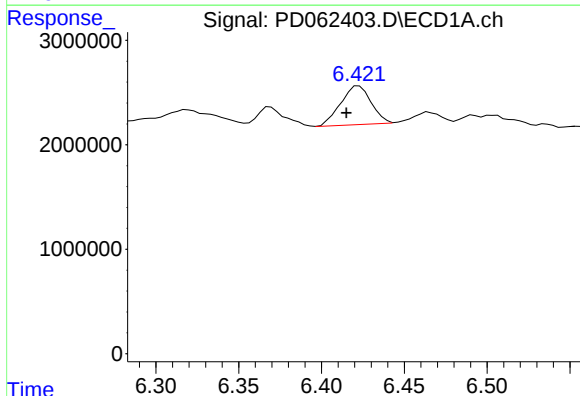


#17 4,4'-DDT

R.T.: 6.421 min
Delta R.T.: 0.006 min
Response: 4773765
Conc: 4.67 ng/ml m

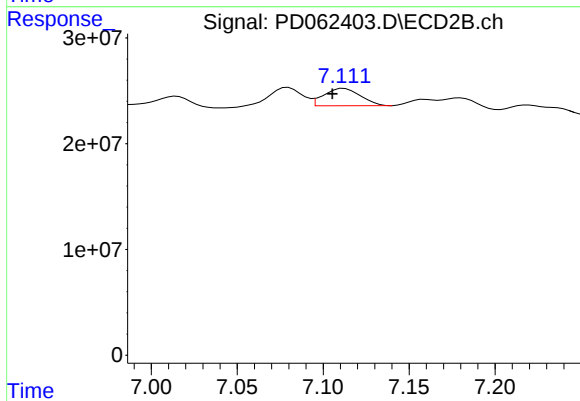

#17 4,4'-DDT

R.T.: 7.112 min
Delta R.T.: 0.007 min
Response: 24338785
Conc: 2.44 ng/ml

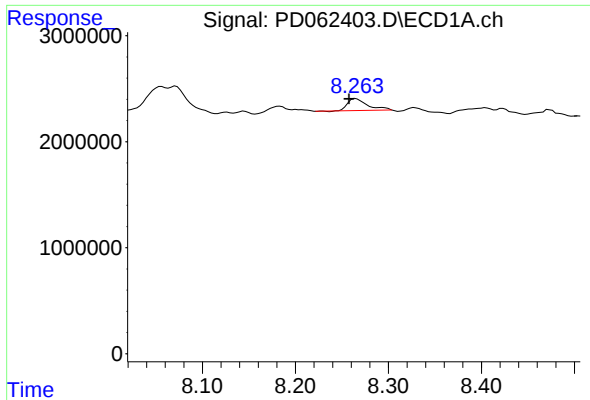


#28 Decachlorobiphenyl

R.T.: 8.265 min
Delta R.T.: 0.007 min
Response: 1688962
Conc: 1.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
20071

Manual Integrations
APPROVED

Ankita
4/27/2021 2:04:24 PM

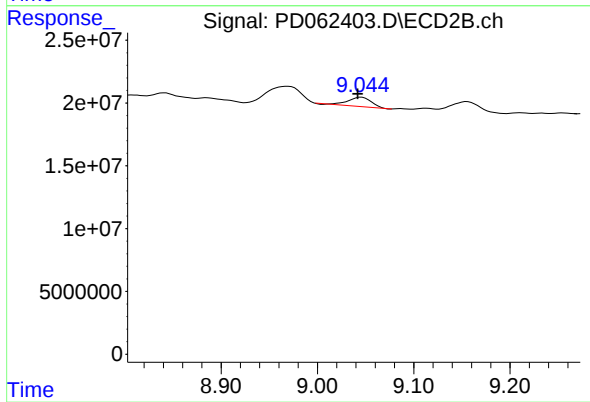

#28 Decachlorobiphenyl

R.T.: 9.046 min
Delta R.T.: 0.004 min
Response: 12214916
Conc: 1.44 ng/ml