

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
 Data File : PD062408.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2021 12:52
 Operator : AR\AJ
 Sample : M2106-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-24-14.5-15.0

Manual Integrations
 APPROVED

Ankita
 4/27/2021 2:04:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 13:25:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.491	3.981	6210732	74645735	7.625	7.088
28) SA Decachlor...	8.264	9.044	11229078	78423305	9.257m	9.243m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
Data File : PD062408.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2021 12:52
Operator : AR\AJ
Sample : M2106-09
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SB-24-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/27/2021 2:04:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 13:25:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

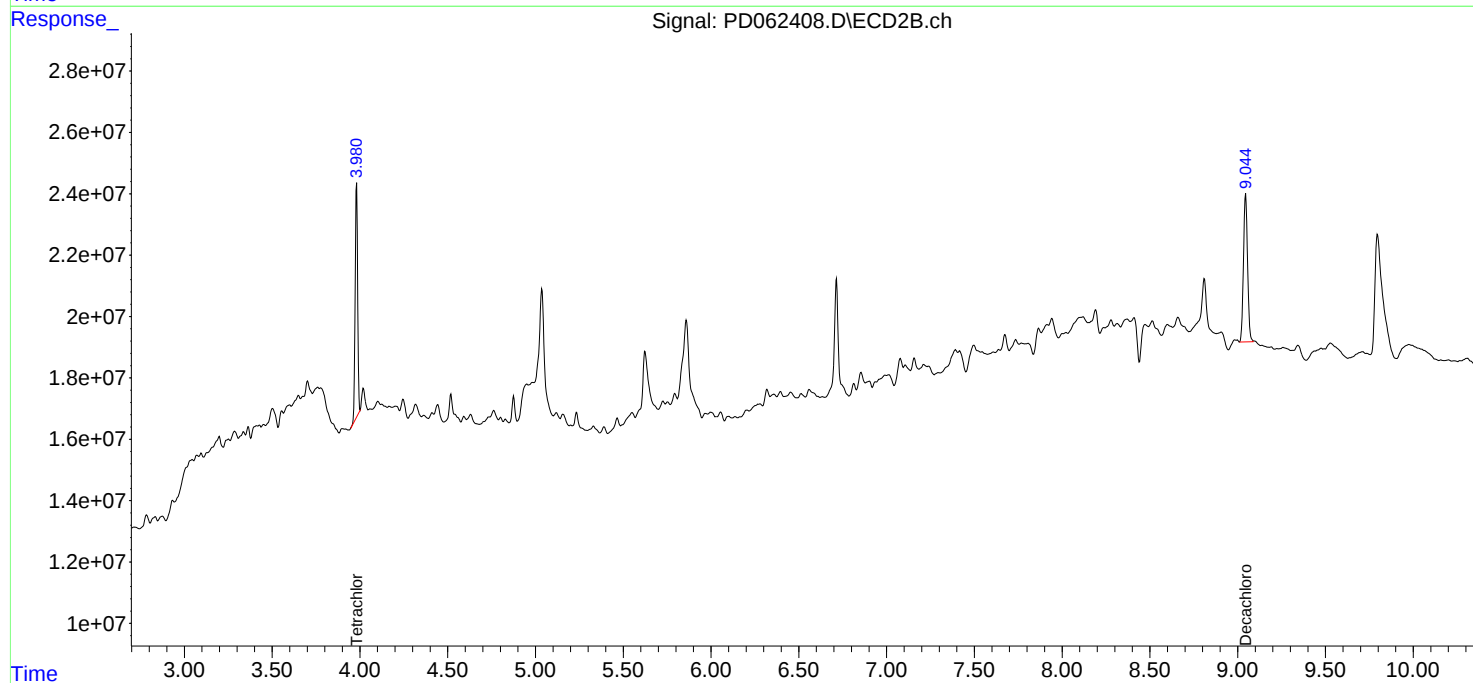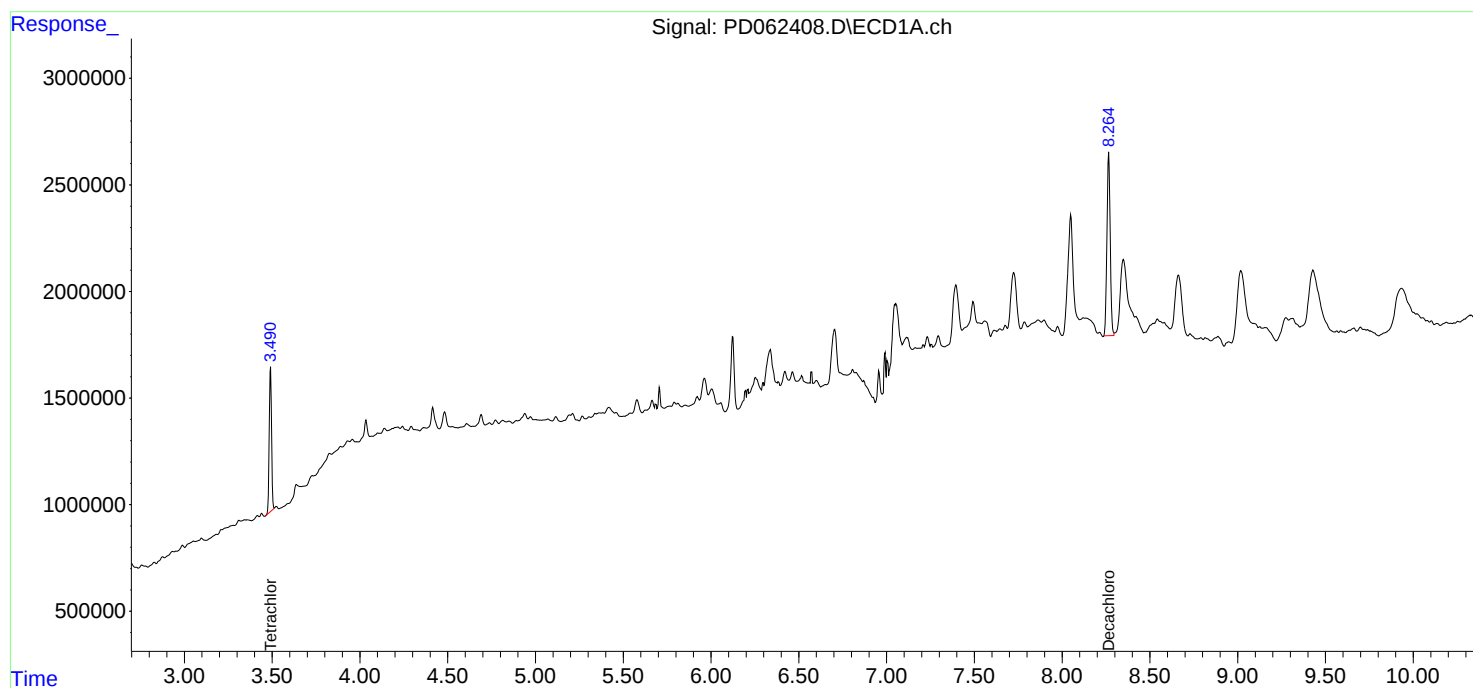

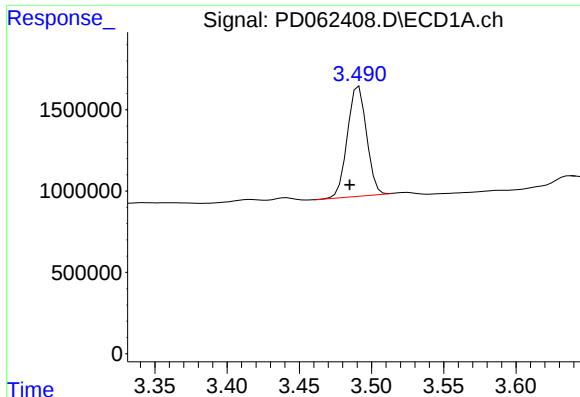


#1 Tetrachloro-m-xylene

R.T.: 3.491 min
Delta R.T.: 0.006 min
Response: 6210732
Conc: 7.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-24-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/27/2021 2:04:28 PM

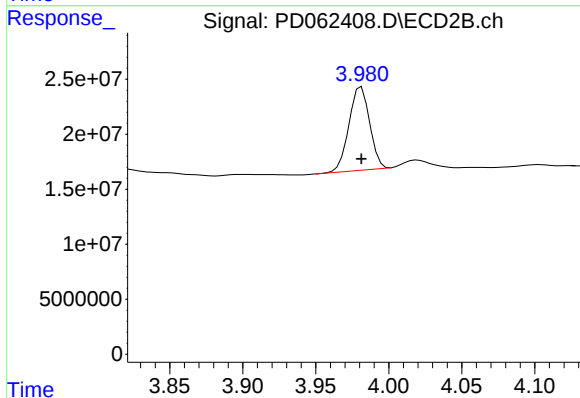


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 74645735
Conc: 7.09 ng/ml

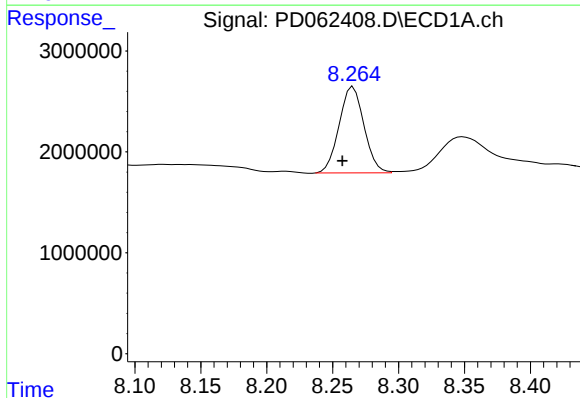

#28 Decachlorobiphenyl

R.T.: 8.264 min
Delta R.T.: 0.007 min
Response: 11229078
Conc: 9.26 ng/ml m

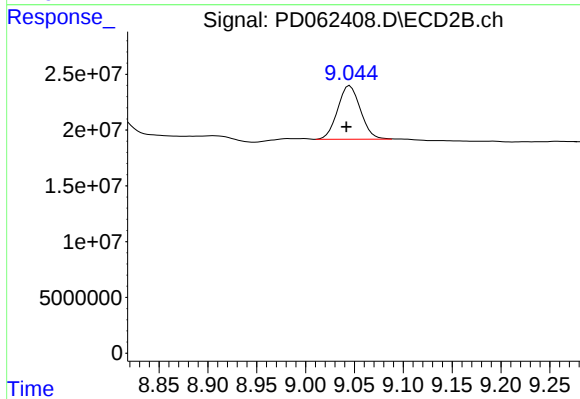

#28 Decachlorobiphenyl

R.T.: 9.044 min
Delta R.T.: 0.002 min
Response: 78423305
Conc: 9.24 ng/ml m