

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
 Data File : PD062413.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2021 14:02
 Operator : AR\AJ
 Sample : M2142-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EO-04-042221

Manual Integrations
 APPROVED

Ankita
 4/28/2021 9:43:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 16:06:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	12024307	144.3E6	14.763	13.706
28)	SA Decachlor...	8.256	9.041	15966663	117.8E6	13.163	13.884
Target Compounds							
17)	MA 4,4'-DDT	6.412	7.105	967386	4761240	0.947m	0.477m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
Data File : PD062413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2021 14:02
Operator : AR\AJ
Sample : M2142-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
EO-04-042221


Manual Integrations
APPROVED

Ankita
4/28/2021 9:43:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 16:06:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

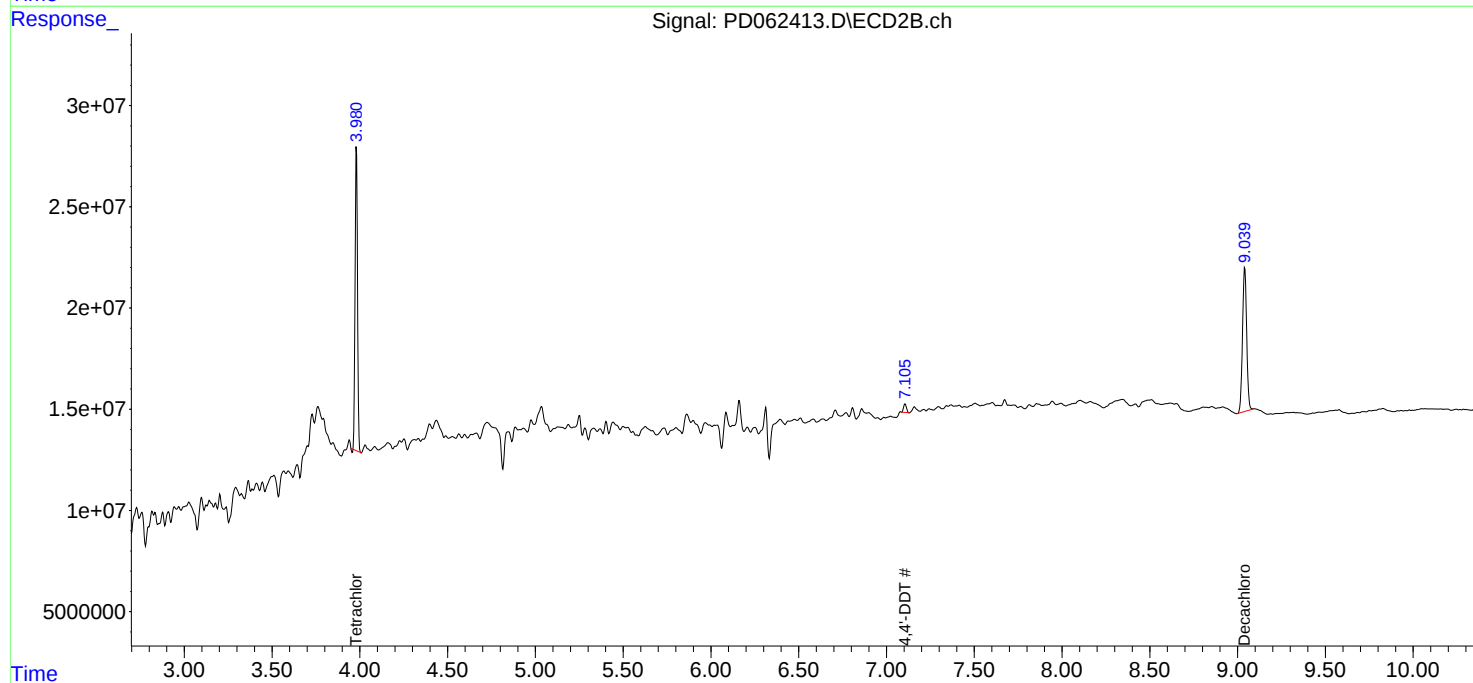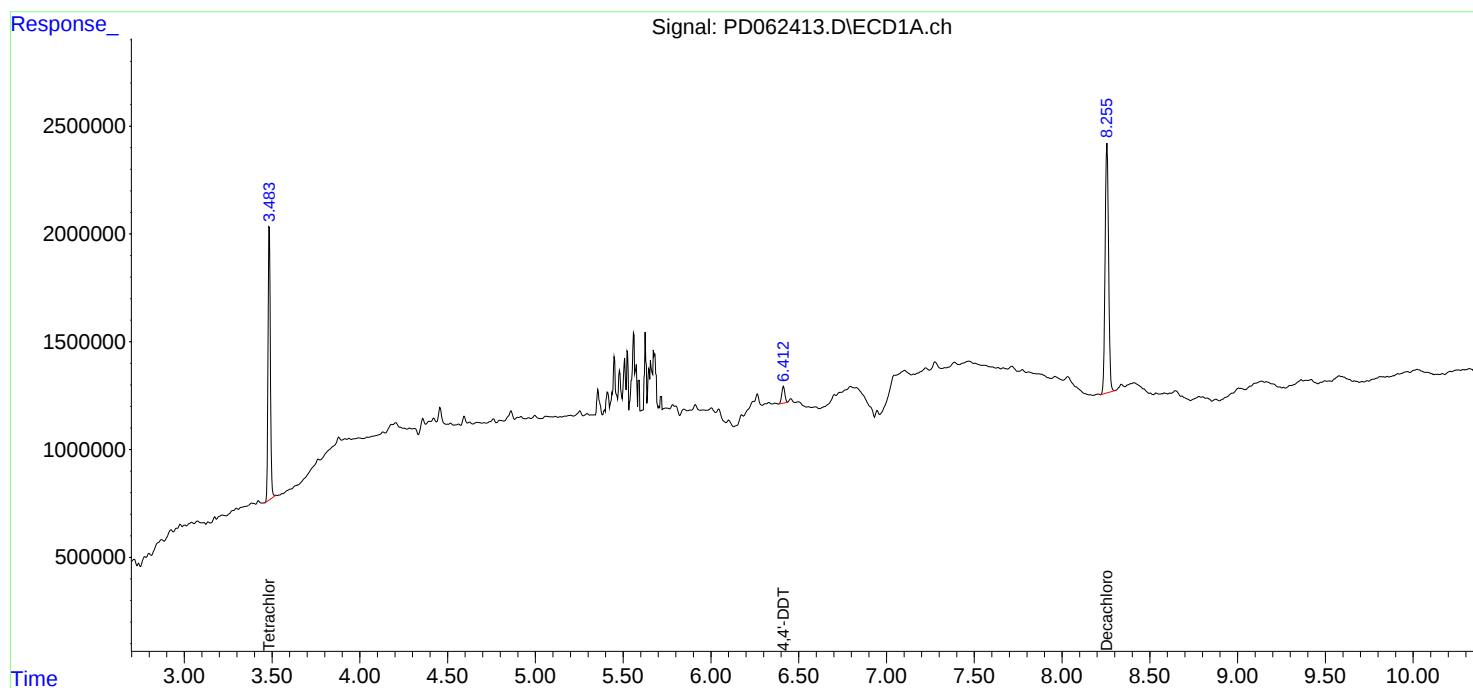

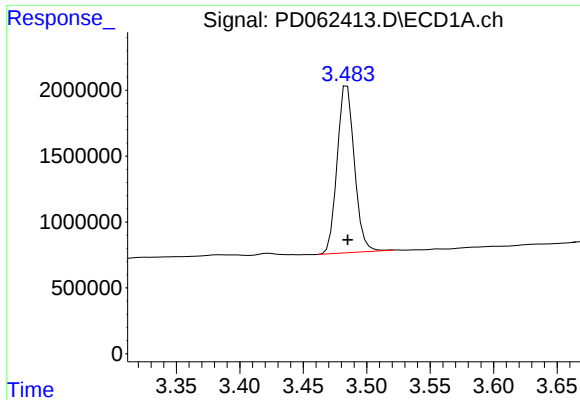


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 12024307
Conc: 14.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
EO-04-042221


Manual Integrations
APPROVED

Ankita
4/28/2021 9:43:36 AM

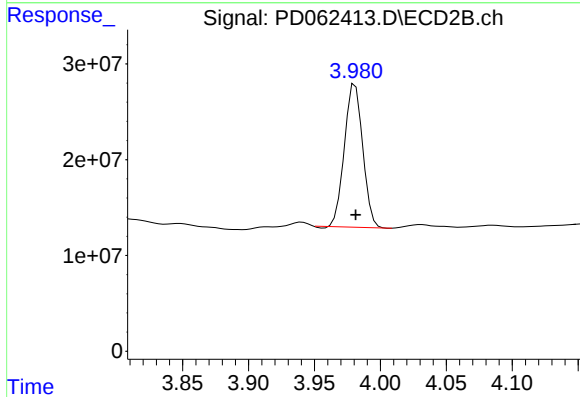


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 144339013
Conc: 13.71 ng/ml

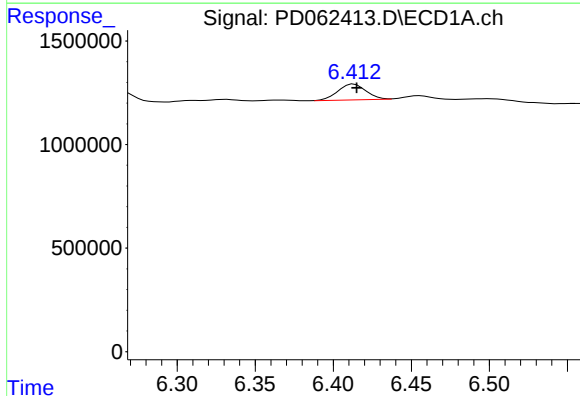


#17 4,4'-DDT

R.T.: 6.412 min
Delta R.T.: -0.003 min
Response: 967386
Conc: 0.95 ng/ml m

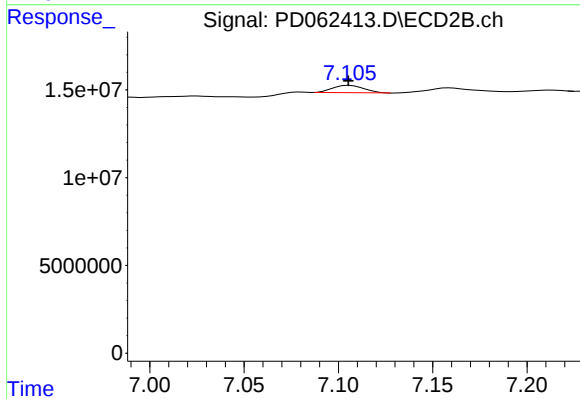

#17 4,4'-DDT

R.T.: 7.105 min
Delta R.T.: 0.000 min
Response: 4761240
Conc: 0.48 ng/ml m

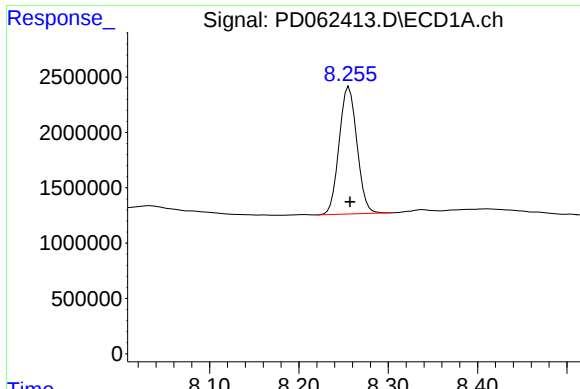


#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.001 min
Response: 15966663
Conc: 13.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
EO-04-042221

Manual Integrations
APPROVED

Ankita
4/28/2021 9:43:36 AM

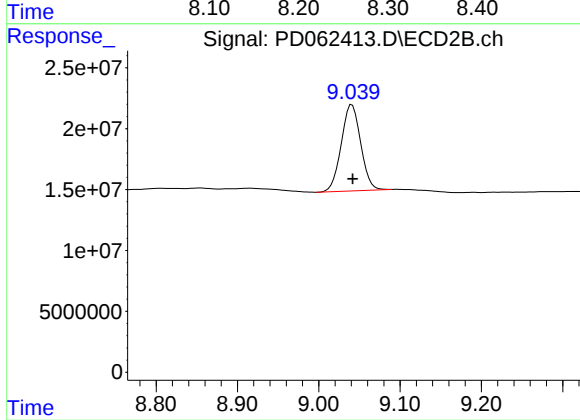

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 117804847
Conc: 13.88 ng/ml