

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
 Data File : PD062428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2021 17:48
 Operator : AR\AJ
 Sample : M2163-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TT-059-RW8-IDWSO-202104-1

Manual Integrations
 APPROVED

Ankita
 4/27/2021 2:04:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 18:40:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.981	16609393	223.5E6	20.392	21.227
28)	SA Decachlor...	8.257	9.040	21247156	156.3E6	17.516	18.424
Target Compounds							
10)	B gamma-Chl...	5.434	6.086	608260	11688771	0.477m	0.828m#
11)	B alpha-Chl...	5.490	6.161	605314	13340030	0.482m	0.972 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
Data File : PD062428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2021 17:48
Operator : AR\AJ
Sample : M2163-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TT-059-RW8-IDWSO-202104-1


Manual Integrations
APPROVED

Ankita
4/27/2021 2:04:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 18:40:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

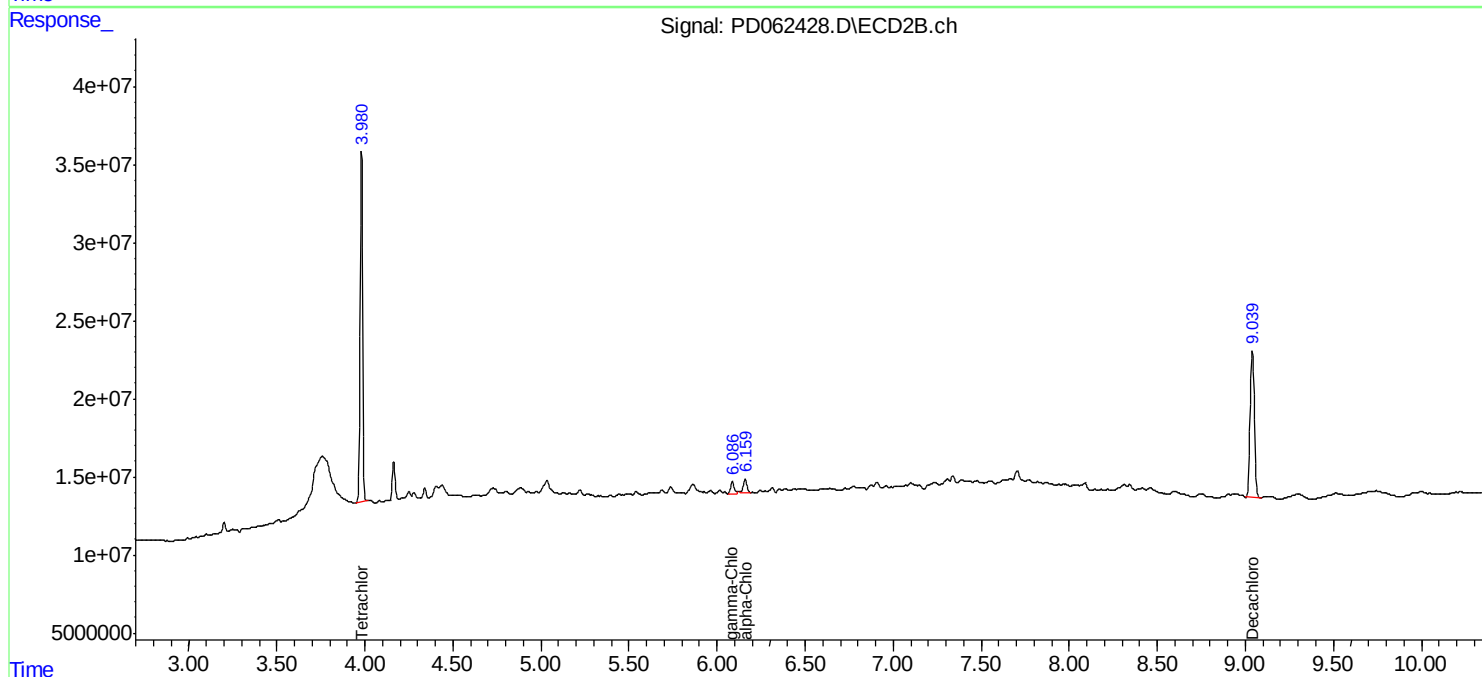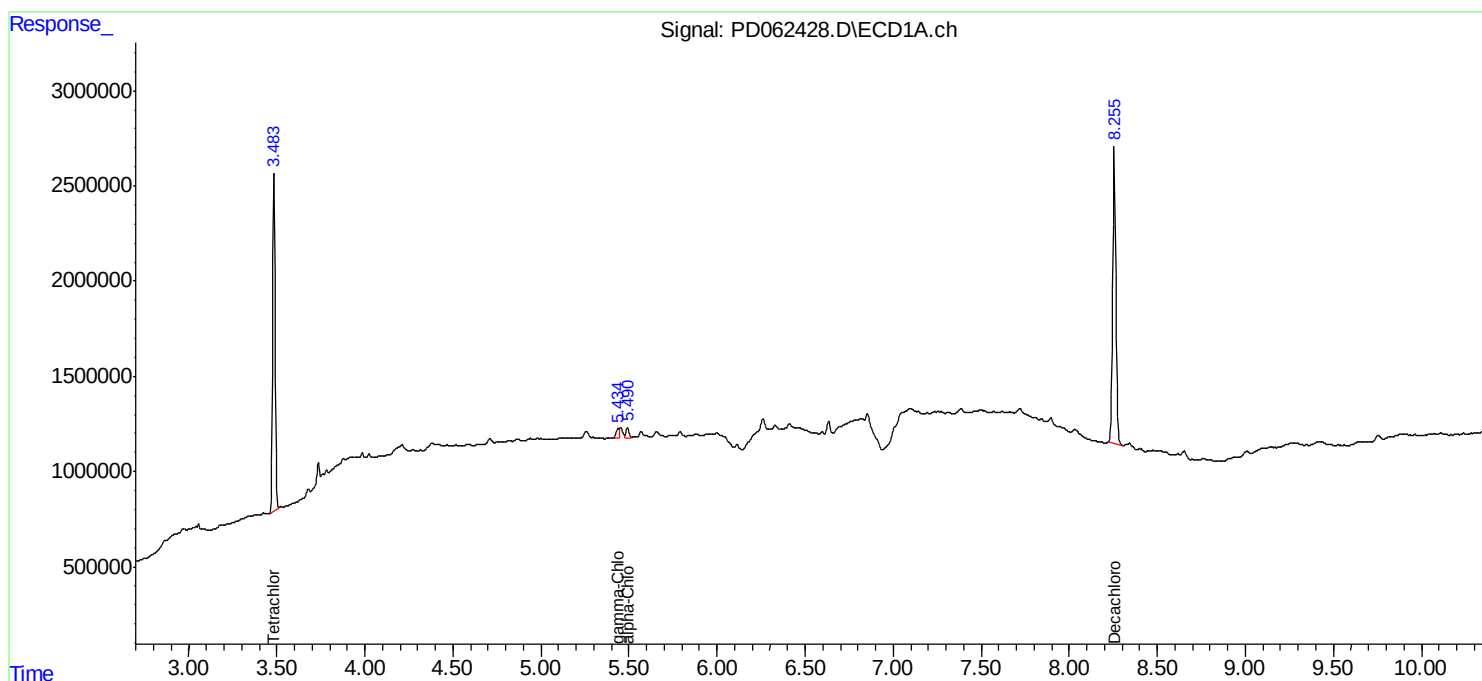

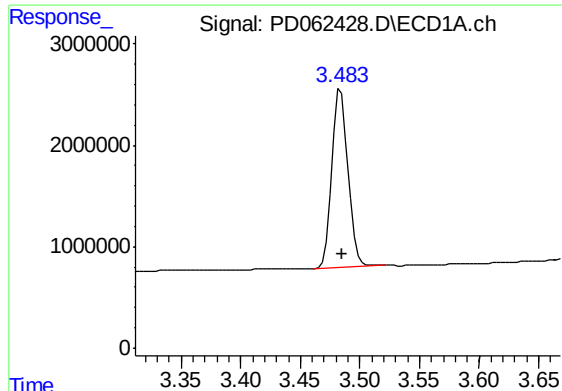


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 16609393
Conc: 20.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
TT-059-RW8-IDWSO-202104-1


Manual Integrations
APPROVED

Ankita
4/27/2021 2:04:36 PM

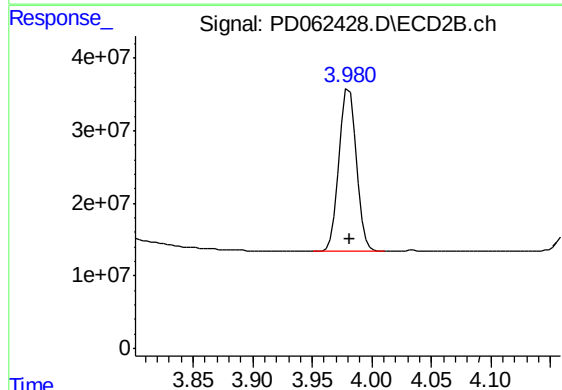


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 223547372
Conc: 21.23 ng/ml

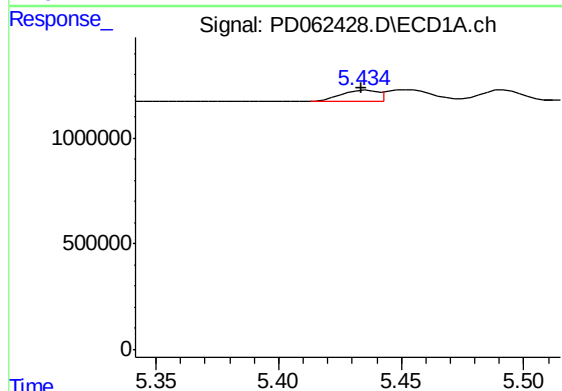


#10 gamma-Chlordane

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 608260
Conc: 0.48 ng/ml m

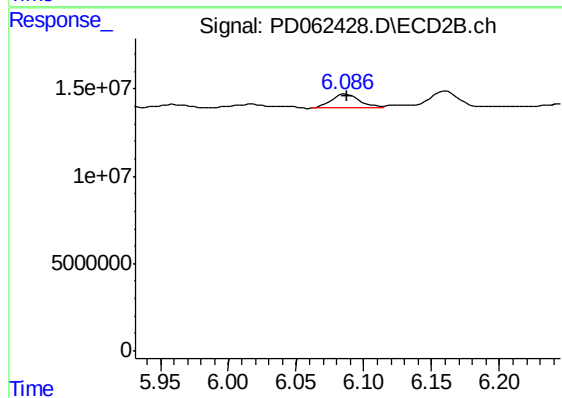

#10 gamma-Chlordane

R.T.: 6.086 min
Delta R.T.: -0.002 min
Response: 11688771
Conc: 0.83 ng/ml m

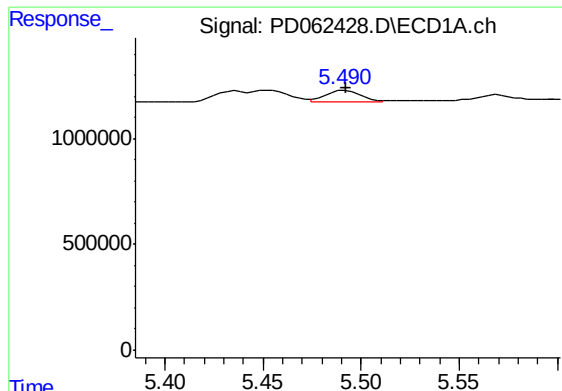


#11 alpha-Chlordane

R.T.: 5.490 min
Delta R.T.: -0.002 min
Response: 605314
Conc: 0.48 ng/ml m

Instrument :
ECD_D
ClientSampleId :
TT-059-RW8-IDWSO-202104-1


Manual Integrations
APPROVED

Ankita
4/27/2021 2:04:36 PM

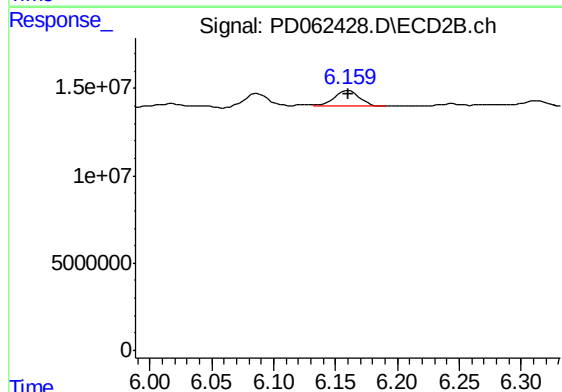


#11 alpha-Chlordane

R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 13340030
Conc: 0.97 ng/ml

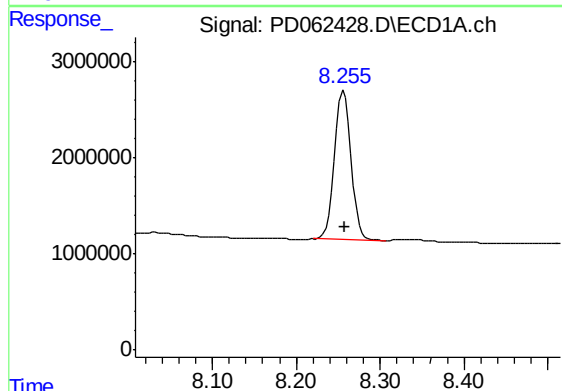

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 21247156
Conc: 17.52 ng/ml

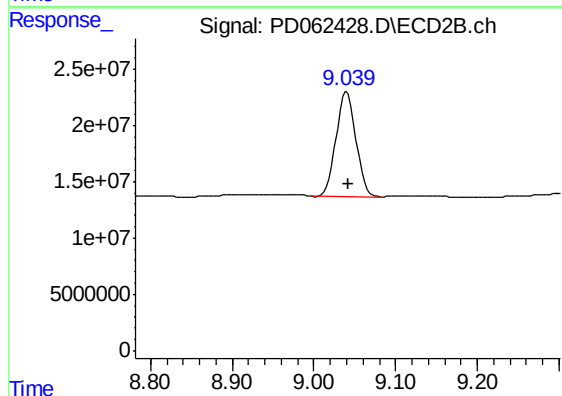

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: -0.002 min
Response: 156331671
Conc: 18.42 ng/ml