

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
 Data File : PD062465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2021 03:35
 Operator : AR\AJ
 Sample : M2176-09
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 STOCKPILE-COMP-2

Manual Integrations
 APPROVED

Ankita
 4/27/2021 2:04:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 05:46:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.979	9477530	121.4E6	11.636	11.523m
28)	SA Decachlor...	8.254	9.039	13223579	96676160	10.901	11.394
Target Compounds							
12)	B 4,4'-DDE	5.652	6.309	1247442	22113009	1.028m	1.566m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
Data File : PD062465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2021 03:35
Operator : AR\AJ
Sample : M2176-09
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
STOCKPILE-COMP-2


Manual Integrations
APPROVED

Ankita
4/27/2021 2:04:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 05:46:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

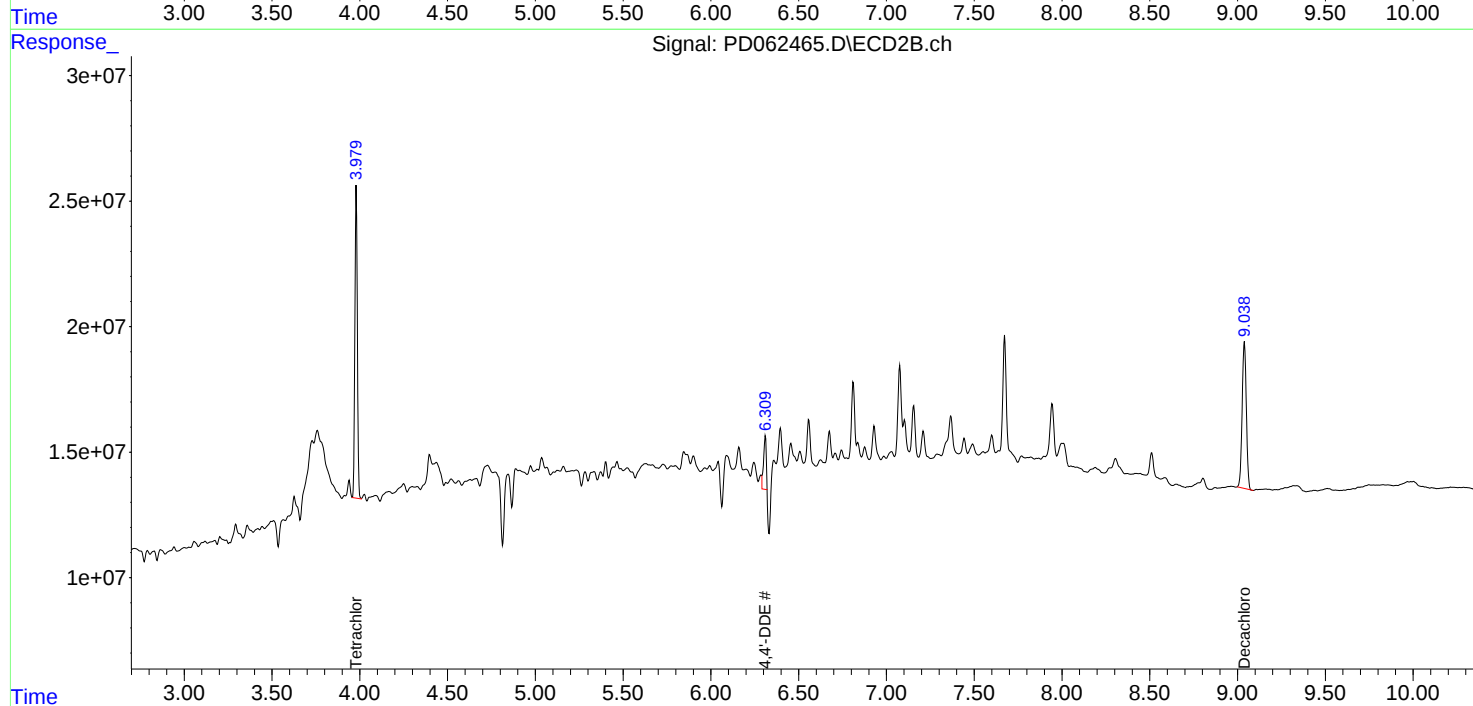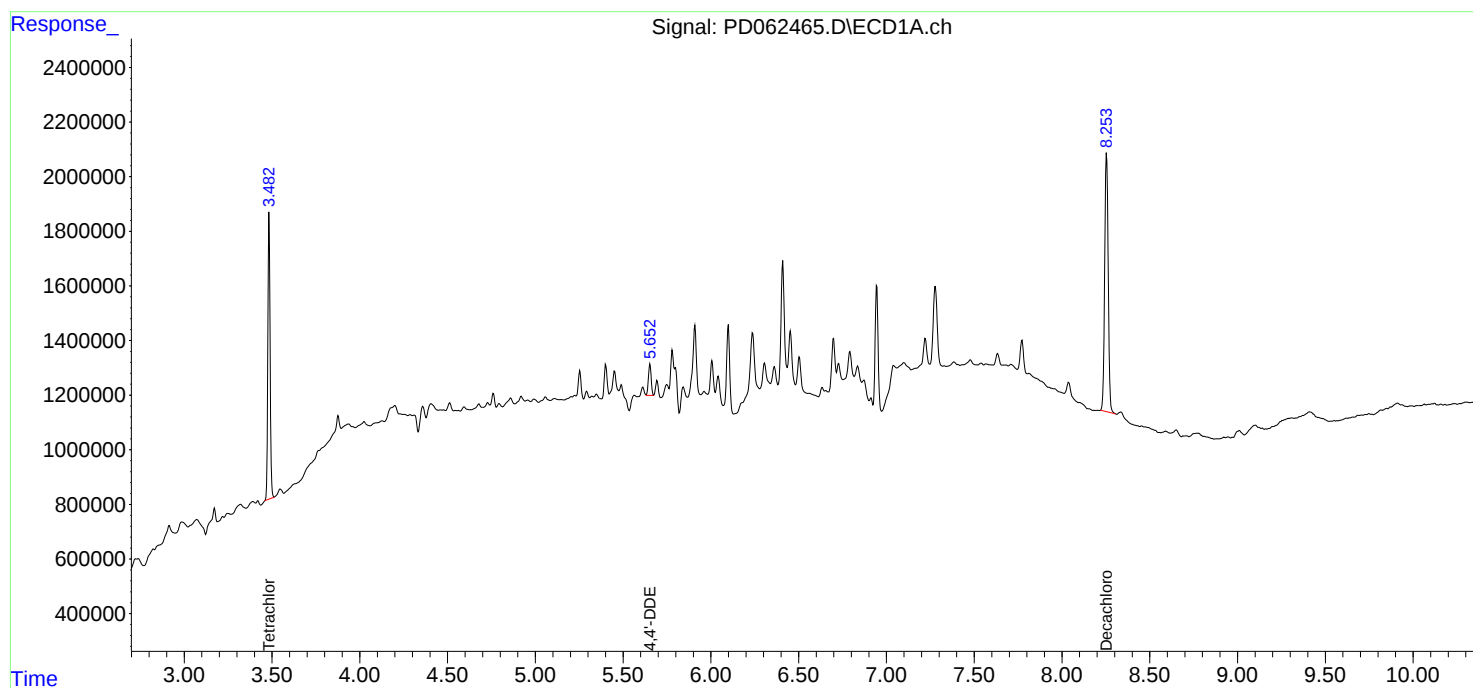

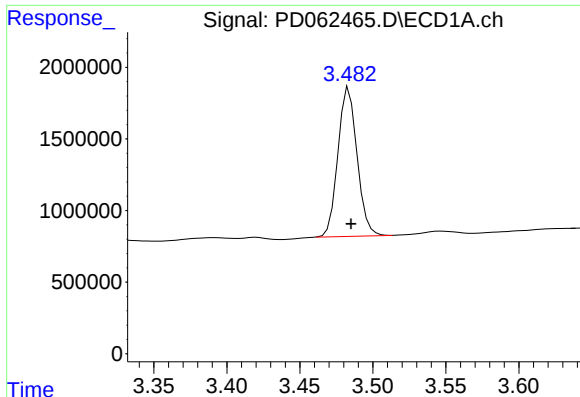


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: -0.001 min
Response: 9477530
Conc: 11.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
STOCKPILE-COMP-2


Manual Integrations
APPROVED

Ankita
4/27/2021 2:04:58 PM

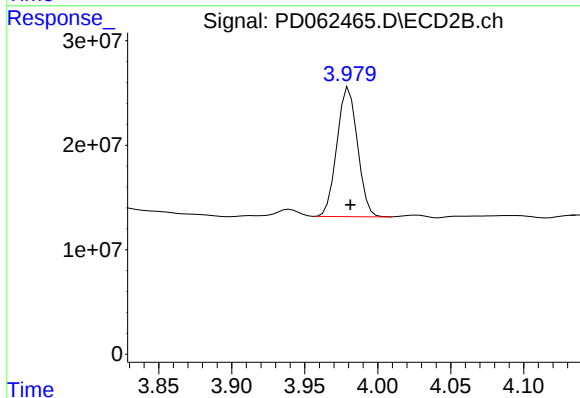


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.002 min
Response: 121353781
Conc: 11.52 ng/ml m

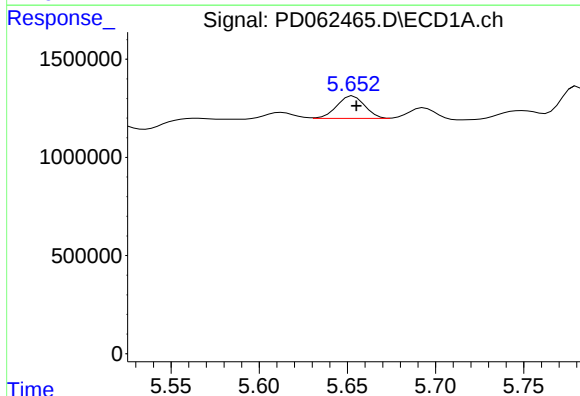


#12 4,4'-DDE

R.T.: 5.652 min
Delta R.T.: -0.003 min
Response: 1247442
Conc: 1.03 ng/ml m

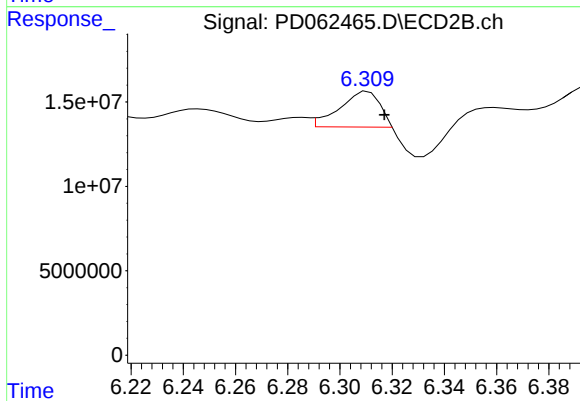

#12 4,4'-DDE

R.T.: 6.309 min
Delta R.T.: -0.008 min
Response: 22113009
Conc: 1.57 ng/ml m

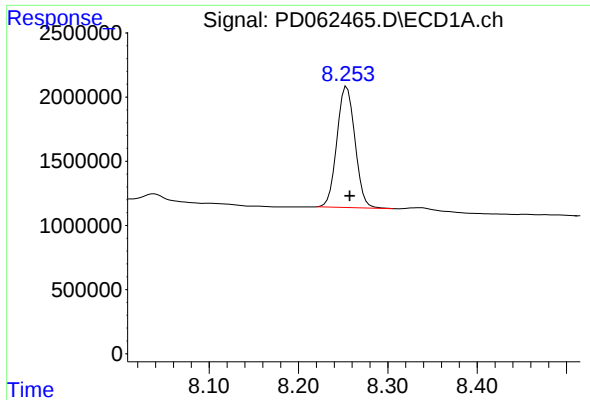


#28 Decachlorobiphenyl

R.T.: 8.254 min
Delta R.T.: -0.003 min
Response: 13223579
Conc: 10.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
STOCKPILE-COMP-2

Manual Integrations
APPROVED

Ankita
4/27/2021 2:04:58 PM

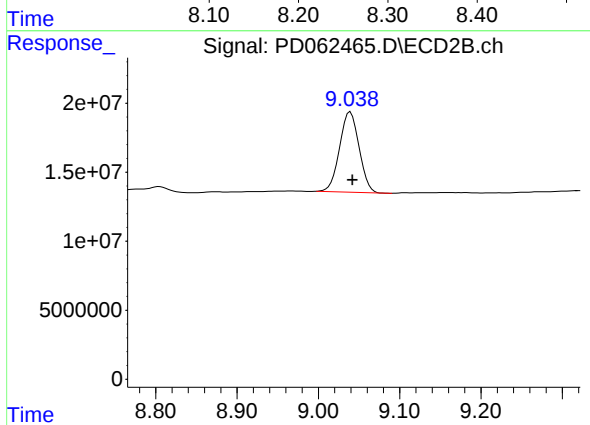

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: -0.003 min
Response: 96676160
Conc: 11.39 ng/ml