

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
 Data File : PD062466.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2021 03:49
 Operator : AR\AJ
 Sample : M2176-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 STOCKPILE-COMP-3

Manual Integrations
 APPROVED

Ankita
 4/27/2021 2:04:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 05:46:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.979	11473208	138.2E6	14.086	13.126m
28)	SA Decachlor...	8.254	9.040	15214911	117.5E6	12.543	13.854
Target Compounds							
12)	B 4,4'-DDE	5.652	6.311	2033393	29231240	1.675m	2.070m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
Data File : PD062466.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2021 03:49
Operator : AR\AJ
Sample : M2176-14
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
STOCKPILE-COMP-3


Manual Integrations
APPROVED

Ankita
4/27/2021 2:04:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 05:46:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

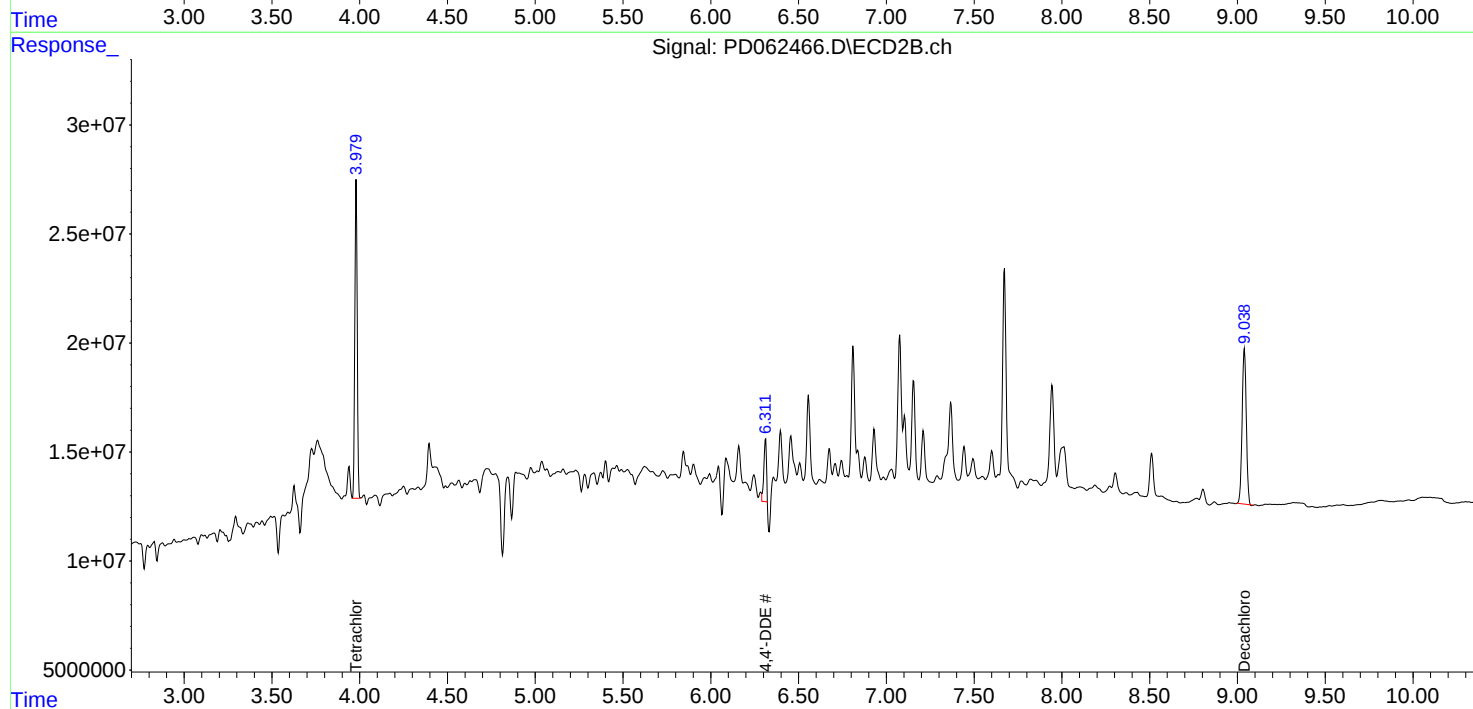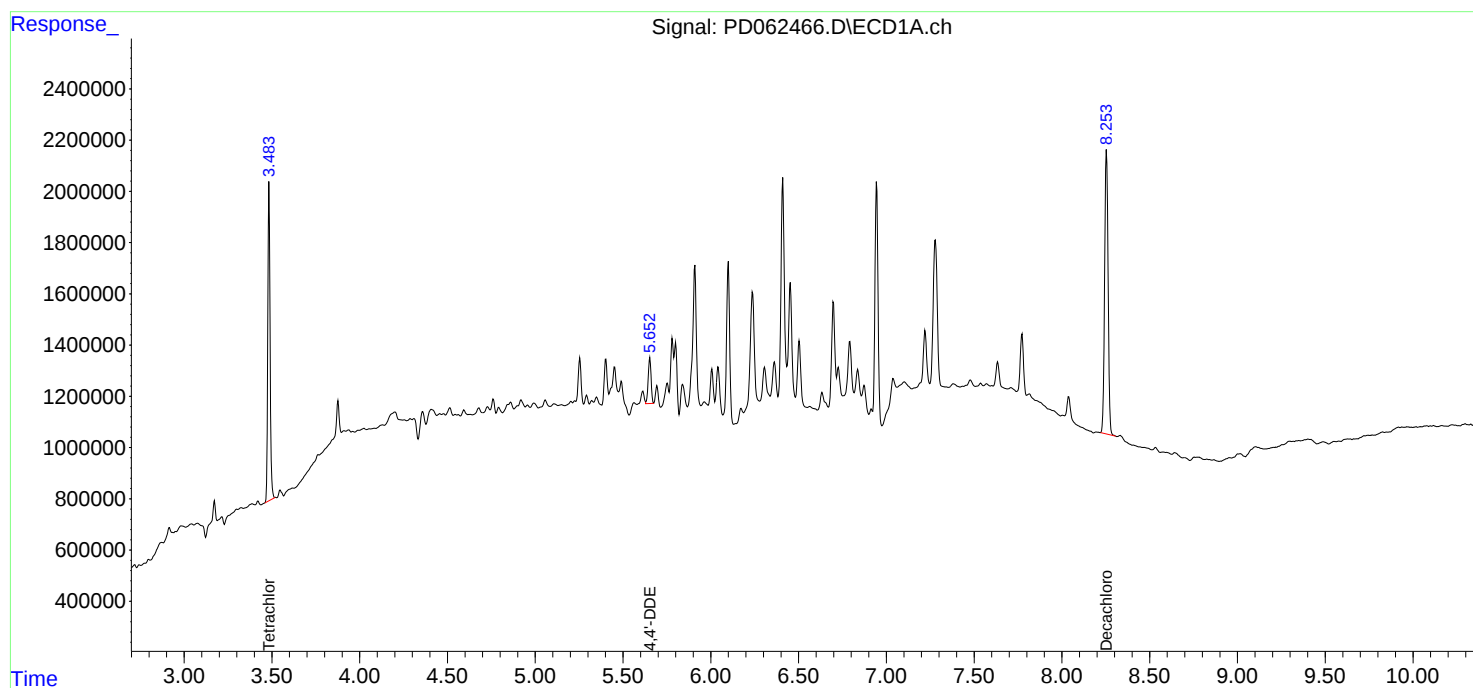

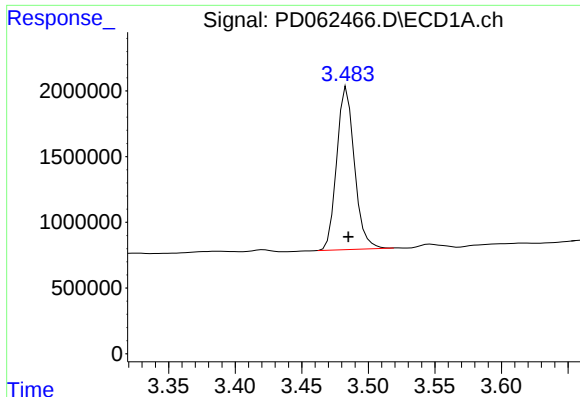


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: -0.001 min
Response: 11473208
Conc: 14.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
STOCKPILE-COMP-3


Manual Integrations
APPROVED

Ankita
4/27/2021 2:04:59 PM

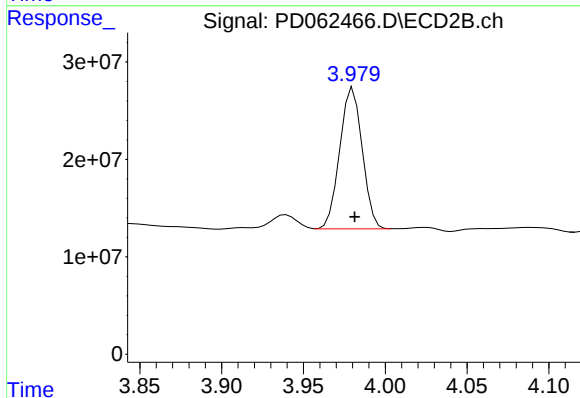


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.002 min
Response: 138238581
Conc: 13.13 ng/ml m

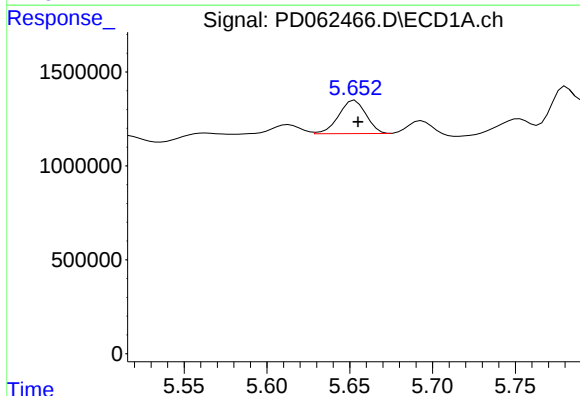


#12 4,4'-DDE

R.T.: 5.652 min
Delta R.T.: -0.003 min
Response: 2033393
Conc: 1.68 ng/ml m

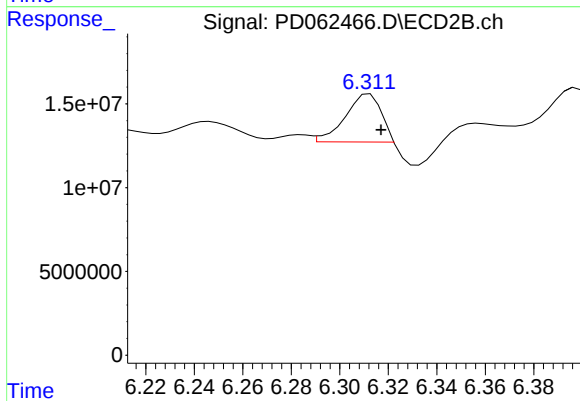

#12 4,4'-DDE

R.T.: 6.311 min
Delta R.T.: -0.006 min
Response: 29231240
Conc: 2.07 ng/ml m

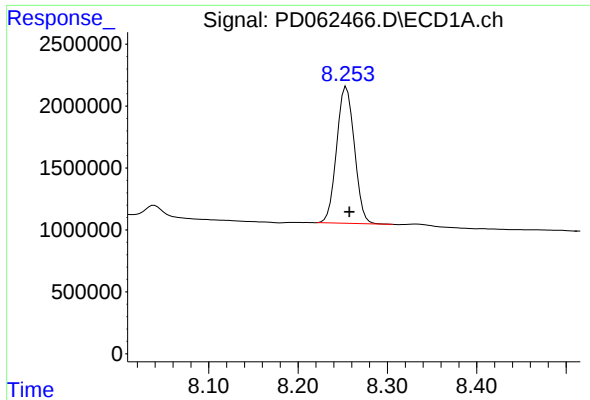


#28 Decachlorobiphenyl

R.T.: 8.254 min
Delta R.T.: -0.003 min
Response: 15214911
Conc: 12.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
STOCKPILE-COMP-3

Manual Integrations
APPROVED

Ankita
4/27/2021 2:04:59 PM

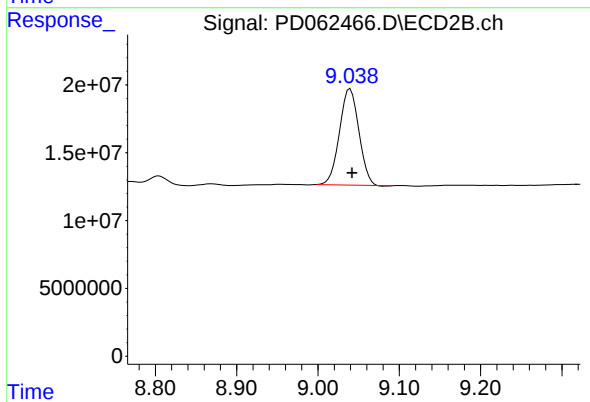

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: -0.002 min
Response: 117548581
Conc: 13.85 ng/ml