

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
 Data File : PD062467.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2021 04:03
 Operator : AR\AJ
 Sample : M2176-18
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 STOCKPILE-COMP-4

Manual Integrations
 APPROVED

Ankita
 4/27/2021 2:05:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 05:47:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.979	10557337	131.7E6	12.962	12.506m
28)	SA Decachlor...	8.256	9.040	15175469	113.6E6	12.510	13.389
Target Compounds							
12)	B 4,4'-DDE	5.652	6.311	1429277	25095417	1.177m	1.777m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042621\
Data File : PD062467.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2021 04:03
Operator : AR\AJ
Sample : M2176-18
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
STOCKPILE-COMP-4


Manual Integrations
APPROVED

Ankita
4/27/2021 2:05:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 05:47:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

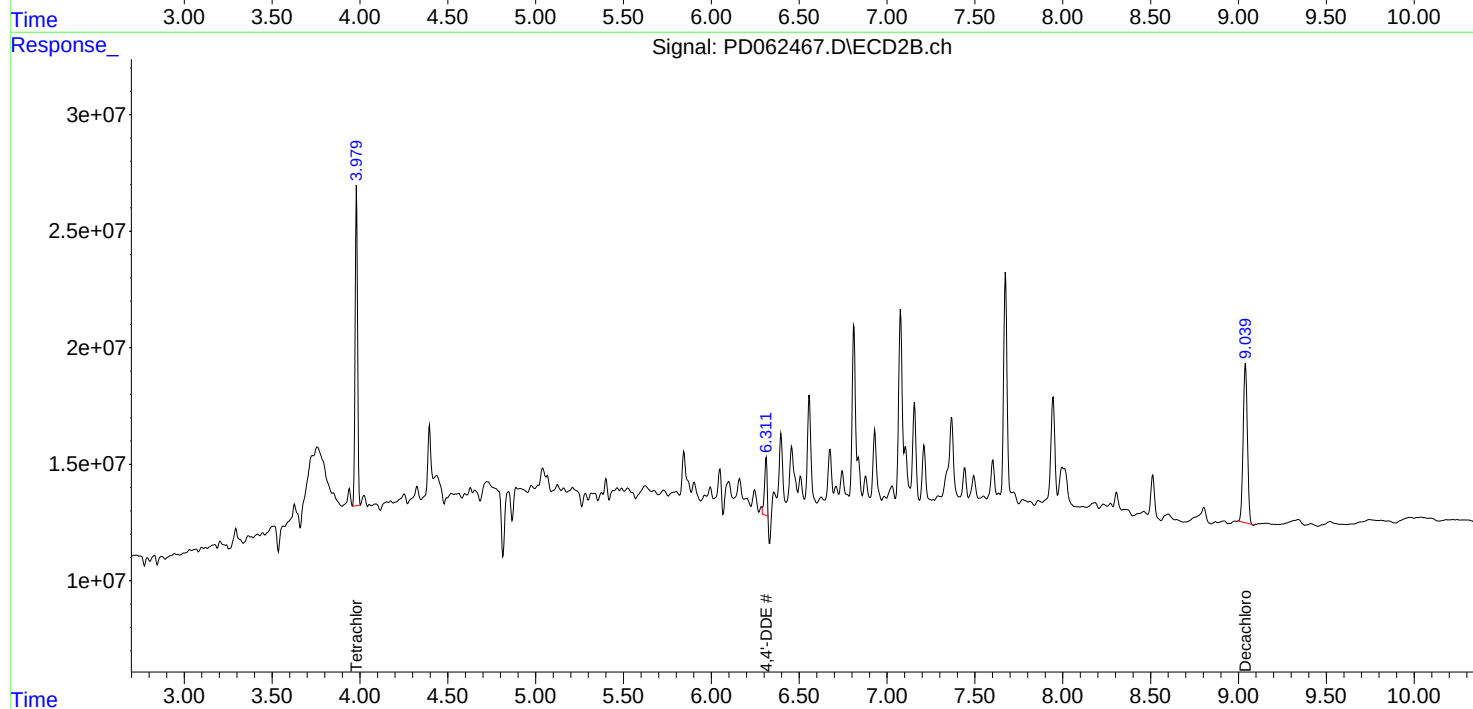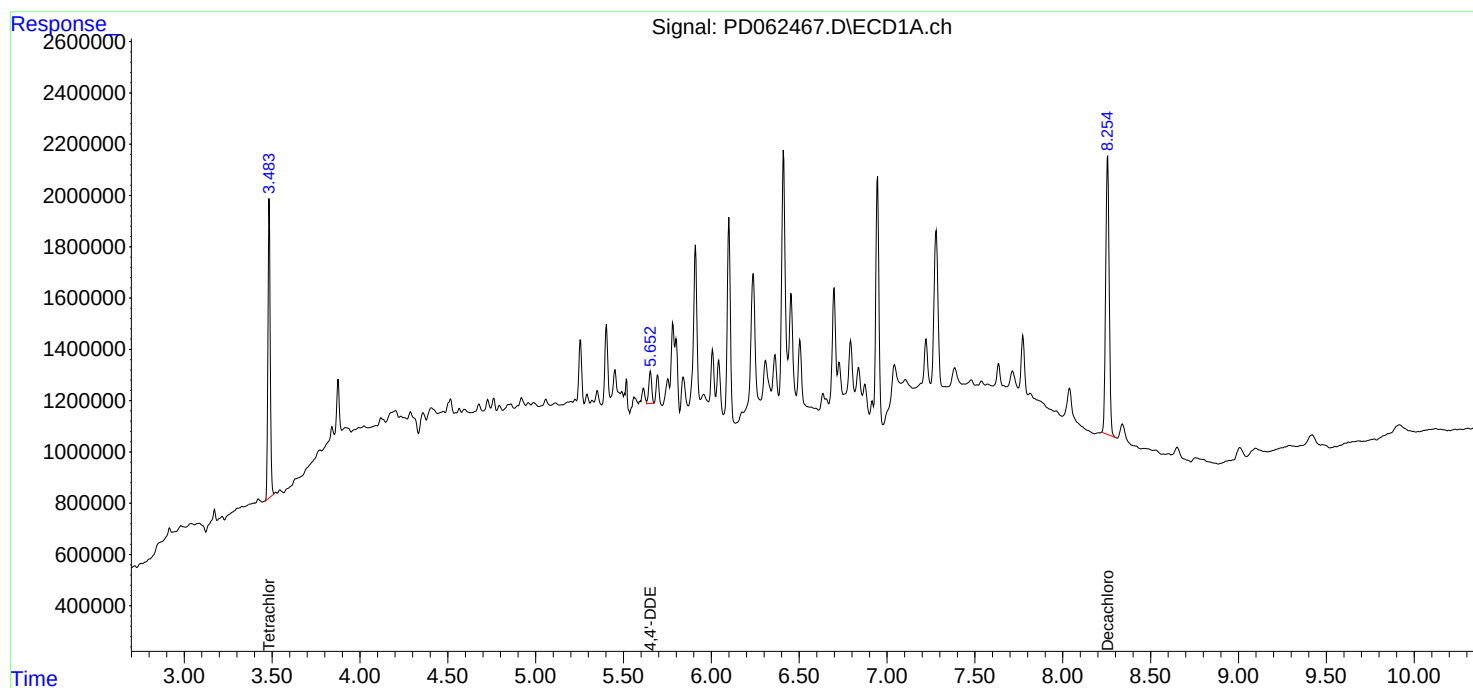

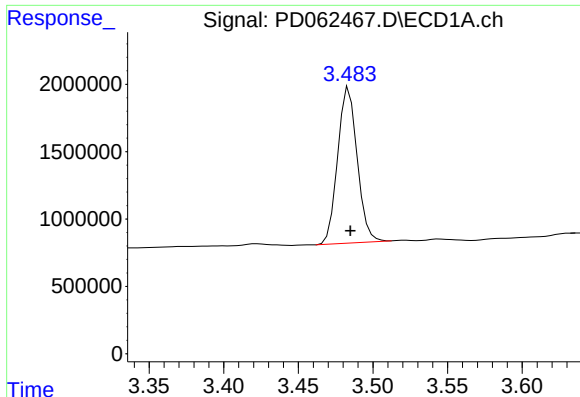


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 10557337
Conc: 12.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
STOCKPILE-COMP-4


Manual Integrations
APPROVED

Ankita
4/27/2021 2:05:01 PM

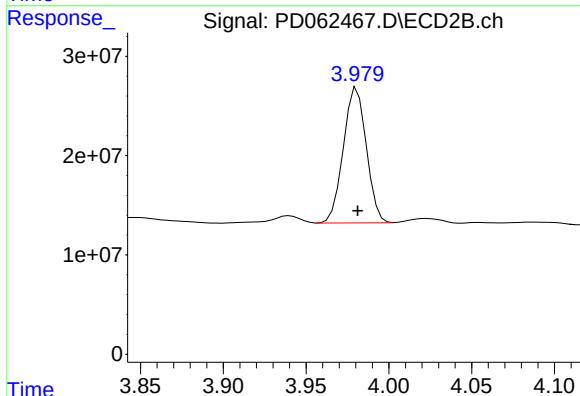


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.002 min
Response: 131702501
Conc: 12.51 ng/ml m

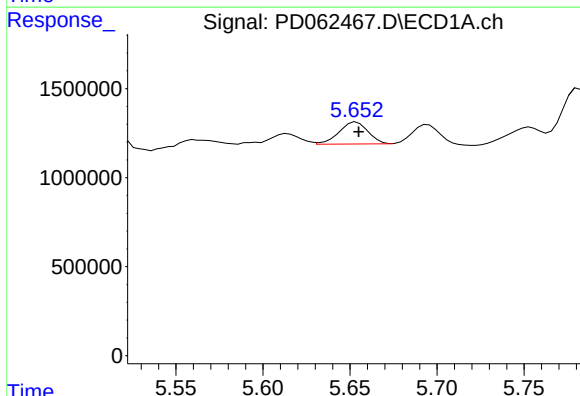


#12 4,4'-DDE

R.T.: 5.652 min
Delta R.T.: -0.003 min
Response: 1429277
Conc: 1.18 ng/ml m

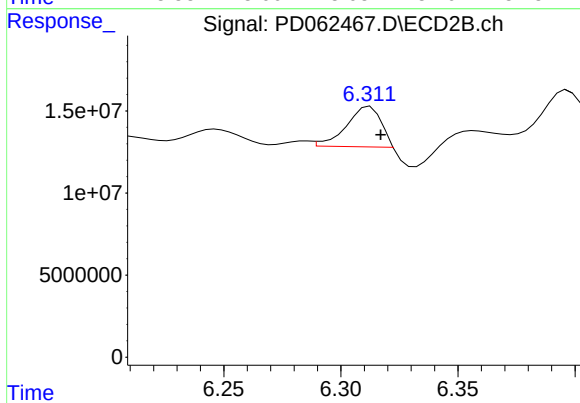

#12 4,4'-DDE

R.T.: 6.311 min
Delta R.T.: -0.006 min
Response: 25095417
Conc: 1.78 ng/ml m

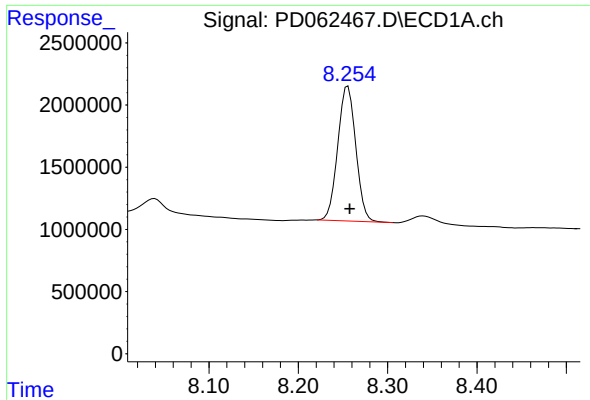


#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.002 min
Response: 15175469
Conc: 12.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
STOCKPILE-COMP-4

Manual Integrations
APPROVED

Ankita
4/27/2021 2:05:01 PM

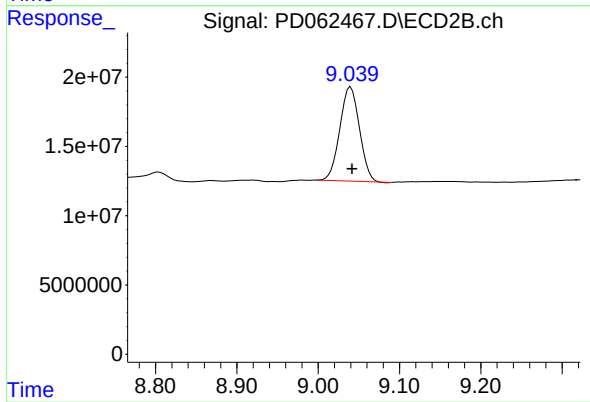

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: -0.002 min
Response: 113606944
Conc: 13.39 ng/ml