

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042622\
 Data File : PD069248.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2022 18:35
 Operator : AR\AJ
 Sample : N2470-03MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFFG0MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/27/2022
 Supervised By :mohammad ahmed 04/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 21:59:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.171	14752001	149.5E6	11.644	12.390
27)	SA Decachlor...	8.198	9.364	23706807	110.4E6	17.828	15.704m
Target Compounds							
2)	A alpha-BHC	3.884	4.568	90965002	648.6E6	50.890	39.452
3)	MA gamma-BHC...	4.167	4.859	97051691	645.9E6	53.655	41.458
4)	MA Heptachlor	4.465	5.386	87467256	602.3E6	51.517	39.787
5)	MB Aldrin	4.712	5.699	88501874	581.7E6	55.557	40.748 #
6)	B beta-BHC	4.417	5.021	40883549	159.2E6	52.782	23.739 #
7)	B delta-BHC	4.621	5.248	42460509	232.7E6	26.601	19.821 #
8)	B Heptachlo...	5.156	6.087	77426081	493.0E6	52.597	44.253
9)	A Endosulfan I	5.495	6.450	53670792	533.4E6	36.779	44.907
10)	B trans-Chl...	5.382	6.322	101.0E6	606.7E6	67.361	47.820m#
11)	B cis-Chlor...	5.441	6.399	88454672	593.5E6	59.260	47.653
12)	B 4,4'-DDE	5.606	6.548	156.9E6	874.5E6	117.011	80.379 #
13)	MA Dieldrin	5.738	6.708	184.8E6	986.1E6	118.756	81.758 #
14)	MA Endrin	5.996	6.929	145.3E6	765.3E6	103.828	78.692
15)	B Endosulfa...	6.270	7.134	146.0E6	839.0E6	113.334	87.541
16)	A 4,4'-DDD	6.123	7.040	118.4E6	782.4E6	97.138	83.553
17)	MA 4,4'-DDT	6.363	7.343	130.5E6	839.5E6	106.380	93.254
18)	B Endrin al...	6.440	7.258	87088555	577.6E6	87.736	80.837
19)	B Endosulfa...	6.652	7.483	115.2E6	616.3E6	91.924	70.238
20)	A Methoxychlor	6.914	7.796	333.2E6	1718.4E6	490.948	416.988
21)	B Endrin ke...	7.144	7.958	139.7E6	743.9E6	96.718	80.575

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042622\
Data File : PD069248.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2022 18:35
Operator : AR\AJ
Sample : N2470-03MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 21:59:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

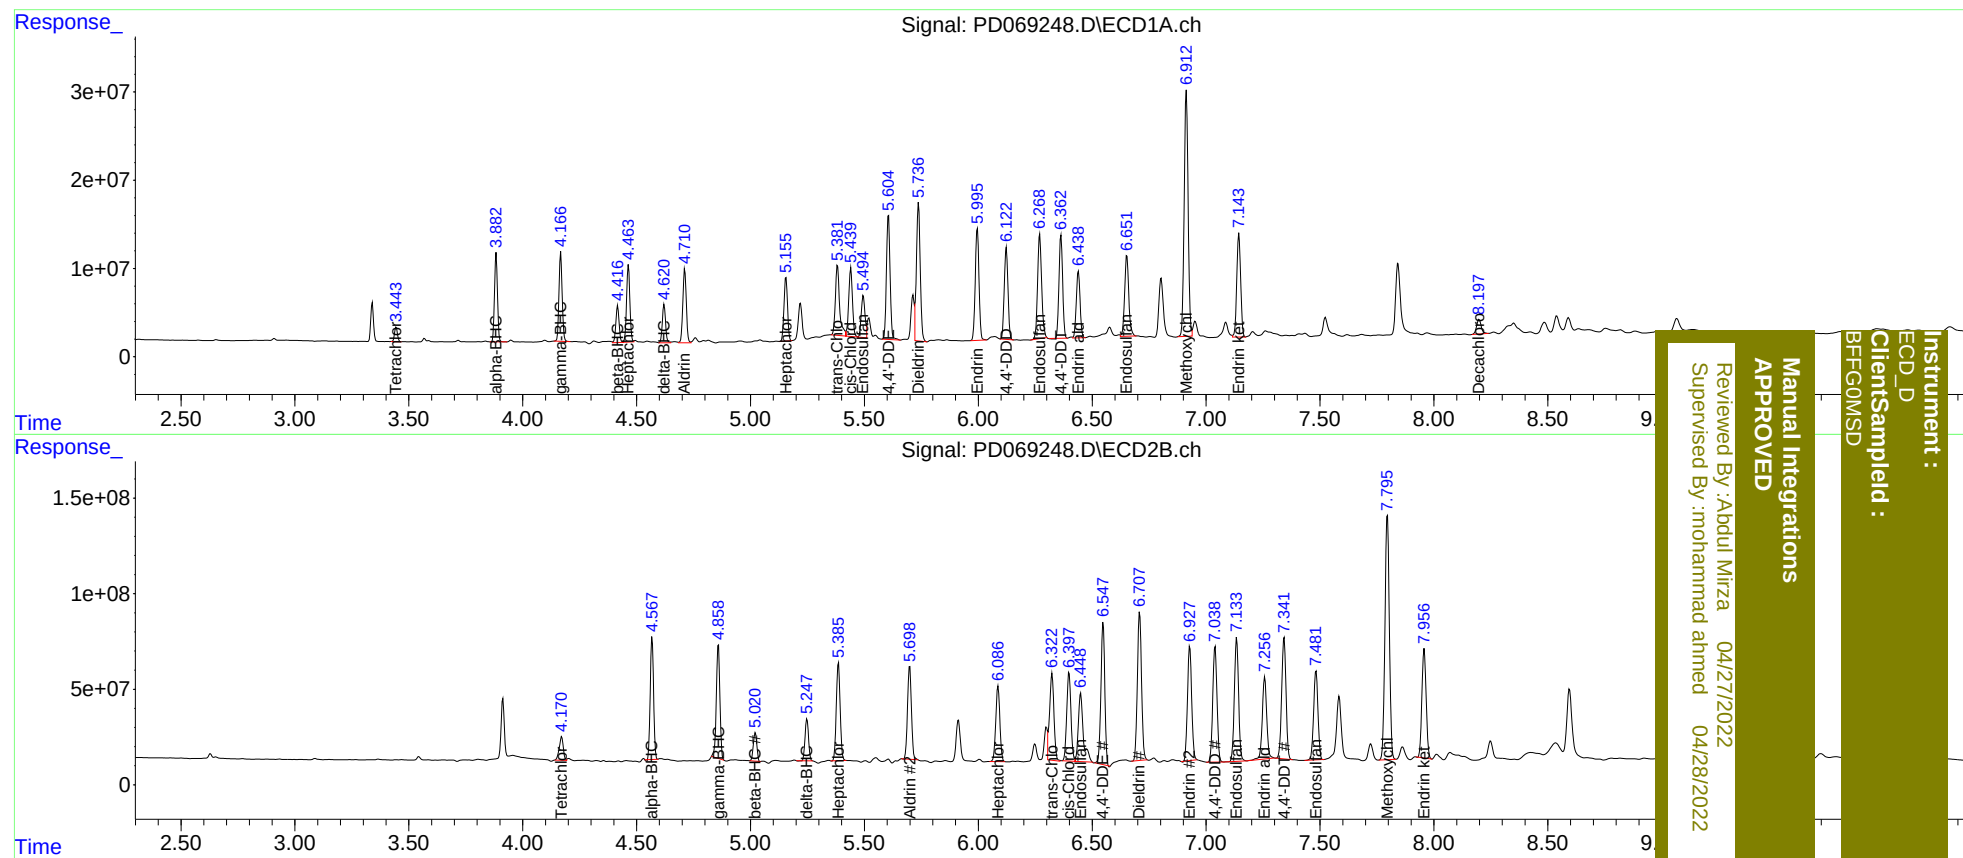

Reviewed By: Abdul Mirza 04/27/2022
Supervised By: mohammad ahmed 04/28/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
BFG0MSD