

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042623\
 Data File : PD074924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2023 11:00
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 01:23:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 14 02:10:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.587f	2.810f	429819	142497	0.168	0.101 #
27)	SA Decachlor...	9.033f	7.978f	1784643	204994	0.582	0.152 #
Target Compounds							
4)	MA Heptachlor	4.953	3.907f	74473	556531	<MDL	0.293 #
5)	MB Aldrin	0.000	4.202	0	356039	N.D.	0.188
6)	B beta-BHC	4.509f	3.907	261008	556531	0.149	0.628 #
7)	B delta-BHC	4.769	4.148	2522094	190185	0.684	<MDL #
8)	B Heptachlo...	5.700	0.000	6788291	0	1.855	N.D. #
9)	A Endosulfan I	6.097	0.000	141810	0	<MDL	N.D. #
10)	B trans-Chl...	5.900f	4.957	834436	117448	0.237	<MDL #
11)	B cis-Chlor...	6.097f	5.012	141810	95765	<MDL	<MDL #
12)	B 4,4'-DDE	6.273f	0.000	1497099	0	0.433	N.D. #
13)	MA Dieldrin	0.000	5.335	0	4475430	N.D.	2.519
14)	MA Endrin	6.627	5.660	7661669	3498842	2.379	2.229
15)	B Endosulfa...	6.793	5.963	1283425	686221	0.400	0.454
16)	A 4,4'-DDD	6.739	0.000	61205	0	<MDL	N.D. #
17)	MA 4,4'-DDT	7.080	0.000	930067	0	0.306	N.D. #
18)	B Endrin al...	6.908f	0.000	1140539	0	0.436	N.D. #
21)	B Endrin ke...	7.699	0.000	1307615	0	0.367	N.D. #
22)	Toxaphene-1	6.273	5.335	1497099	4475430	53.860	454.407 #
23)	Toxaphene-2	6.498	5.660	1233957	3498842	35.713	319.265 #
24)	Toxaphene-3	6.627	5.963	7661669	686221	330.662	56.627 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042623\
Data File : PD074924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2023 11:00
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 01:23:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 14 02:10:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

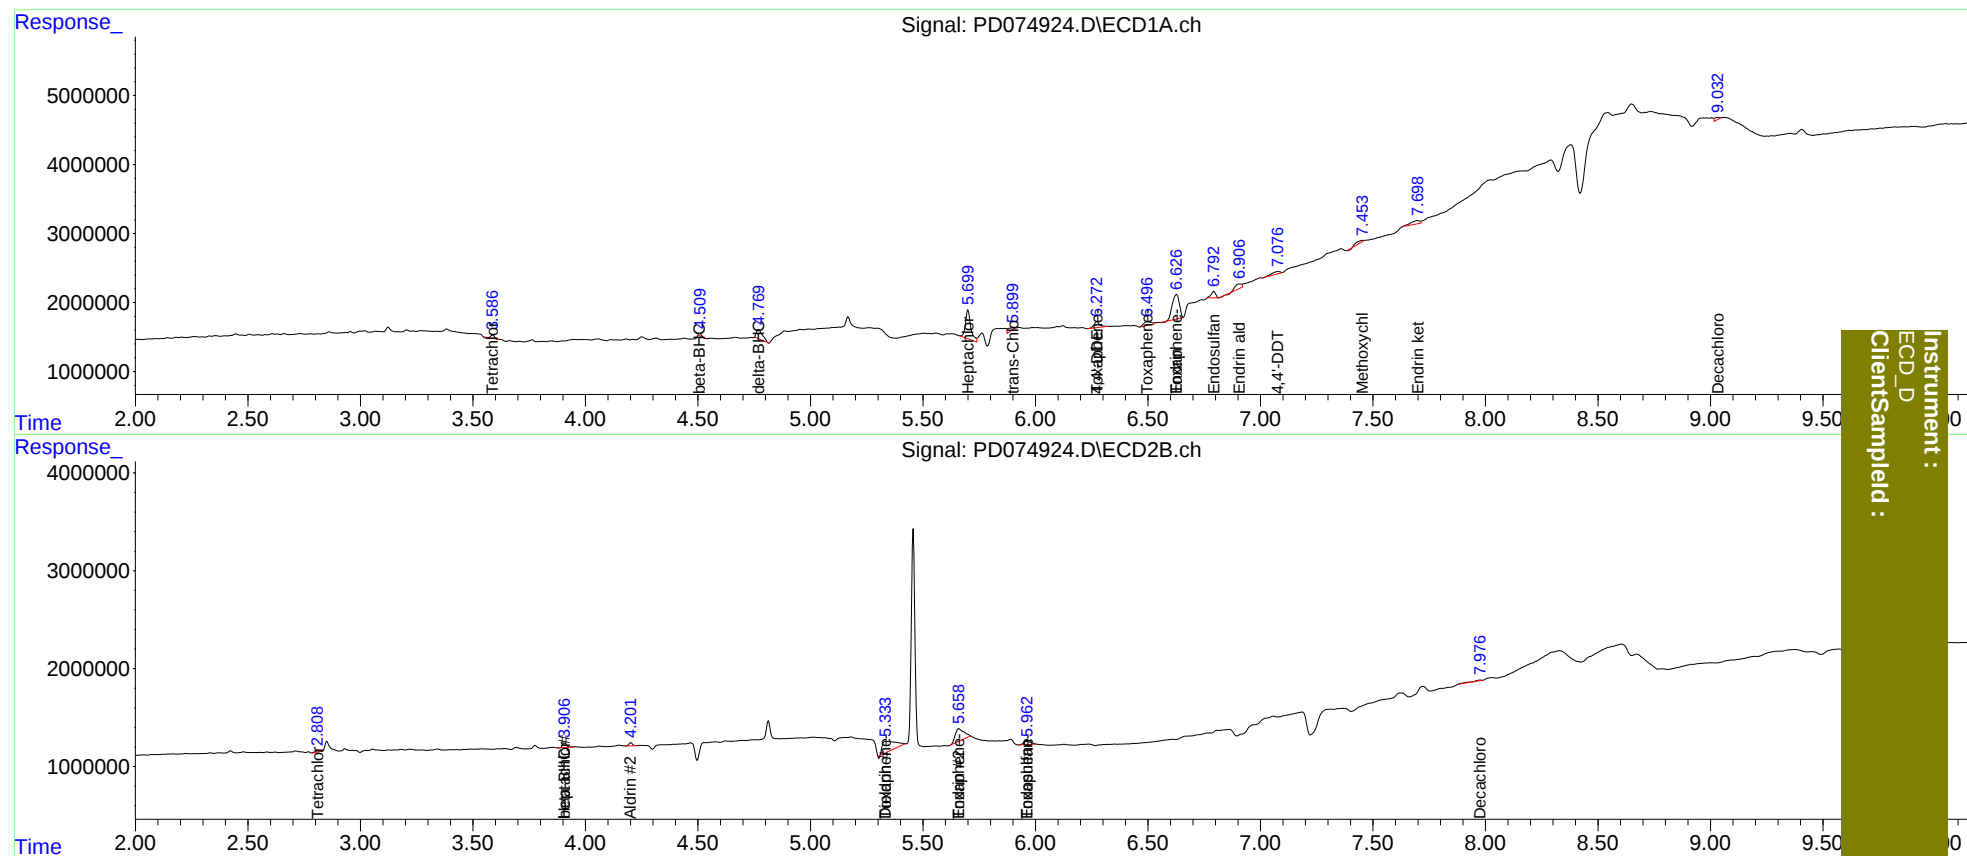

Instrument :
ECD_D
ClientSampled :