

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042623\
 Data File : PD074937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2023 16:14
 Operator : AR\AJ
 Sample : 02418-21MSDRE
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW8Z5MSDRE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/27/2023
 Supervised By : Ankita Jodhani 05/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 01:27:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 14 02:10:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.770	29208727	11112378	11.441	7.899 #
27)	SA Decachlor...	9.074	7.918	70748517	24379112	23.080	18.063
Target Compounds							
2)	A alpha-BHC	4.003	3.273	180.6E6	68329484	43.551	34.064
3)	MA gamma-BHC...	4.335	3.603	154.1E6	84619483	39.181m	43.661m
4)	MA Heptachlor	4.928	3.944	170.1E6	66735824	41.643	35.130
5)	MB Aldrin	5.272	4.225	170.8E6	67094668	43.397	35.460
6)	B beta-BHC	4.532	3.899	55946374	28884070	31.923	32.585
7)	B delta-BHC	4.780	4.129	115.1E6	55262359	31.203	28.263
8)	B Heptachlo...	5.698	4.727	147.9E6	52745328	40.419	30.316
9)	A Endosulfan I	6.085	5.099	126.4E6	36089389	37.332	23.159 #
10)	B trans-Chl...	5.953	4.978	170.2E6	75277577	48.273m	44.087
11)	B cis-Chlor...	6.035	5.042	186.6E6	62123721	50.803	35.941 #
12)	B 4,4'-DDE	6.205	5.231	263.6E6	118.4E6	76.321m	72.521
13)	MA Dieldrin	6.361	5.363	384.6E6	157.9E6	102.899	88.914
14)	MA Endrin	6.591	5.638	294.0E6	115.1E6	91.267	73.349
15)	B Endosulfa...	6.810	5.932	265.0E6	112.2E6	82.615	74.251
16)	A 4,4'-DDD	6.724	5.786	268.5E6	91867301	94.281	66.422 #
17)	MA 4,4'-DDT	7.038	6.037	314.0E6	104.6E6	103.179m	72.755 #
18)	B Endrin al...	6.940	6.110	197.4E6	72847295	75.461	59.185m
19)	B Endosulfa...	7.175	6.332	264.9E6	86136447	86.465	60.895m#
20)	A Methoxychlor	7.515	6.614	739.4E6	254.8E6	434.838	346.504
21)	B Endrin ke...	7.662	6.840	256.0E6	88700076	71.909	52.651 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042623\
Data File : PD074937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2023 16:14
Operator : AR\AJ
Sample : 02418-21MSDRE
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 01:27:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 14 02:10:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

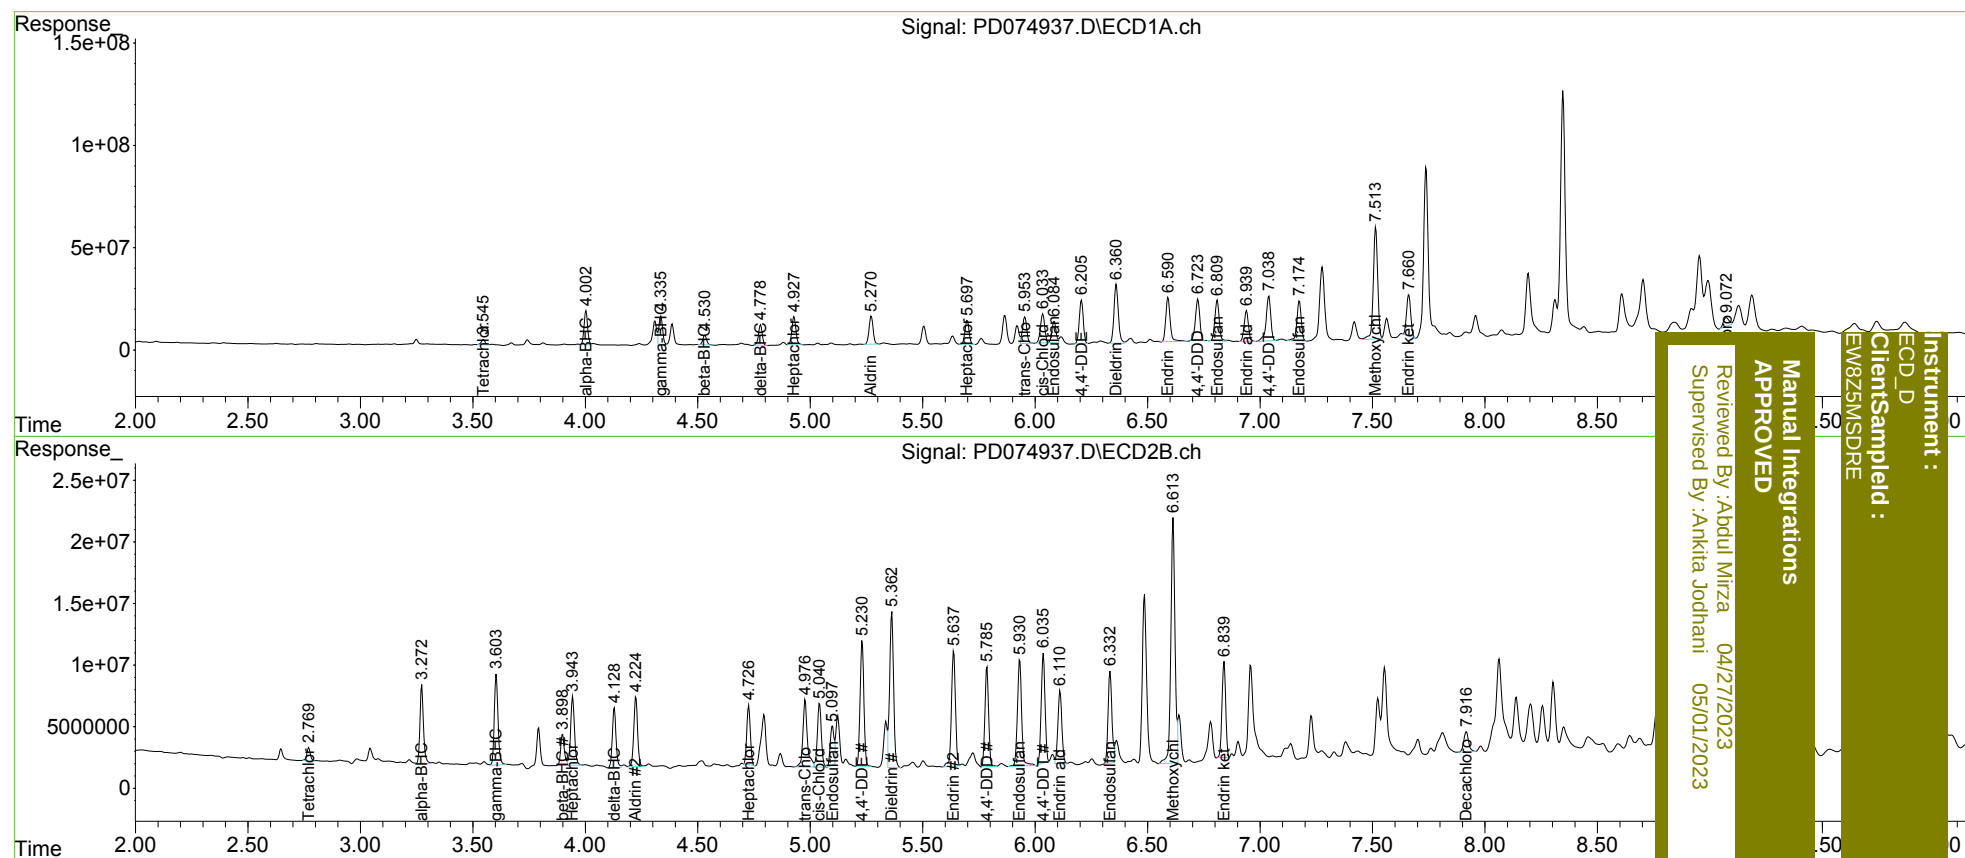

Instrument :
ECD_D
Client Sampled :
EWZ5MSDRE
Manual Integrations
APPROVED
Reviewed By : Abdul Mirza 04/27/2023
Supervised By : Ankita Jodhani 05/01/2023