

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042623\
 Data File : PD074956.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2023 00:48
 Operator : AR\AJ
 Sample : 02374-03MS
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB9D6MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/27/2023
 Supervised By : Ankita Jodhani 05/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 01:33:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 14 02:10:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.771	35018455	13144737	13.716	9.344 #
2)	SA Decachlor...	9.087	7.919	48454717	20041245	15.807	14.849
Target Compounds							
2)	A alpha-BHC	4.003	3.274	163.8E6	62311766	39.503m	31.064
3)	MA gamma-BHC...	4.337	3.604	144.9E6	65619536	36.847m	33.857
4)	MA Heptachlor	4.930	3.945	147.6E6	57739557	36.147	30.394
5)	MB Aldrin	5.273	4.225	149.8E6	62926472	38.053	33.257
6)	B beta-BHC	4.534	3.899	55710990	25595219	31.788	28.875
7)	B delta-BHC	4.782	4.130	114.0E6	47401571	30.896	24.243
8)	B Heptachlo...	5.700	4.727	133.6E6	50057207	36.510	28.771
9)	A Endosulfan I	6.087	5.099	111.2E6	37276903	32.865	23.921 #
10)	B trans-Chl...	5.955	4.978	139.4E6	58796660	39.540m	34.435
11)	B cis-Chlor...	6.036	5.043	138.6E6	54616436	37.734	31.598
12)	B 4,4'-DDE	6.208	5.232	225.9E6	99576224	65.413	60.986
13)	MA Dieldrin	6.363	5.364	280.8E6	118.3E6	75.127	66.589
14)	MA Endrin	6.593	5.640	236.8E6	99010441	73.508	63.078
15)	B Endosulfa...	6.812	5.933	230.2E6	95235026	71.757	63.007
16)	A 4,4'-DDD	6.726	5.787	213.9E6	73485091	75.101	53.132 #
17)	MA 4,4'-DDT	7.040	6.039	237.7E6	84083554	78.111m	58.474 #
18)	B Endrin al...	6.942	6.112	159.5E6	60588948	60.990	49.225
19)	B Endosulfa...	7.177	6.335	195.7E6	78066335	63.858	55.190
20)	A Methoxychlor	7.517	6.615	596.6E6	232.5E6	350.880	316.141
21)	B Endrin ke...	7.663	6.842	240.2E6	87605712	67.476	52.001

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042623\
Data File : PD074956.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2023 00:48
Operator : AR\AJ
Sample : 02374-03MS
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 01:33:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 14 02:10:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

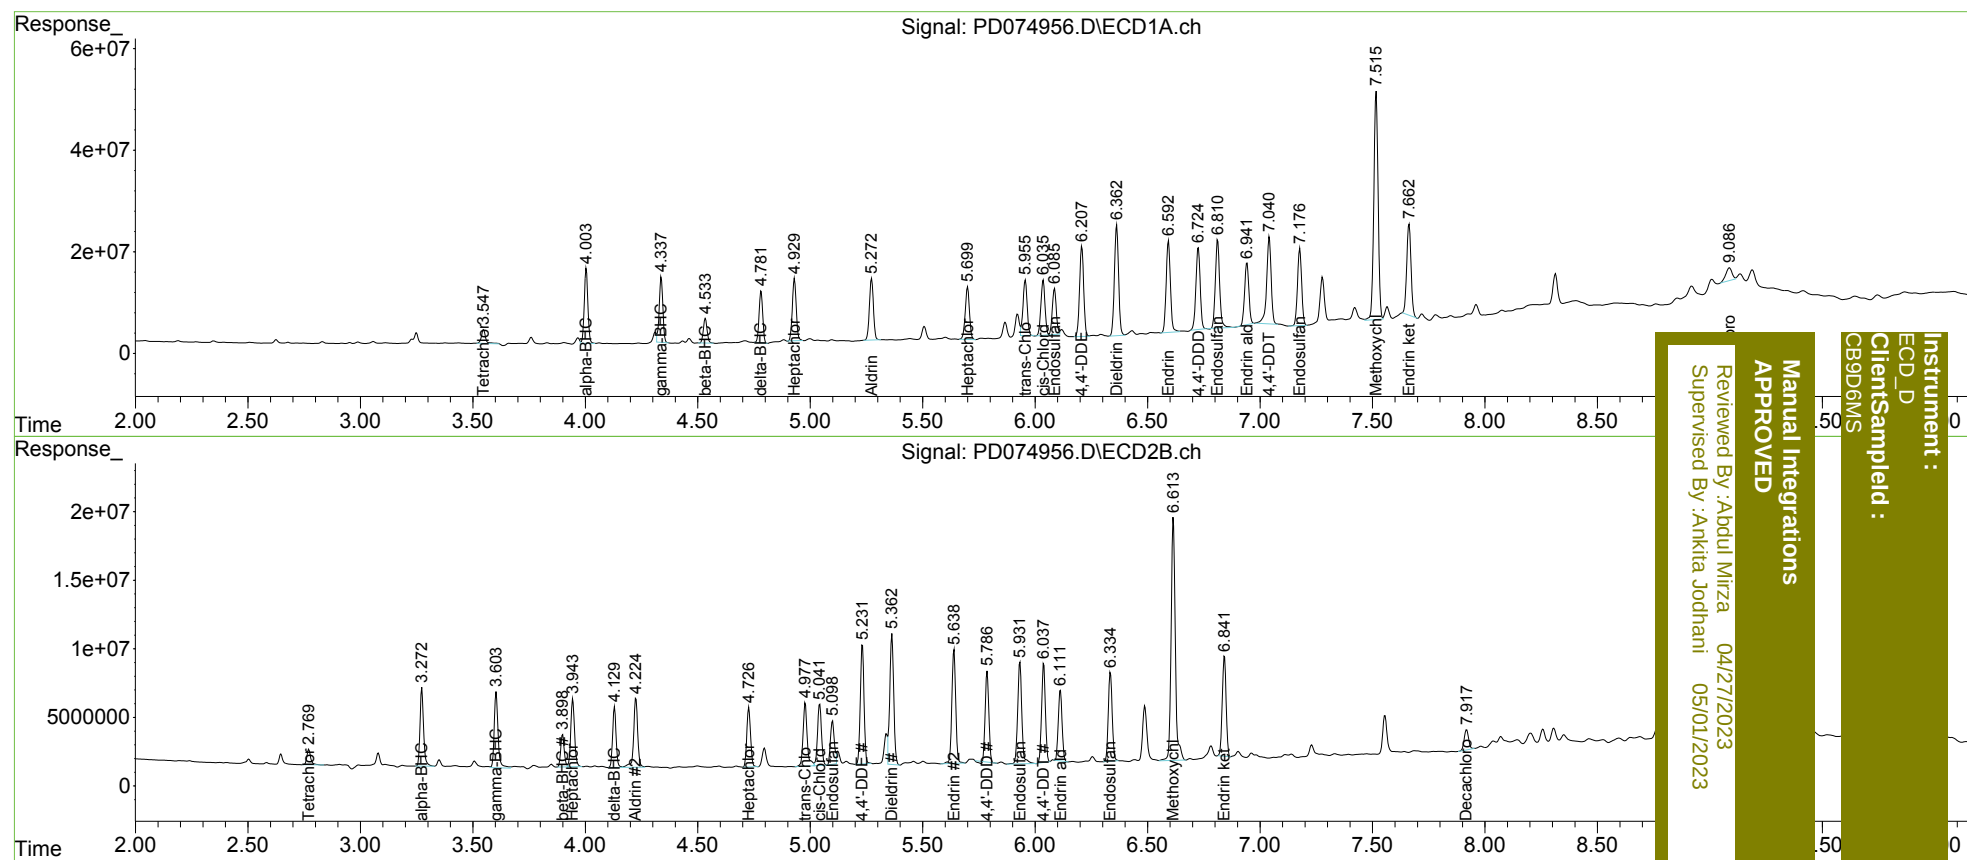

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 04/27/2023
Supervised By: Ankita Jodhani 05/01/2023

Instrument :
ECD_D
Client Sampled :
CB9D6MS