

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042623\
 Data File : PD074957.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2023 01:15
 Operator : AR\AJ
 Sample : 02374-04MSD
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB9D6MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/27/2023
 Supervised By : Ankita Jodhani 05/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 09:03:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 14 02:10:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.770	32760689	12515033	12.832	8.896 #
27)	SA Decachlor...	9.090	7.919	32094183	20327804	10.470	15.062 #
Target Compounds							
2)	A alpha-BHC	4.003	3.273	156.3E6	59532664	37.692m	29.679
3)	MA gamma-BHC...	4.336	3.602	140.9E6	59589592	35.828m	30.746m
4)	MA Heptachlor	4.929	3.945	146.0E6	56625452	35.758	29.808
5)	MB Aldrin	5.273	4.225	146.9E6	61974292	37.330	32.754
6)	B beta-BHC	4.533	3.899	54661112	25029732	31.189	28.237
7)	B delta-BHC	4.781	4.130	111.5E6	46648830	30.229	23.858
8)	B Heptachlo...	5.700	4.727	130.3E6	49675272	35.621	28.551
9)	A Endosulfan I	6.087	5.099	106.5E6	37118067	31.454	23.820
10)	B trans-Chl...	5.955	4.978	141.0E6	58465393	39.981m	34.241
11)	B cis-Chlor...	6.036	5.043	133.8E6	54409956	36.433	31.479
12)	B 4,4'-DDE	6.207	5.232	218.5E6	98930576	63.254m	60.591
13)	MA Dieldrin	6.363	5.363	273.2E6	117.7E6	73.093	66.267
14)	MA Endrin	6.593	5.639	230.4E6	98593477	71.531	62.812
15)	B Endosulfa...	6.811	5.933	228.6E6	94633525	71.282	62.609
16)	A 4,4'-DDD	6.726	5.785	209.3E6	76720665	73.488	55.471m
17)	MA 4,4'-DDT	7.040	6.038	221.1E6	83252288	72.664m	57.896
18)	B Endrin al...	6.942	6.112	158.4E6	60006844	60.570	48.752
19)	B Endosulfa...	7.177	6.335	193.9E6	77543616	63.277	54.821
20)	A Methoxychlor	7.517	6.614	583.8E6	230.3E6	343.358	313.283
21)	B Endrin ke...	7.663	6.842	234.6E6	87343579	65.893	51.846

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042623\
Data File : PD074957.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2023 01:15
Operator : AR\AJ
Sample : 02374-04MSD
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 09:03:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 14 02:10:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

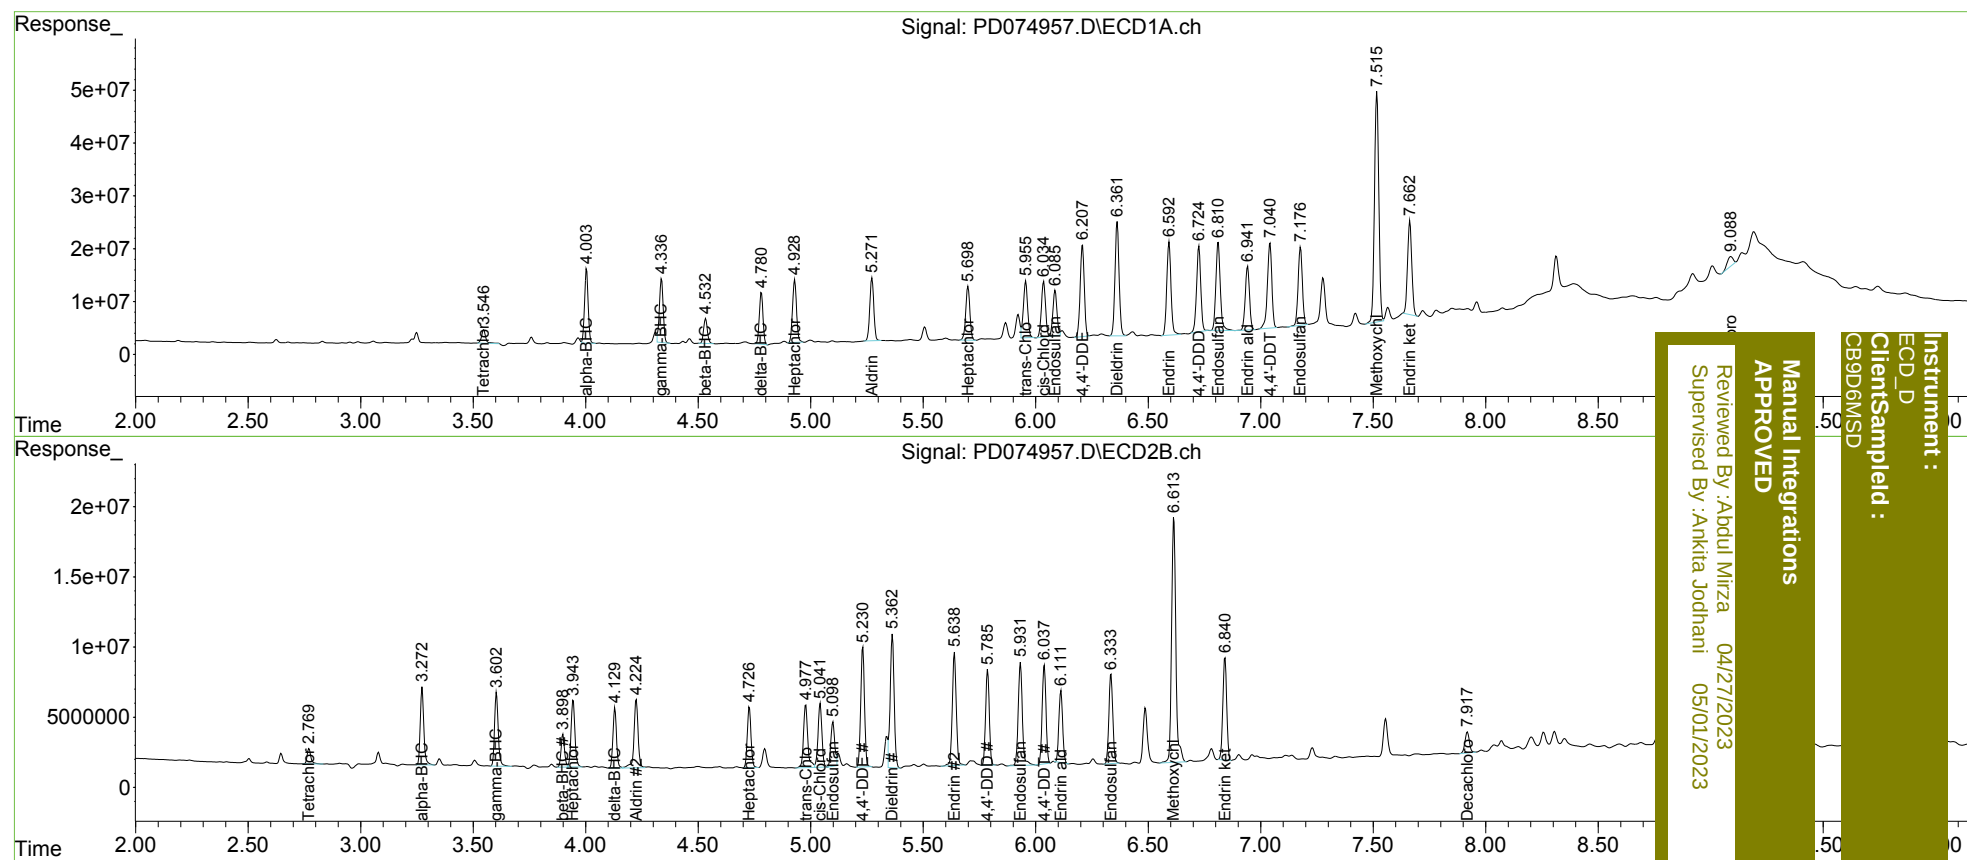

Instrument :
ECD_D
ClientSampled :
CB9D6MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Miza 04/27/2023
Supervised By :Ankita Jodhani 05/01/2023