

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042624\
 Data File : PD082619.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2024 19:01
 Operator : AR\AJ
 Sample : P2204-06MSD 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1CX4MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/30/2024
 Supervised By :mohammad ahmed 05/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 21:31:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041124CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 06:17:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.776	38486144	82738433	25.103	23.841
27)	SA Decachlor...	9.118	7.905	48655464	94909826	25.152	28.854
Target Compounds							
2)	A alpha-BHC	4.022	3.276	137.4E6	303.0E6	51.812	55.268
3)	MA gamma-BHC...	4.356	3.604	136.8E6	293.8E6	53.716	58.691
4)	MA Heptachlor	4.949	3.944	136.3E6	290.4E6	51.280	60.109
5)	MB Aldrin	5.292	4.223	123.6E6	279.3E6	50.048	60.162
6)	B beta-BHC	4.551	3.900	55089487	122.5E6	50.956	57.784
7)	B delta-BHC	4.800	4.130	70671225	160.1E6	27.469	31.668
8)	B Heptachlo...	5.719	4.724	123.6E6	272.4E6	54.525	62.646
9)	A Endosulfan I	6.105	5.093	115.7E6	247.0E6	54.615m	64.229
10)	B trans-Chl...	5.976	4.973	121.3E6	272.3E6	56.386	65.976
11)	B cis-Chlor...	6.054	5.037	125.7E6	276.4E6	57.120m	66.741
12)	B 4,4'-DDE	6.226	5.226	244.5E6	527.2E6	113.955	132.771
13)	MA Dieldrin	6.382	5.357	255.1E6	558.9E6	112.503	128.669
14)	MA Endrin	6.613	5.632	213.6E6	488.2E6	115.639	131.288
15)	B Endosulfa...	6.832	5.926	207.2E6	451.0E6	109.247	126.199
16)	A 4,4'-DDD	6.746	5.780	183.2E6	421.6E6	114.400	132.934
17)	MA 4,4'-DDT	7.061	6.030	195.2E6	441.3E6	117.868	130.267
18)	B Endrin al...	6.963	6.105	156.7E6	345.9E6	112.728	127.283
19)	B Endosulfa...	7.198	6.327	177.8E6	396.8E6	104.556	116.561
20)	A Methoxychlor	7.537	6.605	480.0E6	967.0E6	560.887	582.872
21)	B Endrin ke...	7.684	6.833	215.7E6	500.4E6	120.758	131.811

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042624\
Data File : PD082619.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2024 19:01
Operator : AR\AJ
Sample : P2204-06MSD 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 21:31:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041124CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 06:17:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

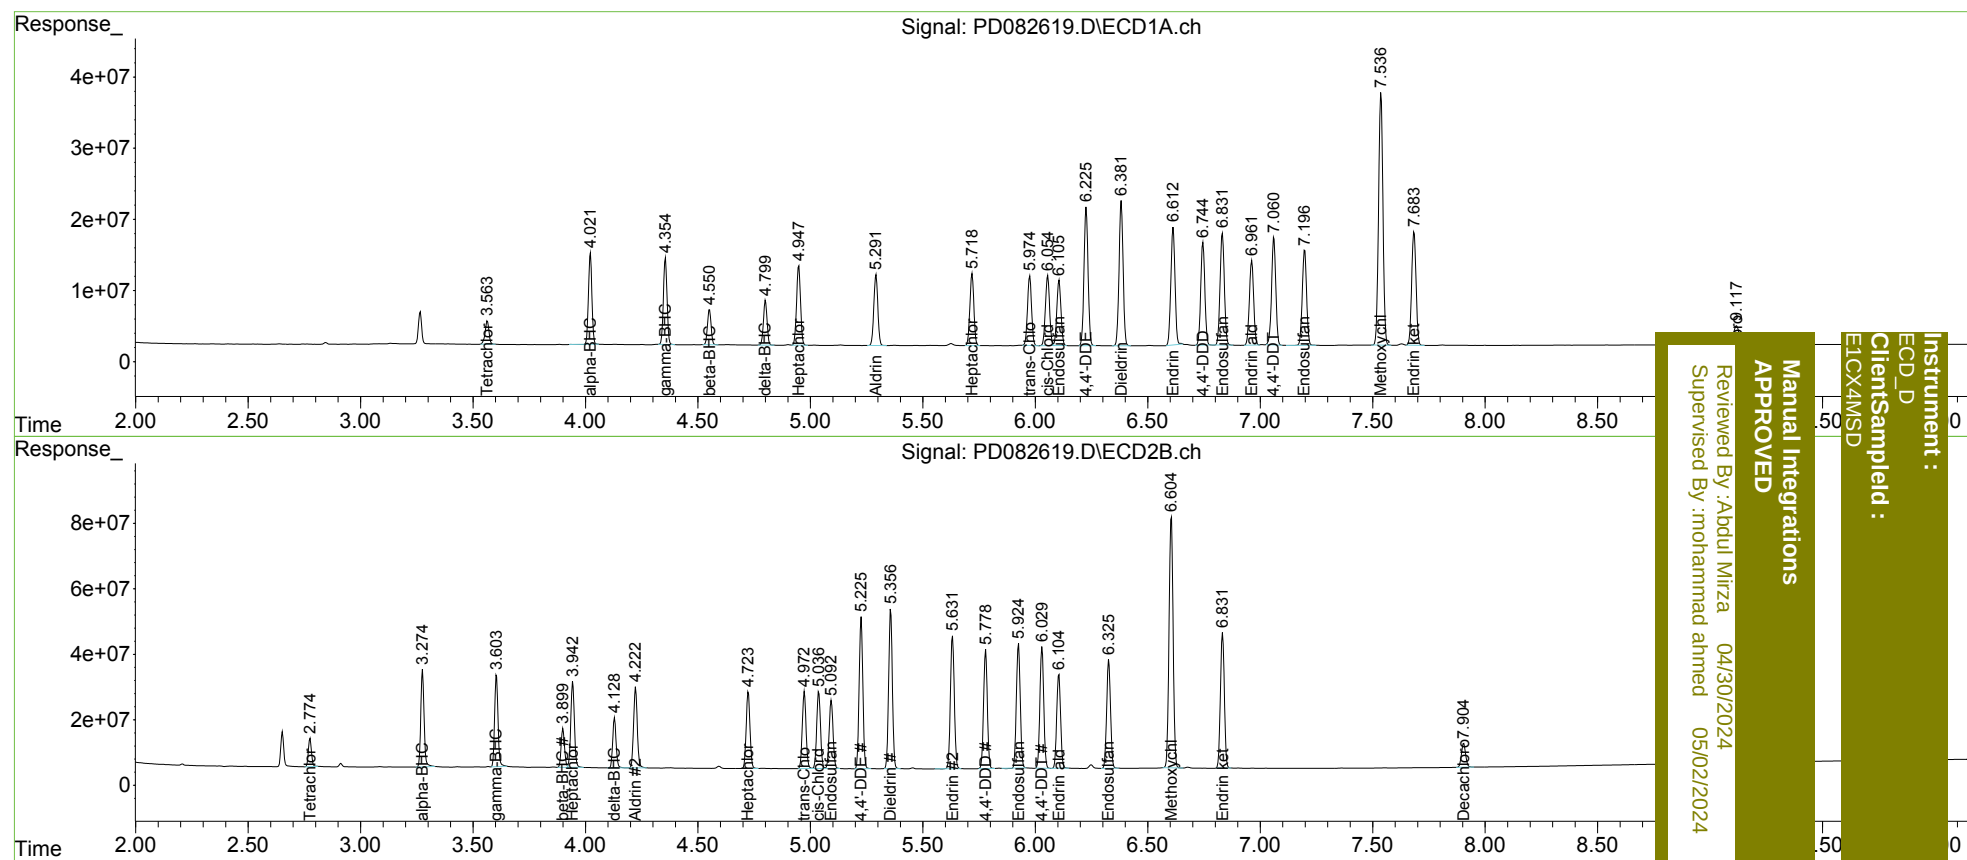

111
Reviewed By: Abdul Mirza 04/30/2024
Supervised By: mohammad ahmed 05/02/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
E10X4MSD