

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042723\
 Data File : PD074964.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2023 14:20
 Operator : AR\AJ
 Sample : TOXAPH101
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 15:55:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 27 15:55:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.770	12920613	5834778	5.332	5.070
27)	SA Decachlor...	9.090	7.920	28287770	11928967	10.358	10.953
Target Compounds							
22)	Toxaphene-1	6.254	5.002	11426928	3426372	520.220	512.609
23)	Toxaphene-2	6.458	5.687	13704917	3734909	510.033	531.376
24)	Toxaphene-3	6.656	5.969	9182016	4407772	495.675	528.443
25)	Toxaphene-4	7.168	6.603	28412914	11520963	482.722	483.958
26)	Toxaphene-5	7.591	6.729	21192303	16786317	467.869	567.257

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042723\
Data File : PD074964.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2023 14:20
Operator : AR\AJ
Sample : TOXAPH101
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 15:55:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 27 15:55:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

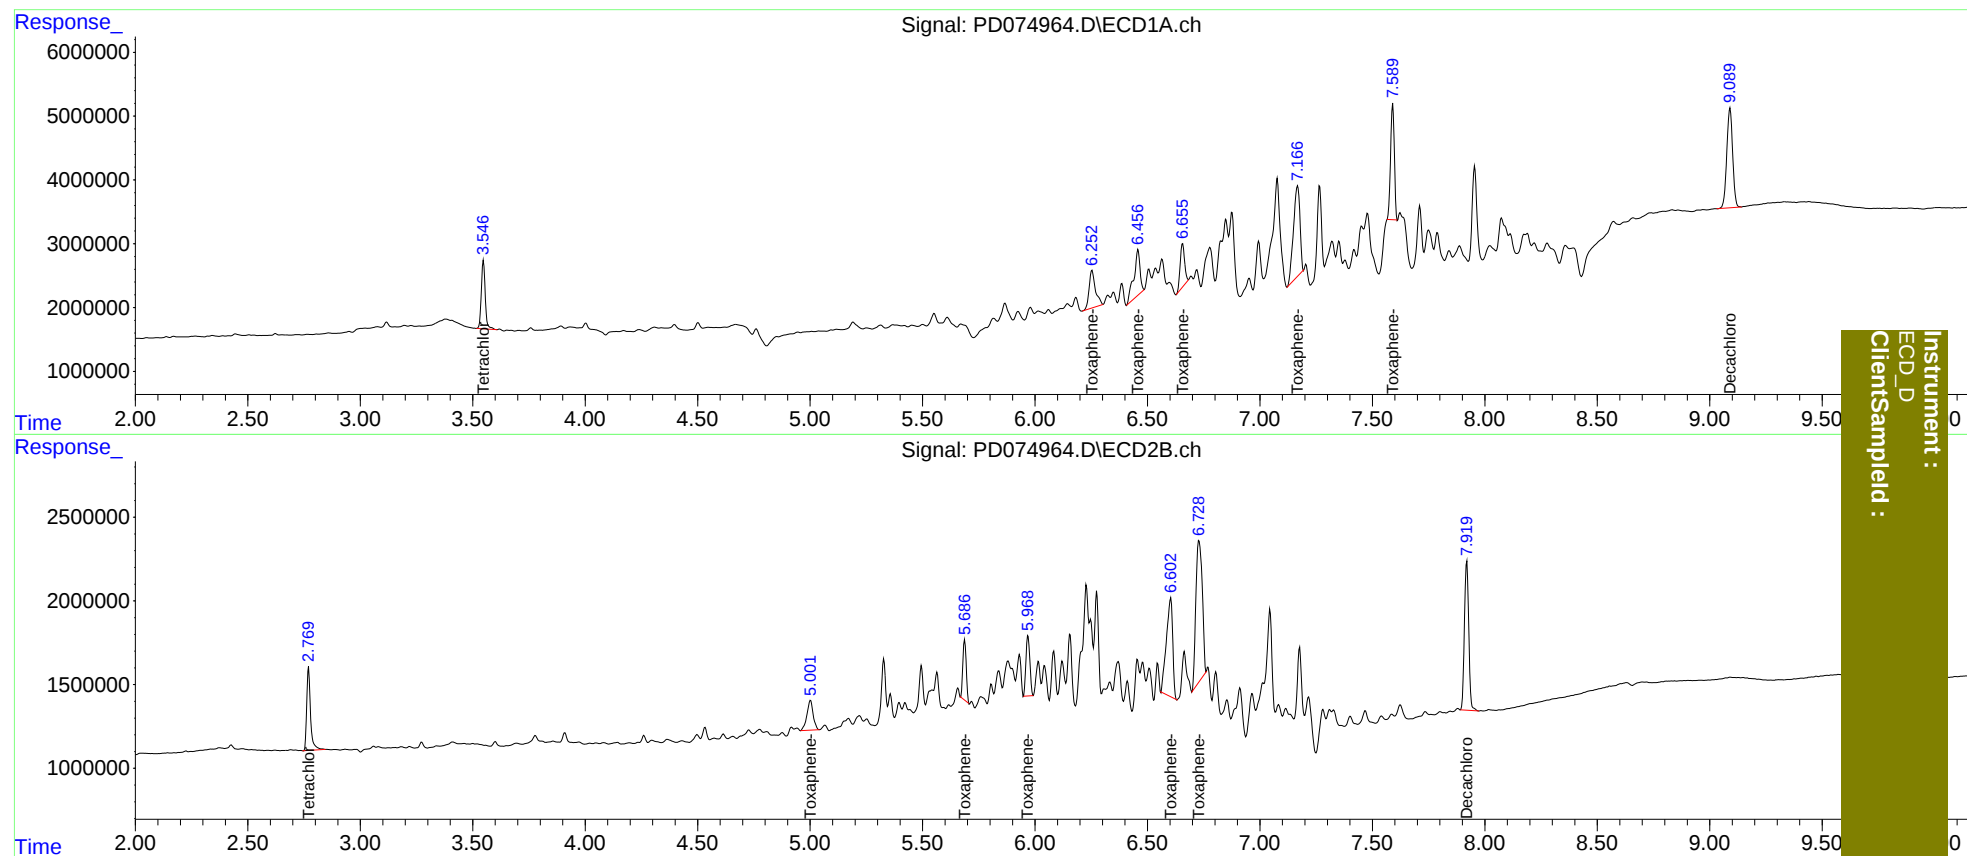

Instrument :
ECD_D
ClientSampled :
0