

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042723\
 Data File : PD074973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2023 16:21
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 01:56:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 01:55:57 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.770	44797012	21243094	20.000	20.000
27)	SA Decachlor...	9.088	7.918	95910748	38643101	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.004	3.273	73563541	29266350	20.000	20.000
3)	MA gamma-BHC...	4.337	3.603	68683186	28333865	20.000	20.000
4)	MA Heptachlor	4.929	3.945	69217220	28046289	20.000	20.000
9)	A Endosulfan I	6.086	5.097	58217291	23059084	20.000	20.000
13)	MA Dieldrin	6.361	5.363	127.9E6	50765306	40.000	40.000
14)	MA Endrin	6.591	5.638	109.0E6	44837147	40.000	40.000
16)	A 4,4'-DDD	6.725	5.786	97254741	39175838	40.000	40.000
17)	MA 4,4'-DDT	7.040	6.038	101.5E6	40505703	40.000	40.000
20)	A Methoxychlor	7.515	6.613	291.5E6	112.8E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042723\
Data File : PD074973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2023 16:21
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 01:56:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 01:55:57 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

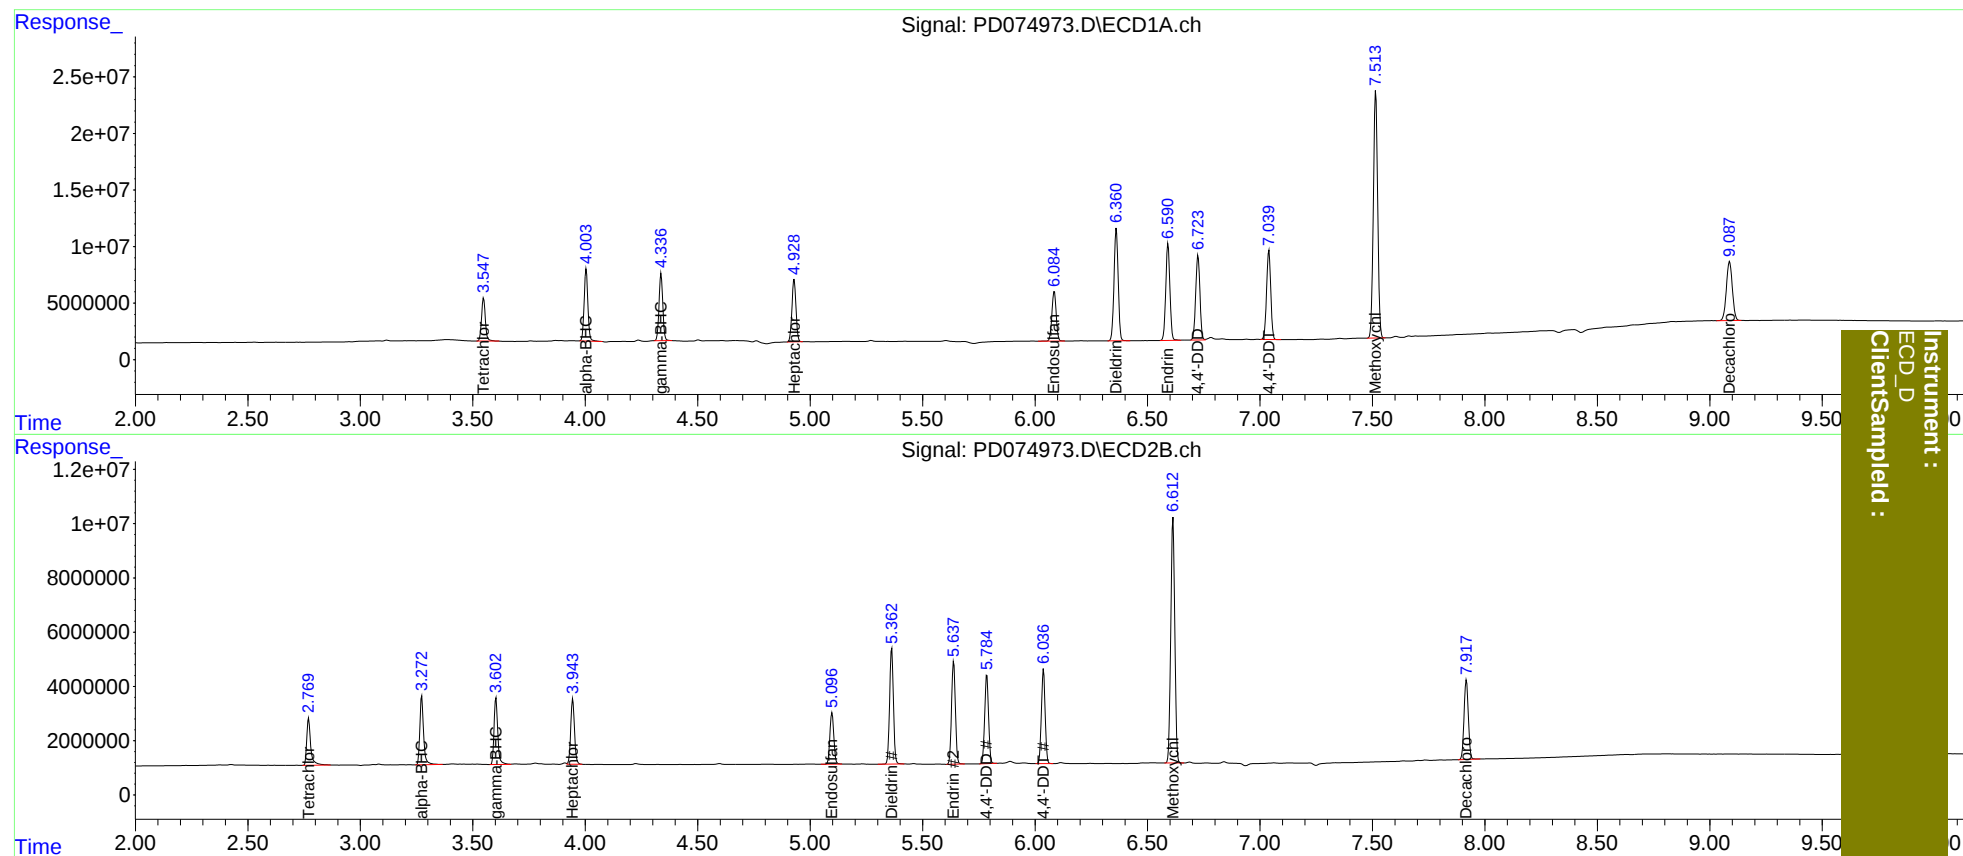


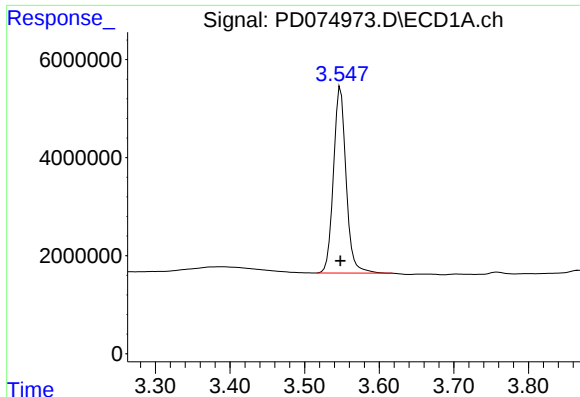

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 44797012
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

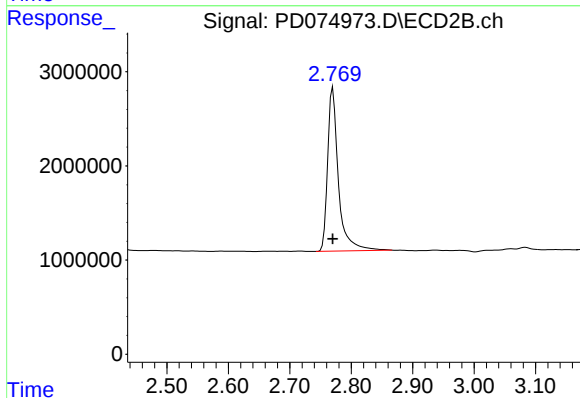


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: 0.000 min
Response: 21243094
Conc: 20.00 ng/ml

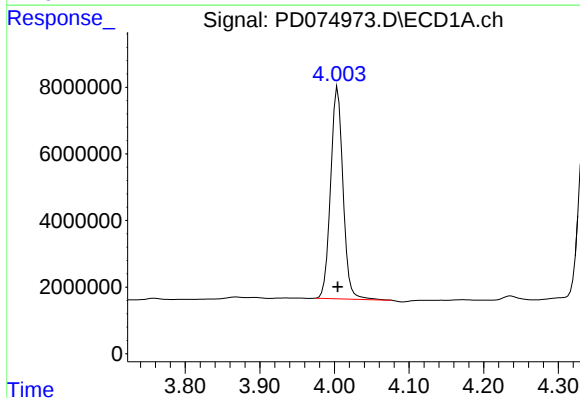


#2 alpha-BHC

R.T.: 4.004 min
Delta R.T.: 0.000 min
Response: 73563541
Conc: 20.00 ng/ml

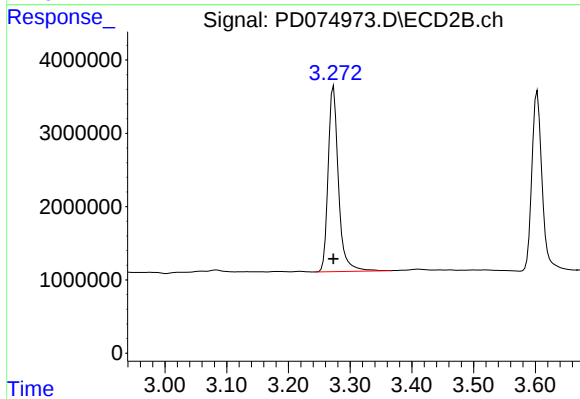

#2 alpha-BHC


R.T.: 3.273 min
Delta R.T.: 0.000 min
Response: 29266350
Conc: 20.00 ng/ml

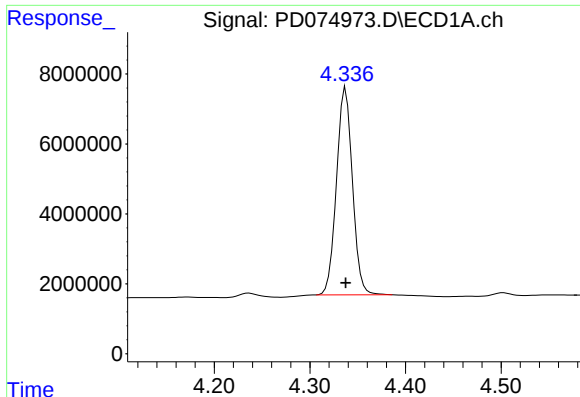

#3 gamma-BHC (Lindane)


R.T.: 4.337 min
Delta R.T.: 0.000 min
Response: 68683186
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

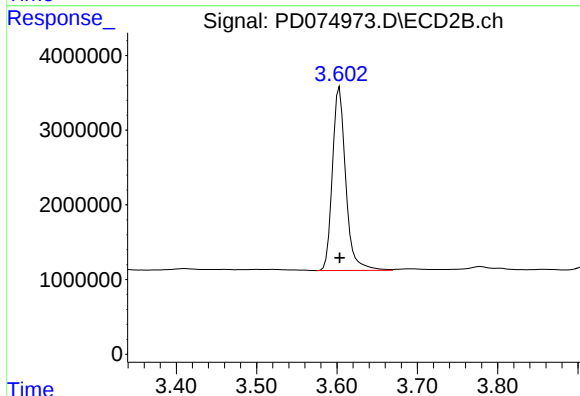


#3 gamma-BHC (Lindane)

R.T.: 3.603 min
Delta R.T.: 0.000 min
Response: 28333865
Conc: 20.00 ng/ml

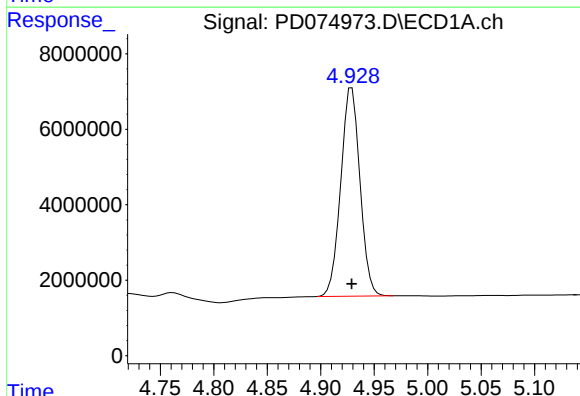


#4 Heptachlor

R.T.: 4.929 min
Delta R.T.: 0.000 min
Response: 69217220
Conc: 20.00 ng/ml

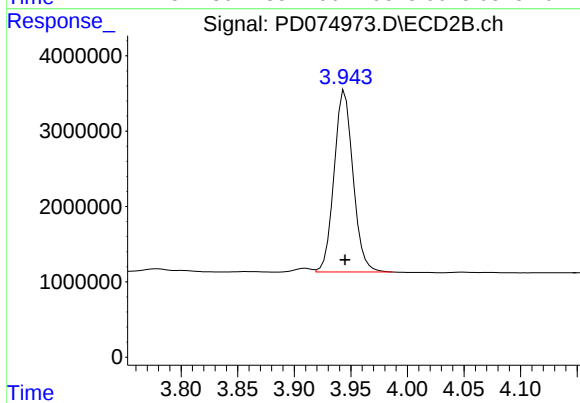

#4 Heptachlor


R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 28046289
Conc: 20.00 ng/ml

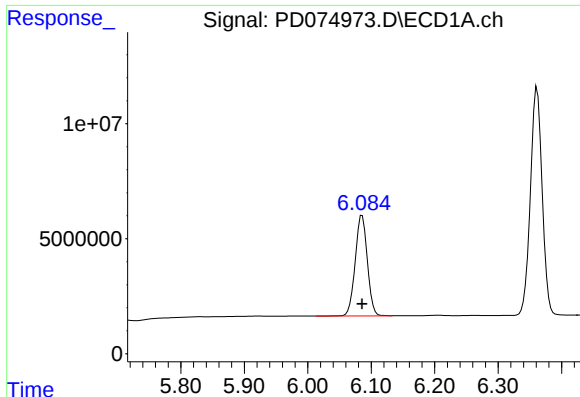

#9 Endosulfan I


R.T.: 6.086 min
Delta R.T.: 0.000 min
Response: 58217291
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

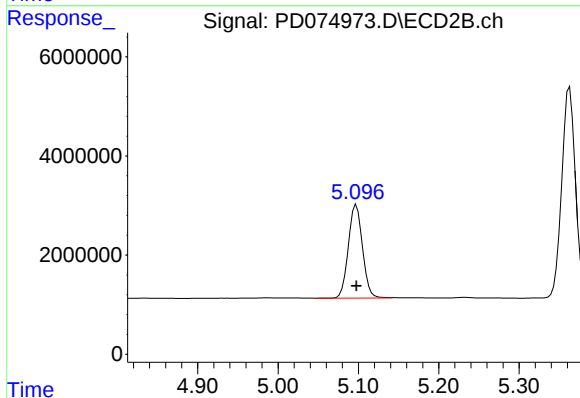


#9 Endosulfan I

R.T.: 5.097 min
Delta R.T.: 0.000 min
Response: 23059084
Conc: 20.00 ng/ml

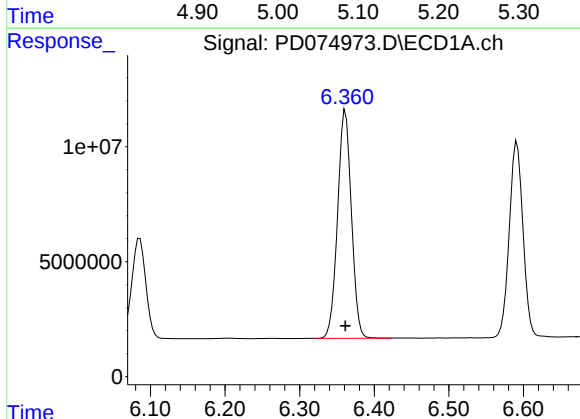


#13 Dieldrin

R.T.: 6.361 min
Delta R.T.: 0.000 min
Response: 127874532
Conc: 40.00 ng/ml

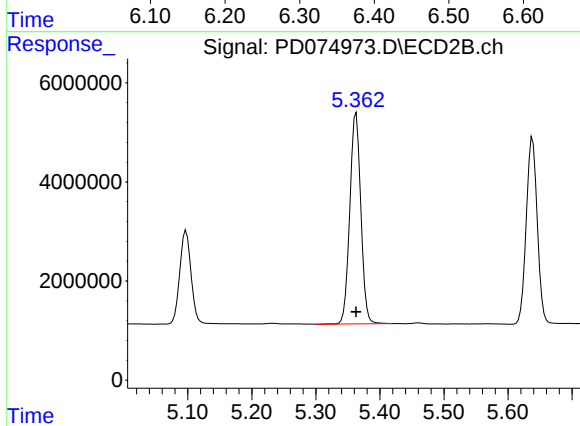

#13 Dieldrin


R.T.: 5.363 min
Delta R.T.: 0.000 min
Response: 50765306
Conc: 40.00 ng/ml

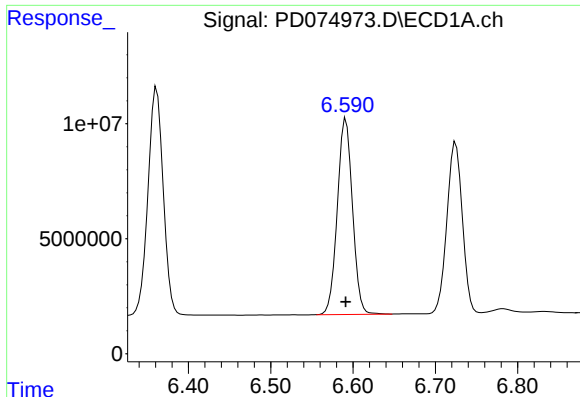

#14 Endrin


R.T.: 6.591 min
Delta R.T.: 0.000 min
Response: 108966228
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

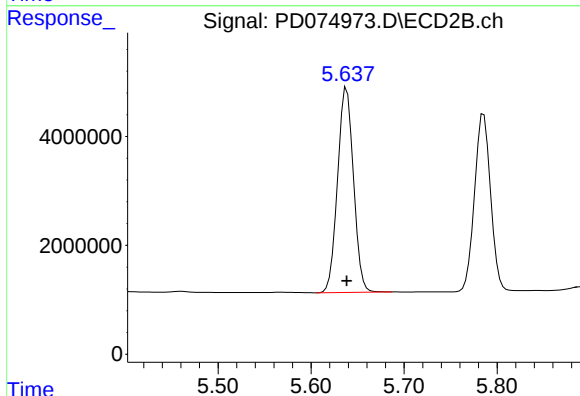


#14 Endrin

R.T.: 5.638 min
Delta R.T.: 0.000 min
Response: 44837147
Conc: 40.00 ng/ml

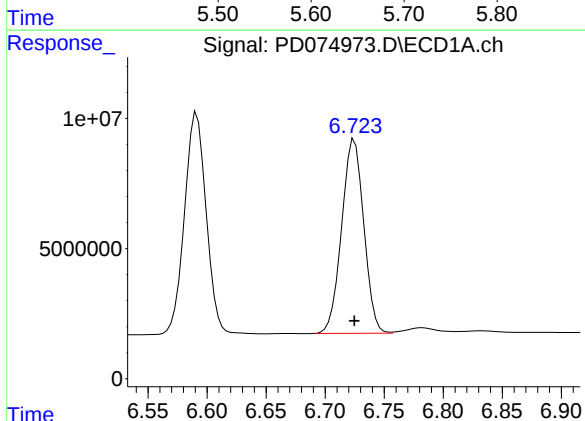


#16 4,4'-DDD

R.T.: 6.725 min
Delta R.T.: 0.000 min
Response: 97254741
Conc: 40.00 ng/ml

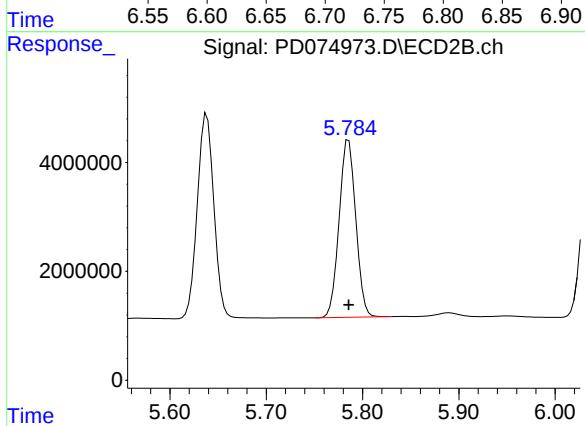

#16 4,4'-DDD


R.T.: 5.786 min
Delta R.T.: 0.000 min
Response: 39175838
Conc: 40.00 ng/ml

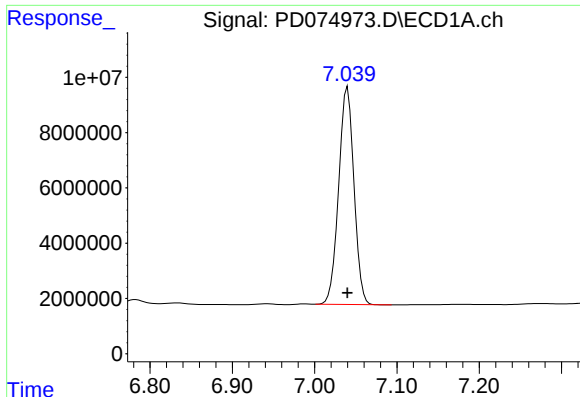

#17 4,4'-DDT


R.T.: 7.040 min
Delta R.T.: 0.000 min
Response: 101539875
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

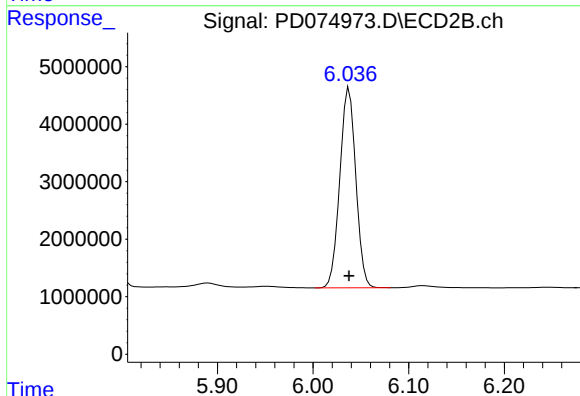


#17 4,4'-DDT

R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 40505703
Conc: 40.00 ng/ml

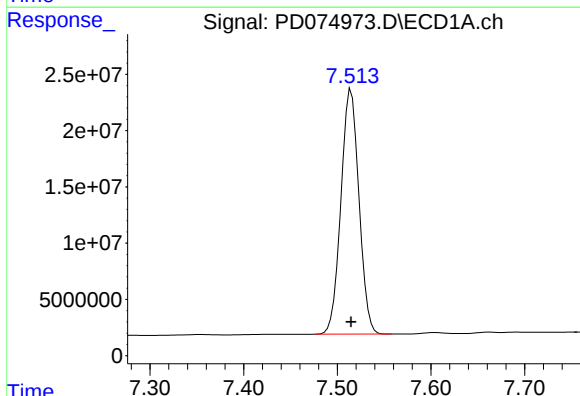


#20 Methoxychlor

R.T.: 7.515 min
Delta R.T.: 0.000 min
Response: 291484681
Conc: 200.00 ng/ml

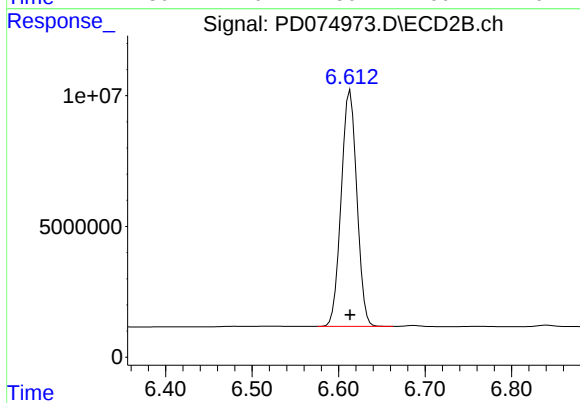

#20 Methoxychlor


R.T.: 6.613 min
Delta R.T.: 0.000 min
Response: 112763996
Conc: 200.00 ng/ml

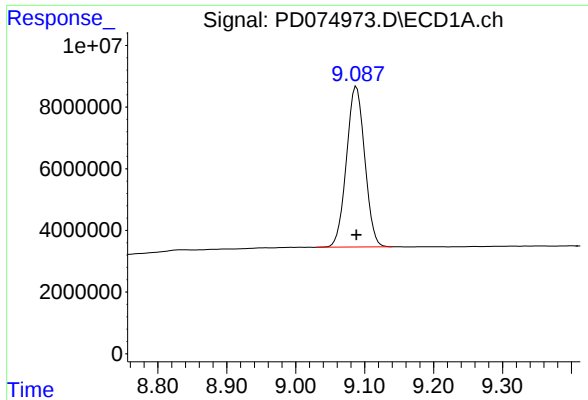

#27 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: 0.000 min
Response: 95910748
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

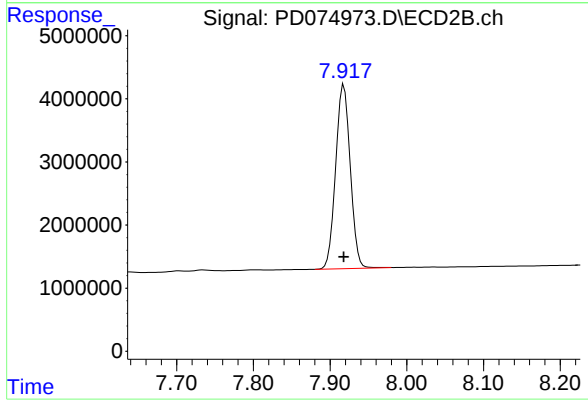

#27 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: 0.000 min
Response: 38643101
Conc: 40.00 ng/ml