

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042723\
 Data File : PD074977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2023 17:15
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5068

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 01:59:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 01:55:57 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.548	2.770	176.9E6	80847166	79.494	78.010
2) SA Decachlor...	9.089	7.919	362.0E6	138.3E6	155.360	151.113
Target Compounds						
2) A alpha-BHC	4.005	3.274	316.8E6	122.1E6	82.946	81.695
3) MA gamma-BHC...	4.338	3.604	291.6E6	115.2E6	82.382	80.653
4) MA Heptachlor	4.930	3.945	290.4E6	110.2E6	81.903	79.296
9) A Endosulfan I	6.087	5.098	232.7E6	89405994	79.972	78.753
13) MA Dieldrin	6.362	5.363	537.1E6	204.4E6	163.908	160.510
14) MA Endrin	6.593	5.639	451.8E6	177.2E6	162.867	159.055
16) A 4,4'-DDD	6.725	5.786	406.0E6	158.0E6	163.411	160.647
17) MA 4,4'-DDT	7.041	6.038	431.7E6	166.3E6	164.873	162.085
20) A Methoxychlor	7.516	6.614	1137.3E6	401.4E6	790.070	753.440

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042723\
Data File : PD074977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2023 17:15
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 01:59:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 01:55:57 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

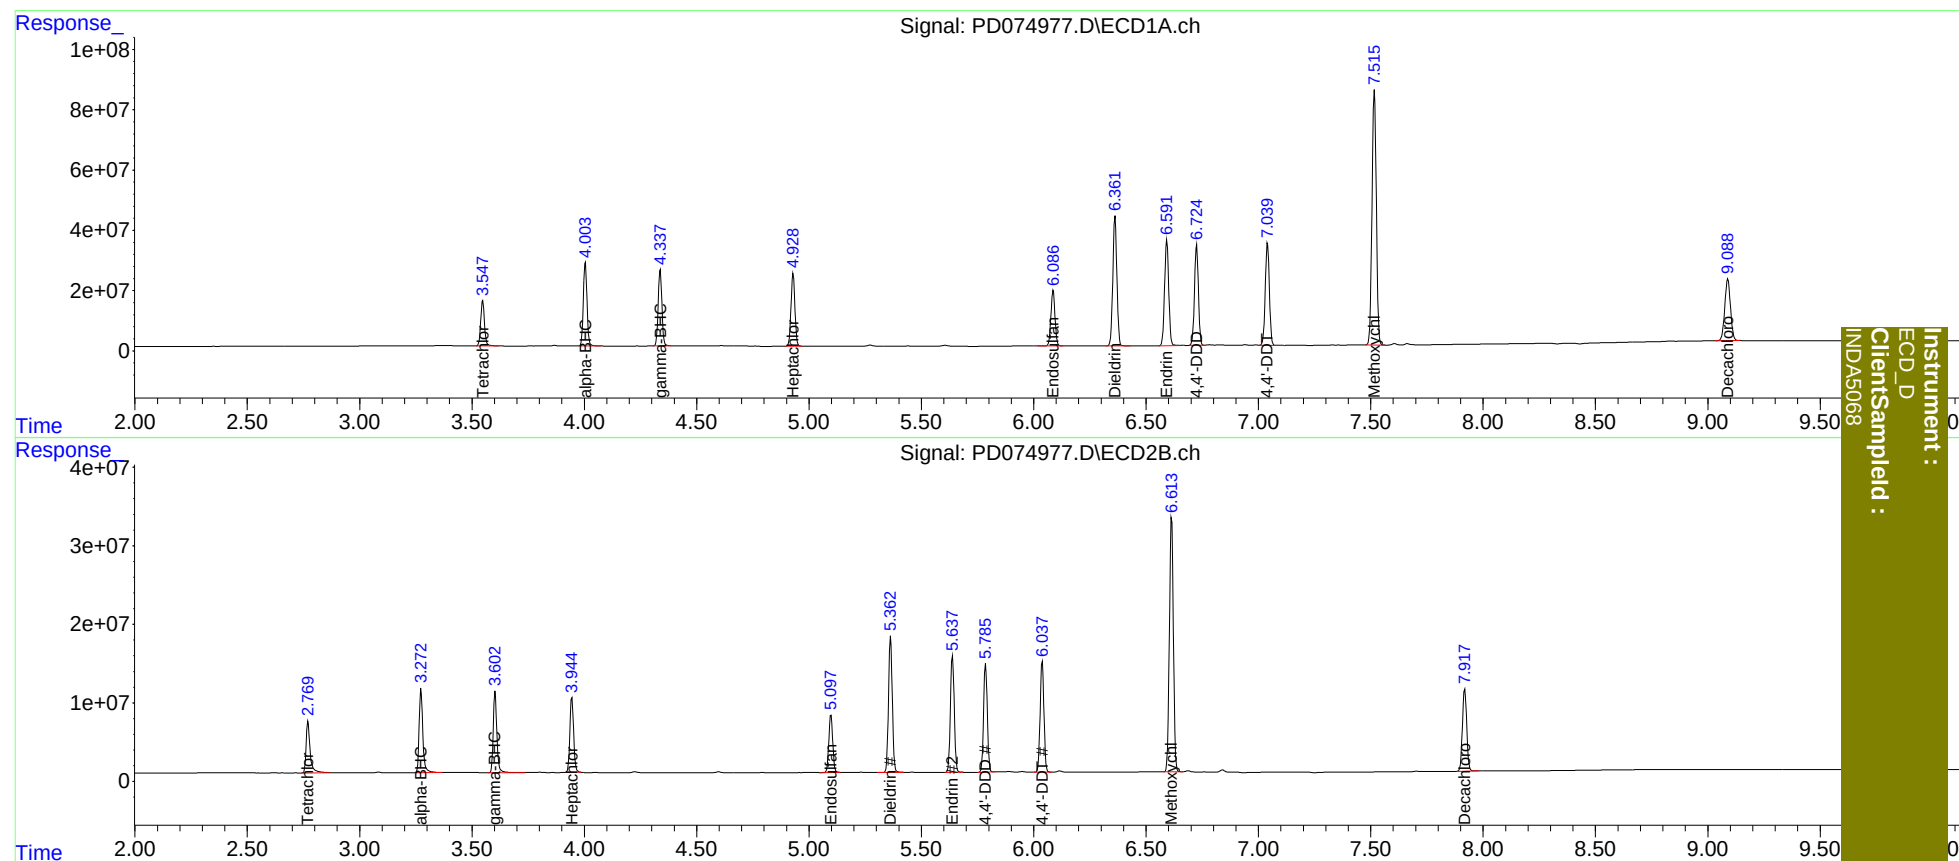

Instrument :
ECD_D
ClientSampled :
INDA5068