

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD042723\  
 Data File : PD075017.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 28 Apr 2023 09:19  
 Operator : AR\AJ  
 Sample : 02374-04MSD  
 Misc :  
 ALS Vial : 53 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 CB9D6MSD

Manual Integrations  
 APPROVED

Reviewed By :Abdul Mirza 05/02/2023  
 Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 28 22:53:26 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD042723CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Apr 28 02:34:46 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


| Compound                    | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|-------|-------|----------|----------|---------|---------|
| -----                       |       |       |          |          |         |         |
| System Monitoring Compounds |       |       |          |          |         |         |
| 1) SA Tetrachlo...          | 3.548 | 2.771 | 31978173 | 13461329 | 14.316  | 12.985  |
| 27) SA Decachlor...         | 9.086 | 7.917 | 41034222 | 20224498 | 17.181m | 21.054  |
| Target Compounds            |       |       |          |          |         |         |
| 2) A alpha-BHC              | 4.003 | 3.273 | 163.7E6  | 61435636 | 44.596m | 42.665  |
| 3) MA gamma-BHC...          | 4.336 | 3.602 | 149.5E6  | 61137544 | 43.713m | 43.936m |
| 4) MA Heptachlor            | 4.930 | 3.944 | 149.9E6  | 57187384 | 43.260  | 41.002  |
| 5) MB Aldrin                | 5.273 | 4.225 | 152.9E6  | 62314514 | 45.660  | 47.388  |
| 6) B beta-BHC               | 4.534 | 3.899 | 55004643 | 25244709 | 37.316  | 37.095  |
| 7) B delta-BHC              | 4.782 | 4.129 | 114.3E6  | 46634972 | 38.175  | 33.152  |
| 8) B Heptachlo...           | 5.699 | 4.727 | 135.8E6  | 48844728 | 45.221  | 39.783  |
| 9) A Endosulfan I           | 6.087 | 5.098 | 113.5E6  | 36377964 | 38.994  | 31.883  |
| 10) B trans-Chl...          | 5.955 | 4.978 | 146.3E6  | 55401323 | 48.881m | 45.732  |
| 11) B cis-Chlor...          | 6.036 | 5.042 | 140.9E6  | 53324292 | 45.192  | 43.067  |
| 12) B 4,4'-DDE              | 6.207 | 5.231 | 230.8E6  | 97149283 | 78.575m | 85.884  |
| 13) MA Dieldrin             | 6.363 | 5.363 | 282.7E6  | 116.4E6  | 88.956  | 92.705  |
| 14) MA Endrin               | 6.593 | 5.638 | 243.1E6  | 96121914 | 89.741  | 86.970  |
| 15) B Endosulfa...          | 6.811 | 5.930 | 230.1E6  | 90600379 | 79.442m | 83.055m |
| 16) A 4,4'-DDD              | 6.724 | 5.786 | 218.4E6  | 75328917 | 90.324m | 77.966  |
| 17) MA 4,4'-DDT             | 7.041 | 6.038 | 226.0E6  | 80844919 | 89.927  | 81.497  |
| 18) B Endrin al...          | 6.942 | 6.112 | 169.7E6  | 58209427 | 75.814  | 65.542  |
| 19) B Endosulfa...          | 7.175 | 6.334 | 204.2E6  | 75429722 | 78.339m | 73.362  |
| 20) A Methoxychlor          | 7.517 | 6.614 | 602.7E6  | 220.2E6  | 418.057 | 398.634 |
| 21) B Endrin ke...          | 7.663 | 6.841 | 246.5E6  | 84971695 | 85.215  | 71.261  |
| -----                       |       |       |          |          |         |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD042723\  
Data File : PD075017.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 28 Apr 2023 09:19  
Operator : AR\AJ  
Sample : 02374-04MSD  
Misc :  
ALS Vial : 53 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 28 22:53:26 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD042723CLP.M  
Quant Title : GC Extractables  
QLast Update : Fri Apr 28 02:34:46 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

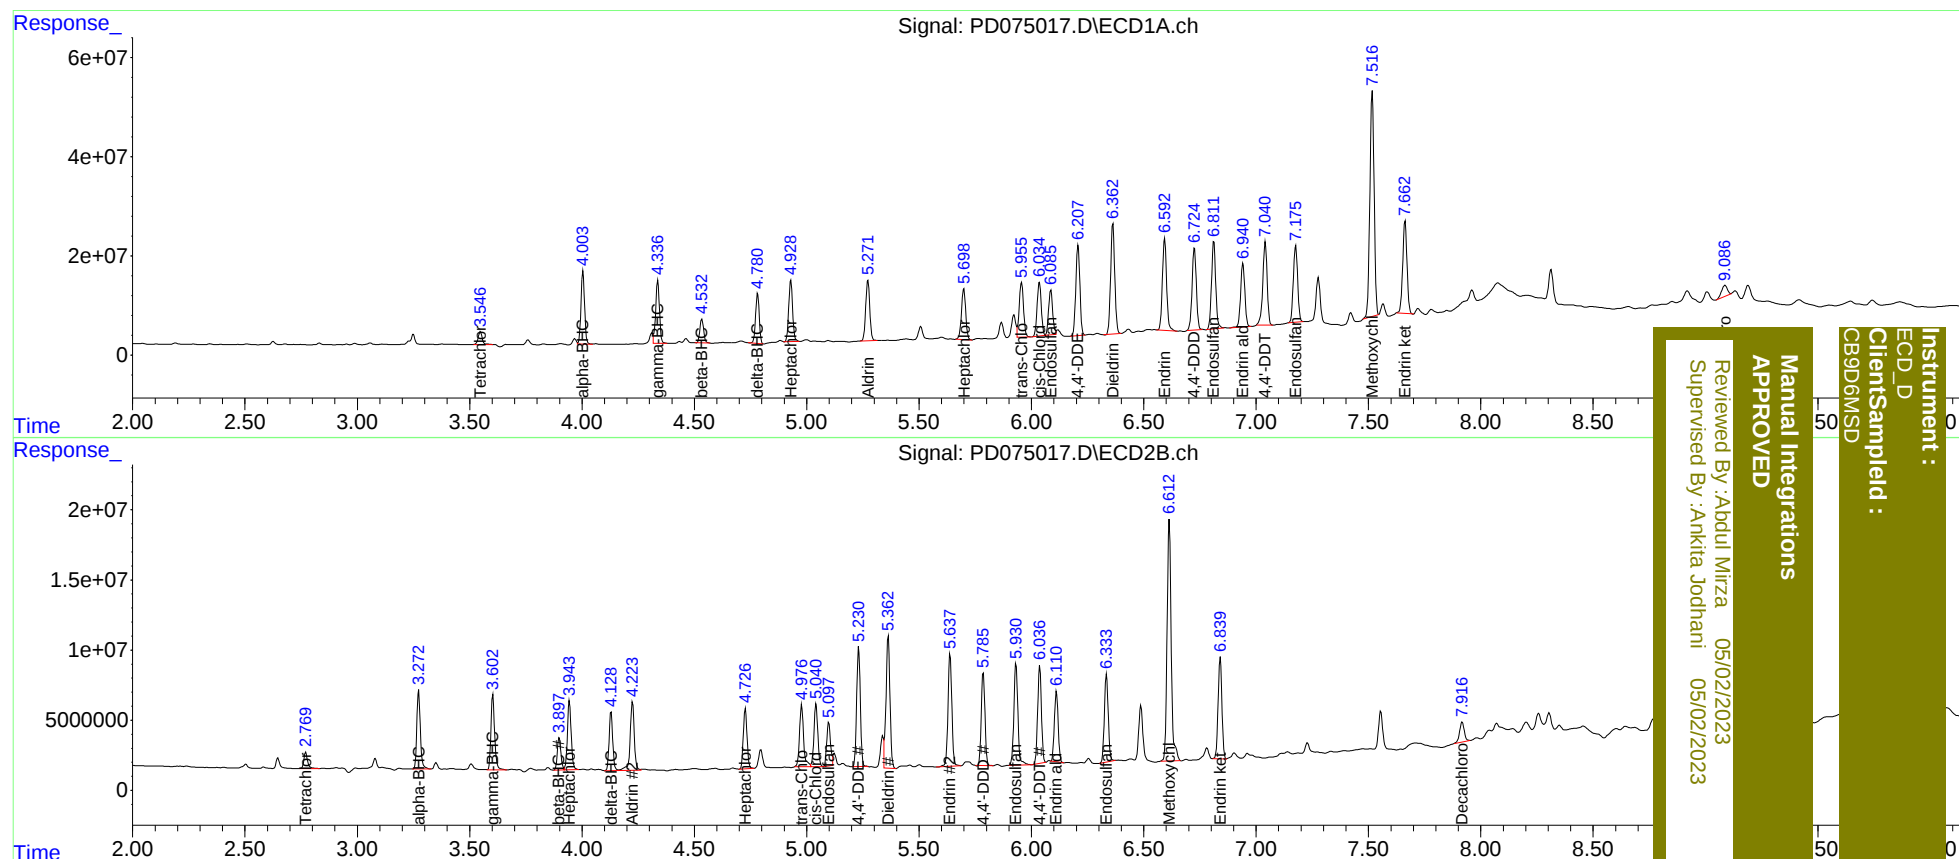

Instrument :  
ECD\_D  
Client Sampled :  
CB9D6MSD

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2023  
Supervised By :Ankita Jodhani 05/02/2023