

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD042723\  
 Data File : PD074988.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Apr 2023 21:54  
 Operator : AR\AJ  
 Sample : PB152373BS  
 Misc :  
 ALS Vial : 27 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 PLCS373

Manual Integrations  
 APPROVED

Reviewed By : Abdul Mirza 04/28/2023  
 Supervised By : Ankita Jodhani 05/01/2023

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 28 03:12:23 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD042723CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Apr 28 02:34:46 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


| Compound                    | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-------|-------|----------|----------|--------|--------|
| -----                       |       |       |          |          |        |        |
| System Monitoring Compounds |       |       |          |          |        |        |
| 1) SA Tetrachlo...          | 3.547 | 2.770 | 47051615 | 20921949 | 21.064 | 20.182 |
| 27) SA Decachlor...         | 9.086 | 7.917 | 97246788 | 39084343 | 40.716 | 40.687 |
| Target Compounds            |       |       |          |          |        |        |
| 2) A alpha-BHC              | 4.003 | 3.273 | 16449272 | 6204877  | 4.482  | 4.309  |
| 3) MA gamma-BHC...          | 4.337 | 3.603 | 15523974 | 6026551  | 4.540  | 4.331  |
| 4) MA Heptachlor            | 4.928 | 3.944 | 17001445 | 6427972  | 4.908  | 4.609  |
| 5) MB Aldrin                | 5.271 | 4.224 | 16838324 | 6552093  | 5.028  | 4.983  |
| 6) B beta-BHC               | 4.532 | 3.899 | 8085405  | 3173536  | 5.485  | 4.663  |
| 7) B delta-BHC              | 4.780 | 4.129 | 13533044 | 5371846  | 4.521  | 3.819  |
| 8) B Heptachlo...           | 5.698 | 4.726 | 16080477 | 5951657  | 5.354  | 4.847  |
| 9) A Endosulfan I           | 6.085 | 5.097 | 13929949 | 5425530  | 4.784  | 4.755  |
| 10) B trans-Chl...          | 5.955 | 4.977 | 14574635 | 5955688  | 4.869  | 4.916  |
| 11) B cis-Chlor...          | 6.034 | 5.041 | 15154467 | 6118953  | 4.862  | 4.942  |
| 12) B 4,4'-DDE              | 6.206 | 5.231 | 27363784 | 10745209 | 9.316  | 9.499  |
| 13) MA Dieldrin             | 6.359 | 5.360 | 30350792 | 11980390 | 9.549m | 9.544m |
| 14) MA Endrin               | 6.590 | 5.637 | 26355158 | 10793710 | 9.728  | 9.766  |
| 15) B Endosulfa...          | 6.809 | 5.931 | 28281205 | 10787470 | 9.764  | 9.889  |
| 16) A 4,4'-DDD              | 6.723 | 5.785 | 22867861 | 9171218  | 9.457  | 9.492  |
| 17) MA 4,4'-DDT             | 7.037 | 6.037 | 23923258 | 9115342  | 9.521m | 9.189  |
| 18) B Endrin al...          | 6.938 | 6.111 | 18921458 | 7887347  | 8.454m | 8.881  |
| 19) B Endosulfa...          | 7.174 | 6.333 | 24054154 | 10094379 | 9.226  | 9.818  |
| 20) A Methoxychlor          | 7.514 | 6.612 | 71351185 | 28888094 | 49.492 | 52.299 |
| 21) B Endrin ke...          | 7.660 | 6.840 | 28229356 | 12003952 | 9.757  | 10.067 |
| -----                       |       |       |          |          |        |        |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD042723\  
Data File : PD074988.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 27 Apr 2023 21:54  
Operator : AR\AJ  
Sample : PB152373BS  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 28 03:12:23 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD042723CLP.M  
Quant Title : GC Extractables  
QLast Update : Fri Apr 28 02:34:46 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

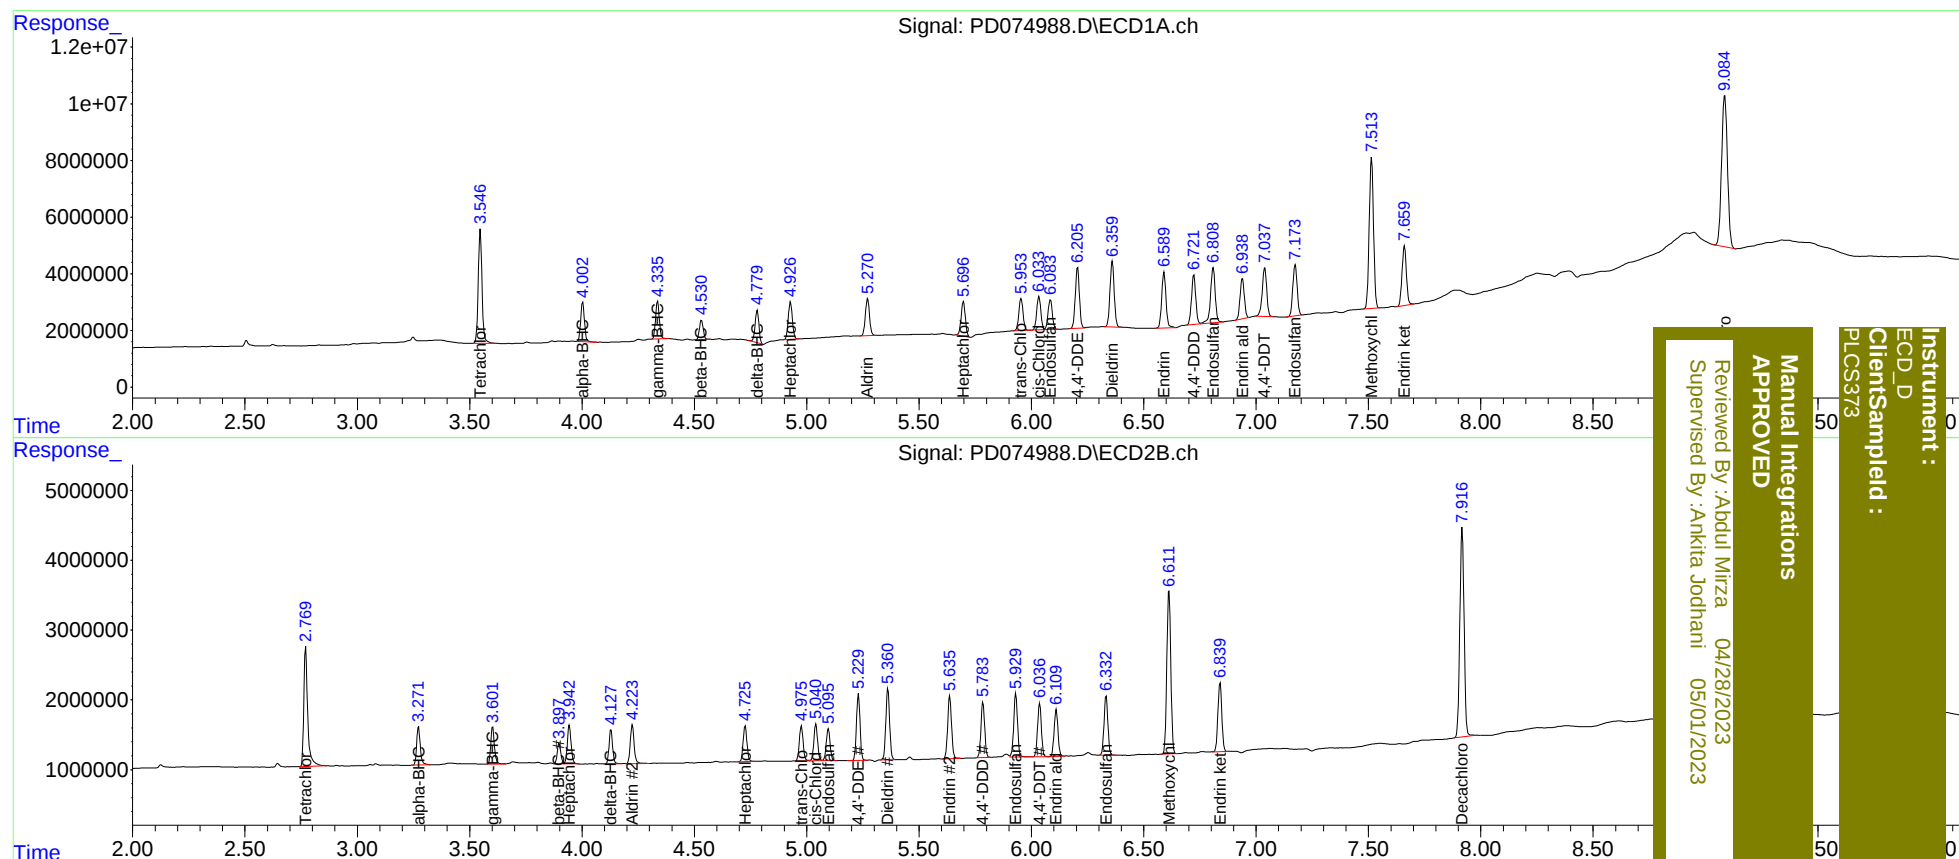

Manual Integrations  
APPROVED  
Reviewed By: Abdul Mirza 04/28/2023  
Supervised By: Ankita Jodhani 05/01/2023

Instrument :  
ECD\_D  
Client Sampled :  
PLCS373