

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042723\
 Data File : PD075017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2023 09:19
 Operator : AR\AJ
 Sample : 02374-04MSD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB9D6MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/02/2023
 Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 22:53:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 28 02:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.548	2.771	31978173	13461329	14.316	12.985
27) SA Decachlor...	9.086	7.917	41034222	20224498	17.181m	21.054
Target Compounds						
2) A alpha-BHC	4.003	3.273	163.7E6	61435636	44.596m	42.665
3) MA gamma-BHC...	4.336	3.602	149.5E6	61137544	43.713m	43.936m
4) MA Heptachlor	4.930	3.944	149.9E6	57187384	43.260	41.002
5) MB Aldrin	5.273	4.225	152.9E6	62314514	45.660	47.388
6) B beta-BHC	4.534	3.899	55004643	25244709	37.316	37.095
7) B delta-BHC	4.782	4.129	114.3E6	46634972	38.175	33.152
8) B Heptachlo...	5.699	4.727	135.8E6	48844728	45.221	39.783
9) A Endosulfan I	6.087	5.098	113.5E6	36377964	38.994	31.883
10) B trans-Chl...	5.955	4.978	146.3E6	55401323	48.881m	45.732
11) B cis-Chlor...	6.036	5.042	140.9E6	53324292	45.192	43.067
12) B 4,4'-DDE	6.207	5.231	230.8E6	97149283	78.575m	85.884
13) MA Dieldrin	6.363	5.363	282.7E6	116.4E6	88.956	92.705
14) MA Endrin	6.593	5.638	243.1E6	96121914	89.741	86.970
15) B Endosulfa...	6.811	5.930	230.1E6	90600379	79.442m	83.055m
16) A 4,4'-DDD	6.724	5.786	218.4E6	75328917	90.324m	77.966
17) MA 4,4'-DDT	7.041	6.038	226.0E6	80844919	89.927	81.497
18) B Endrin al...	6.942	6.112	169.7E6	58209427	75.814	65.542
19) B Endosulfa...	7.175	6.334	204.2E6	75429722	78.339m	73.362
20) A Methoxychlor	7.517	6.614	602.7E6	220.2E6	418.057	398.634
21) B Endrin ke...	7.663	6.841	246.5E6	84971695	85.215	71.261

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042723\
Data File : PD075017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2023 09:19
Operator : AR\AJ
Sample : 02374-04MSD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 22:53:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042723CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 28 02:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

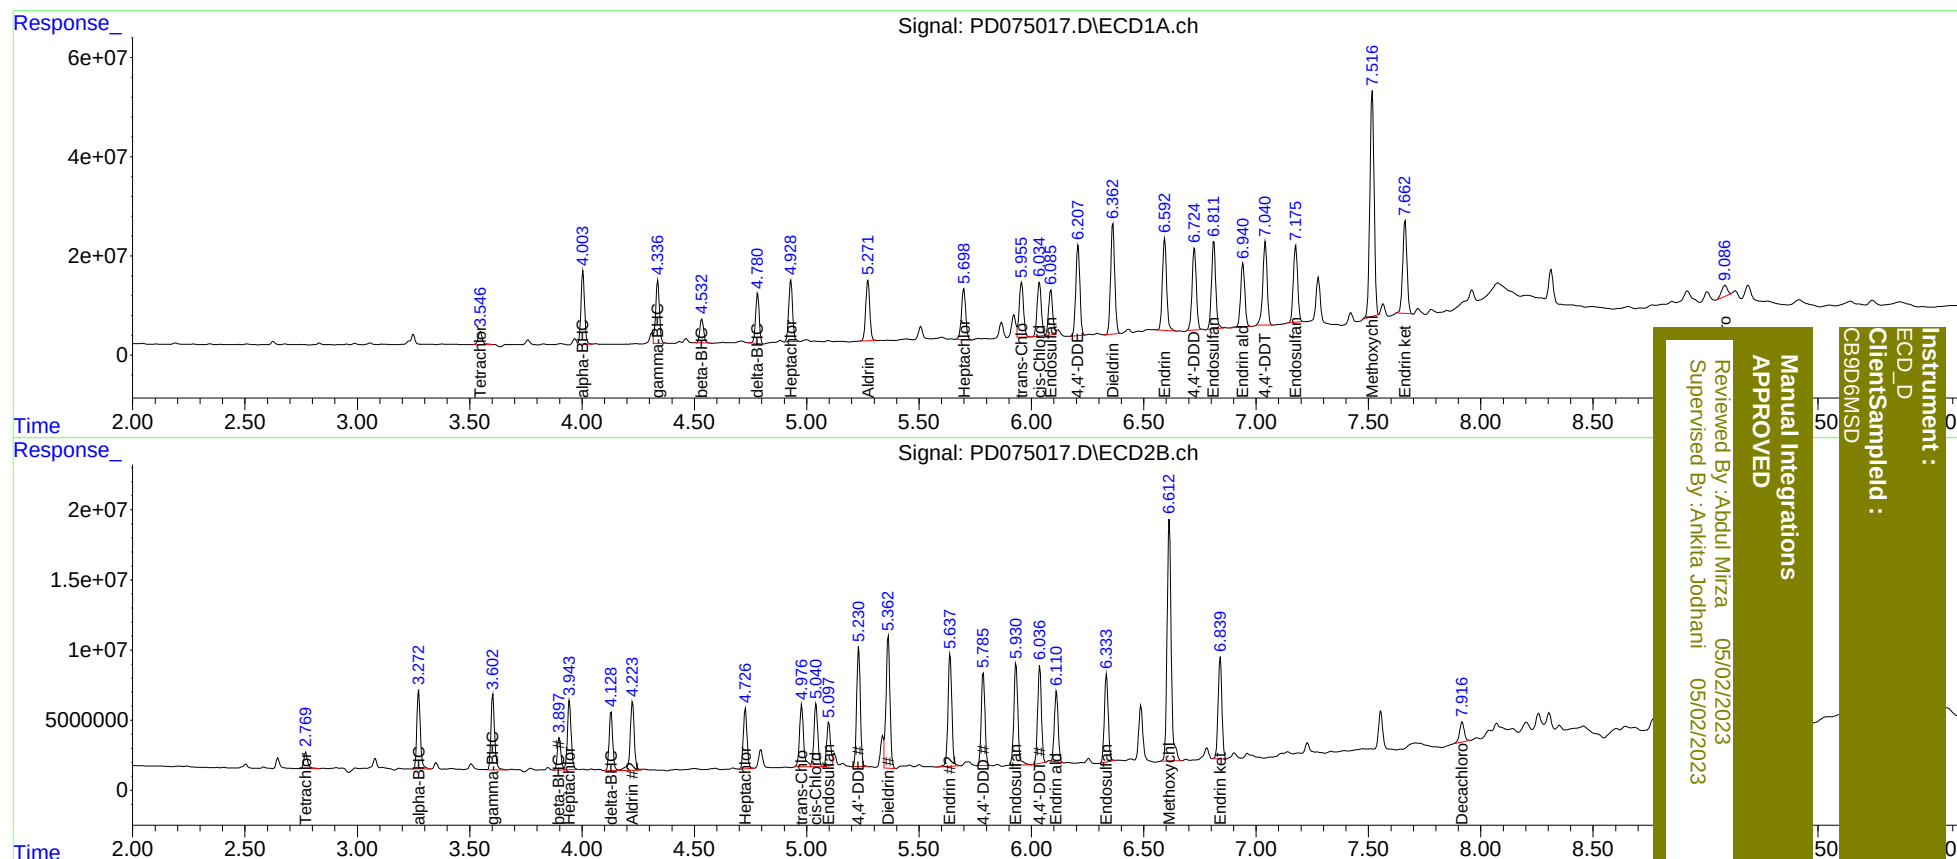

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/02/2023
Supervised By: Ankita Jodhani 05/02/2023

Instrument :
ECD_D
Client Sampled :
CB9D6MSD