

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042724\
 Data File : PD082637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2024 23:27
 Operator : AR\AJ
 Sample : P2203-22MSD
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1CX4MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/29/2024
 Supervised By : mohammad ahmed 05/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 06:31:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042424CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 24 16:11:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.775	29311079	67847692	20.728	19.387
27)	SA Decachlor...	9.116	7.905	32553897	63825720	16.707	16.913
Target Compounds							
2)	A alpha-BHC	4.020	3.275	117.4E6	271.5E6	49.188m	48.364
3)	MA gamma-BHC...	4.354	3.604	124.1E6	263.6E6	53.065m	47.645
4)	MA Heptachlor	4.946	3.943	119.3E6	308.2E6	50.878m	59.786
5)	MB Aldrin	5.292	4.221	117.6E6	266.1E6	51.877	51.313m
6)	B beta-BHC	4.551	3.900	38880929	106.9E6	37.055m	46.974 #
7)	B delta-BHC	4.799	4.130	64179933	161.9E6	27.250m	29.557
8)	B Heptachlo...	5.718	4.724	116.5E6	240.1E6	54.442	49.478
9)	A Endosulfan I	6.106	5.094	96634578	174.8E6	47.639	40.489
10)	B trans-Chl...	5.974	4.973	105.8E6	244.1E6	50.696m	51.695
11)	B cis-Chlor...	6.055	5.037	103.5E6	249.0E6	48.457	51.525
12)	B 4,4'-DDE	6.226	5.226	171.7E6	432.6E6	81.479	94.462
13)	MA Dieldrin	6.382	5.357	203.9E6	467.7E6	94.987	96.963
14)	MA Endrin	6.612	5.632	173.5E6	400.3E6	94.935	94.584
15)	B Endosulfa...	6.831	5.925	161.4E6	389.3E6	86.388	95.871
16)	A 4,4'-DDD	6.745	5.779	146.9E6	343.1E6	96.200	96.370
17)	MA 4,4'-DDT	7.060	6.029	146.7E6	343.4E6	91.169	91.359
18)	B Endrin al...	6.961	6.104	122.4E6	278.3E6	83.997	84.584
19)	B Endosulfa...	7.197	6.327	139.5E6	327.2E6	82.354	85.174
20)	A Methoxychlor	7.537	6.604	371.3E6	820.7E6	436.683	435.331
21)	B Endrin ke...	7.684	6.832	169.5E6	364.1E6	93.645	84.930

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042724\
Data File : PD082637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2024 23:27
Operator : AR\AJ
Sample : P2203-22MSD
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 06:31:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042424CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 24 16:11:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

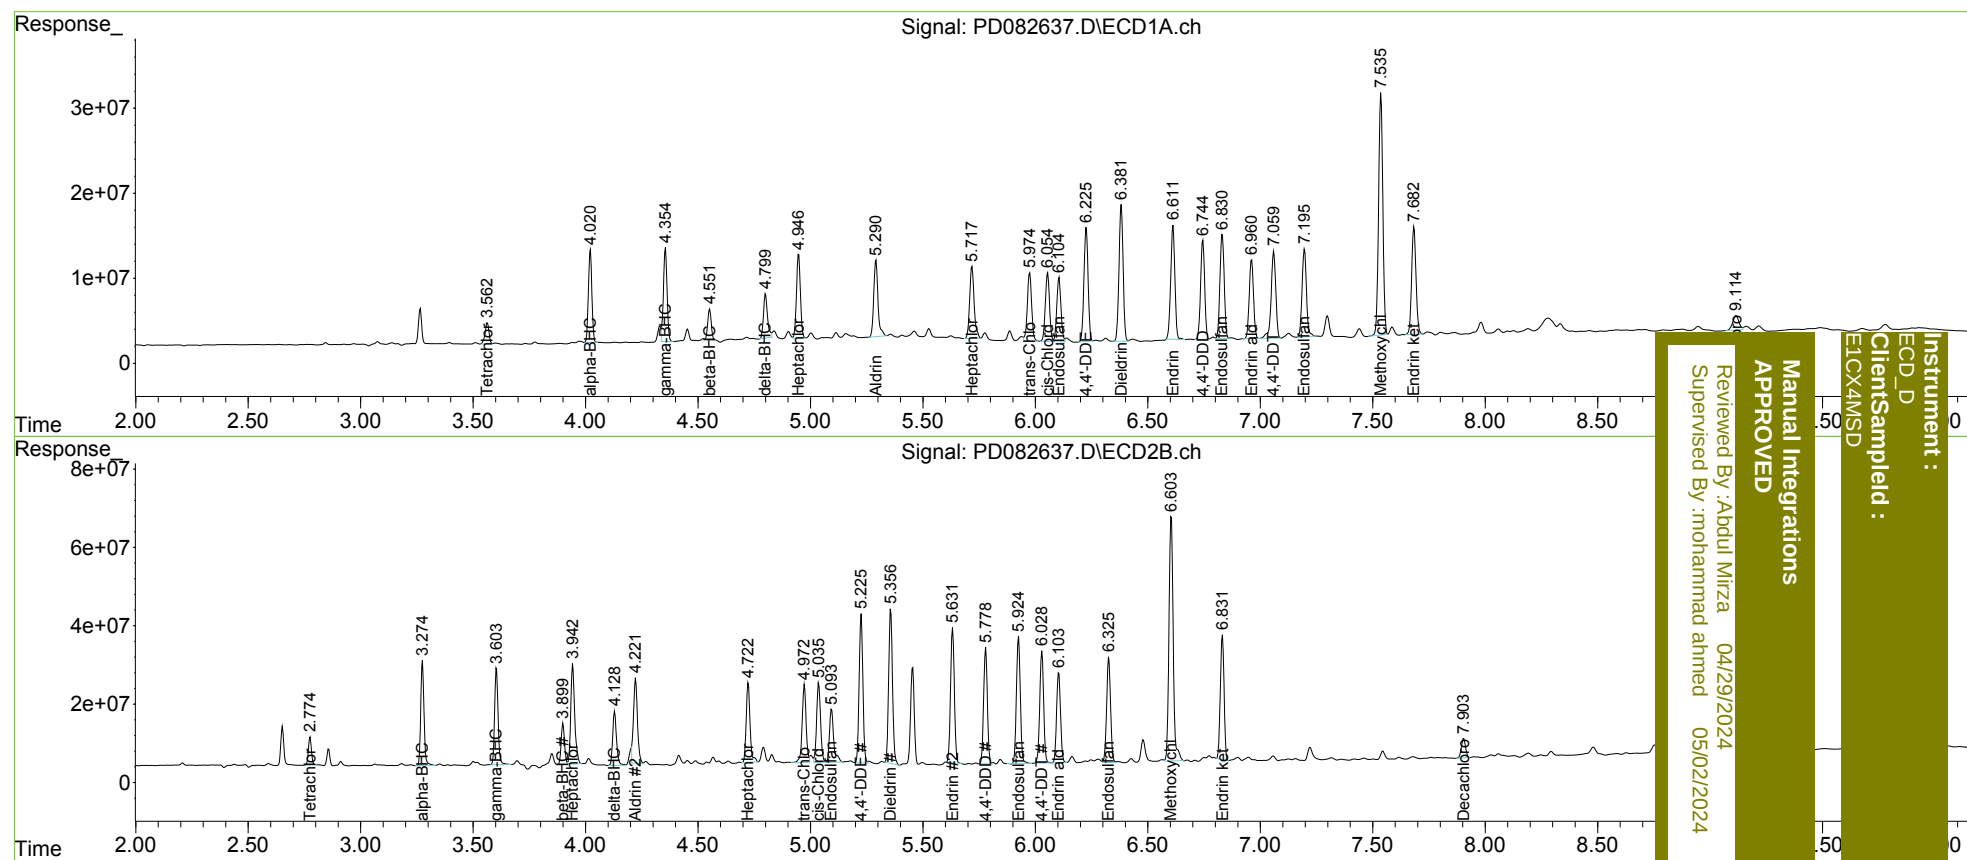

Instrument :
ECD_D
Client Sampled :
E10X4MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 04/29/2024
Supervised By: mohammad ahmed 05/02/2024