

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042724\
 Data File : PD082632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2024 22:21
 Operator : AR\AJ
 Sample : P2203-17
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1CW9

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/29/2024
 Supervised By :mohammad ahmed 05/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 03:35:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042424CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 24 16:11:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.564	2.776	22127458	56122798	15.648	16.037
27) SA Decachlor...	9.114	7.905	23076380	50355009	11.843m	13.343
Target Compounds						
5) MB Aldrin	5.317	4.238	7249100	16196616	3.197m	3.123
7) B delta-BHC	4.819	4.137	7680795	18196651	3.261m	3.322m
11) B cis-Chlor...	6.042	5.046	5430250	12033691	2.542	2.490m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042724\
Data File : PD082632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2024 22:21
Operator : AR\AJ
Sample : P2203-17
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 03:35:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042424CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 24 16:11:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

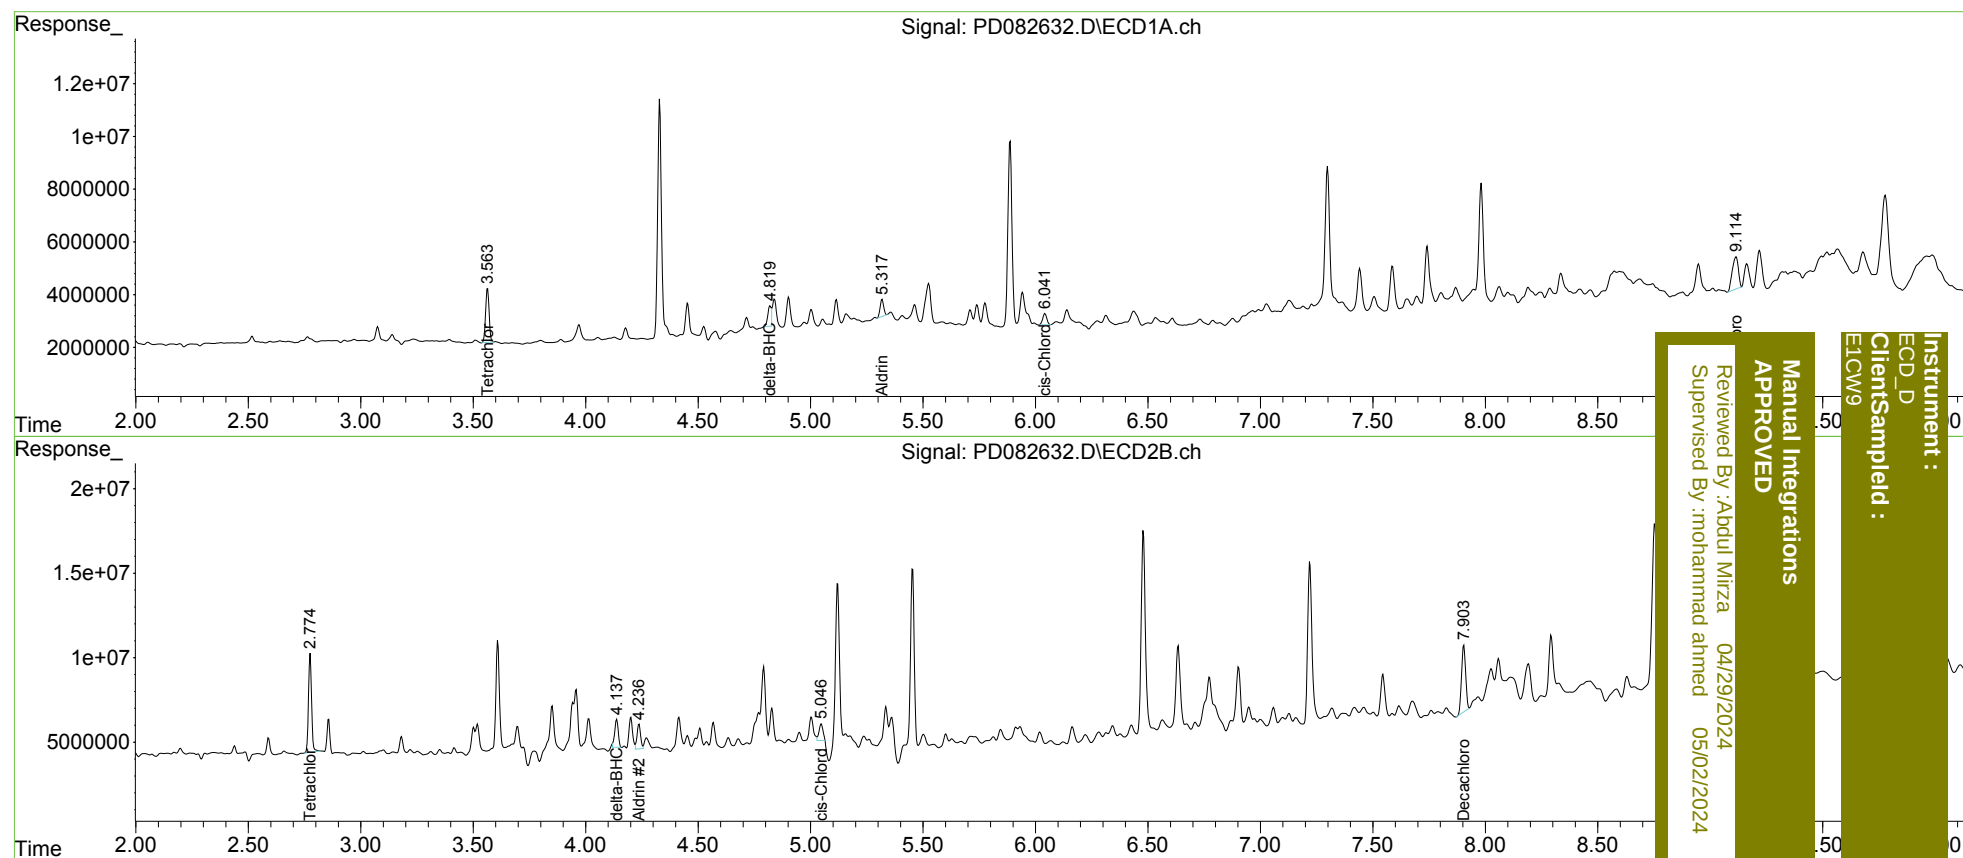

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 04/29/2024
Supervised By: mohammad ahmed 05/02/2024

Instrument :
ECD_D
ClientSampled :
EICW9