

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042724\
 Data File : PD082633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2024 22:34
 Operator : AR\AJ
 Sample : P2203-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1CX0

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/29/2024
 Supervised By :mohammad ahmed 05/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 03:49:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042424CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 24 16:11:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.775	18228702	45465675	12.891	12.992
27)	SA Decachlor...	9.116	7.905	27792661	44009264	14.264	11.662
Target Compounds							
5)	MB Aldrin	5.316	4.238	6155882	15345611	2.715m	2.959
7)	B delta-BHC	4.818	4.139	7833818	17804556	3.326m	3.250
11)	B cis-Chlor...	6.042	5.047	1626521	7068629	0.762	1.463m#
17)	MA 4,4'-DDT	7.071	6.020	1671226	6522069	1.039	1.735 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042724\
Data File : PD082633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2024 22:34
Operator : AR\AJ
Sample : P2203-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 03:49:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042424CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 24 16:11:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

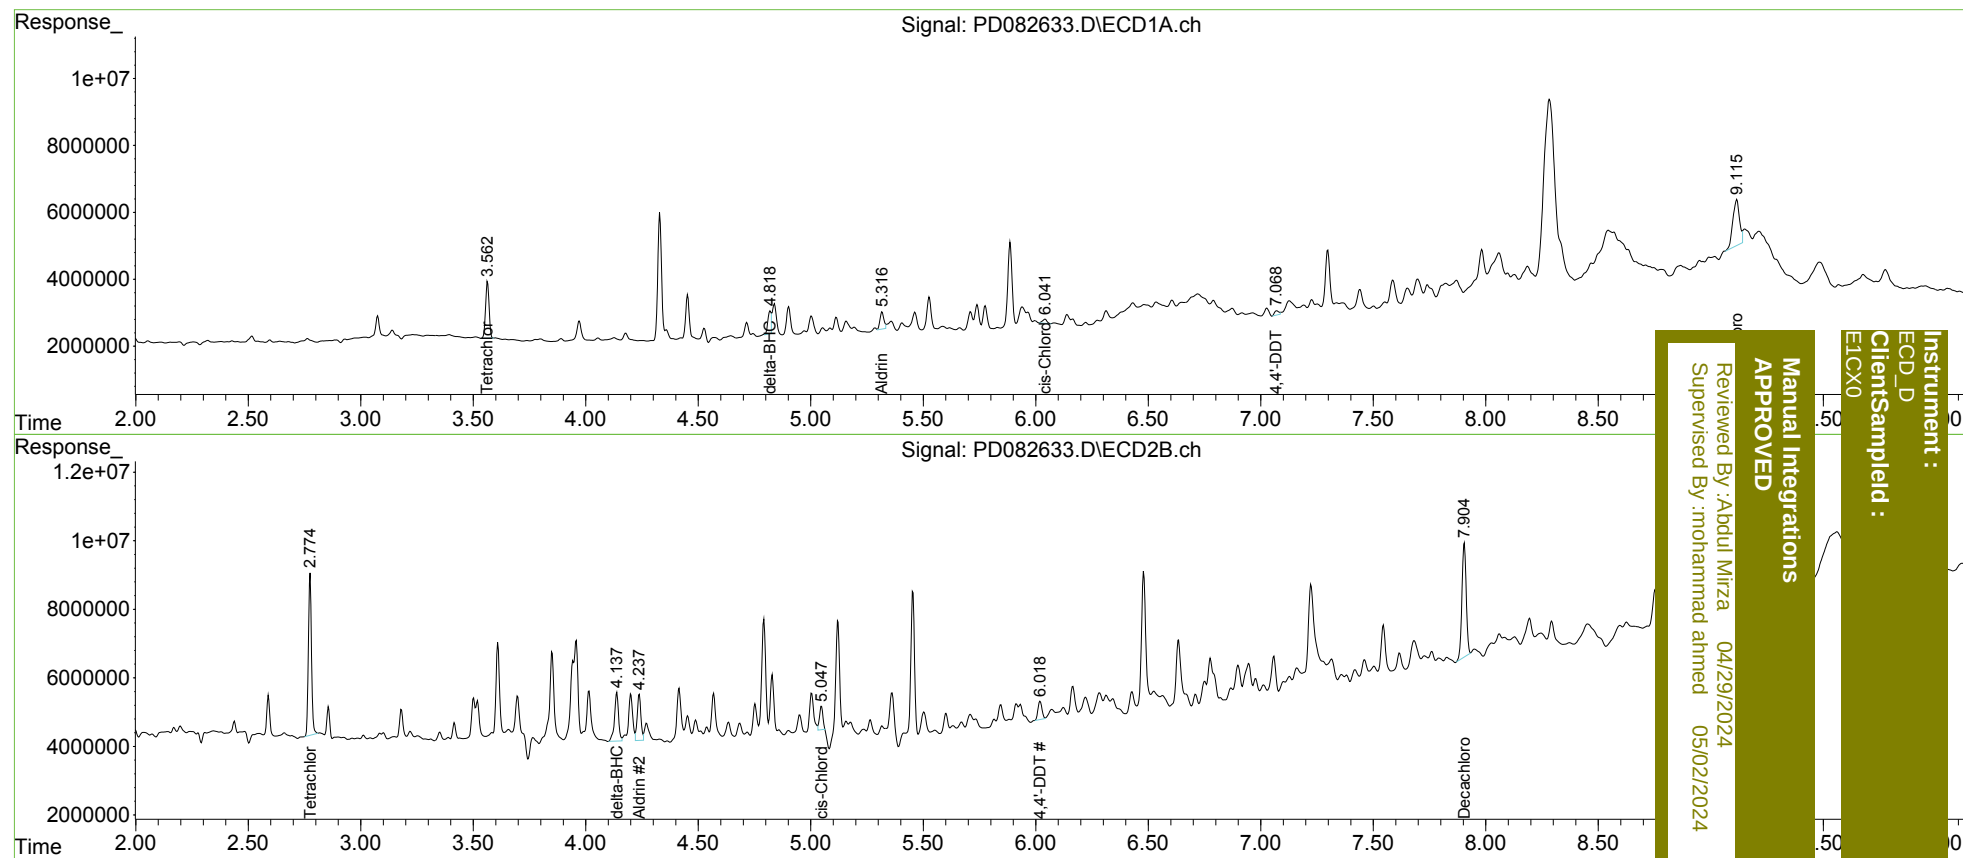

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 04/29/2024
Supervised By: mohammad ahmed 05/02/2024

Instrument :
ECD_D
ClientSampled :
E1CX0